


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100920\  
Data File : VU040585.D  
Acq On : 09 Oct 2020 15:43  
Operator : SY/MD  
Sample : L4349-11  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
Client Sampled :  
BG189

Manual Integrations  
APPROVED  
MMDadoda  
10/12/2020 11:50:56 AM

Quant Time: Oct 10 05:14:04 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Sat Oct 10 04:13:39 2020  
Response via : Initial Calibration

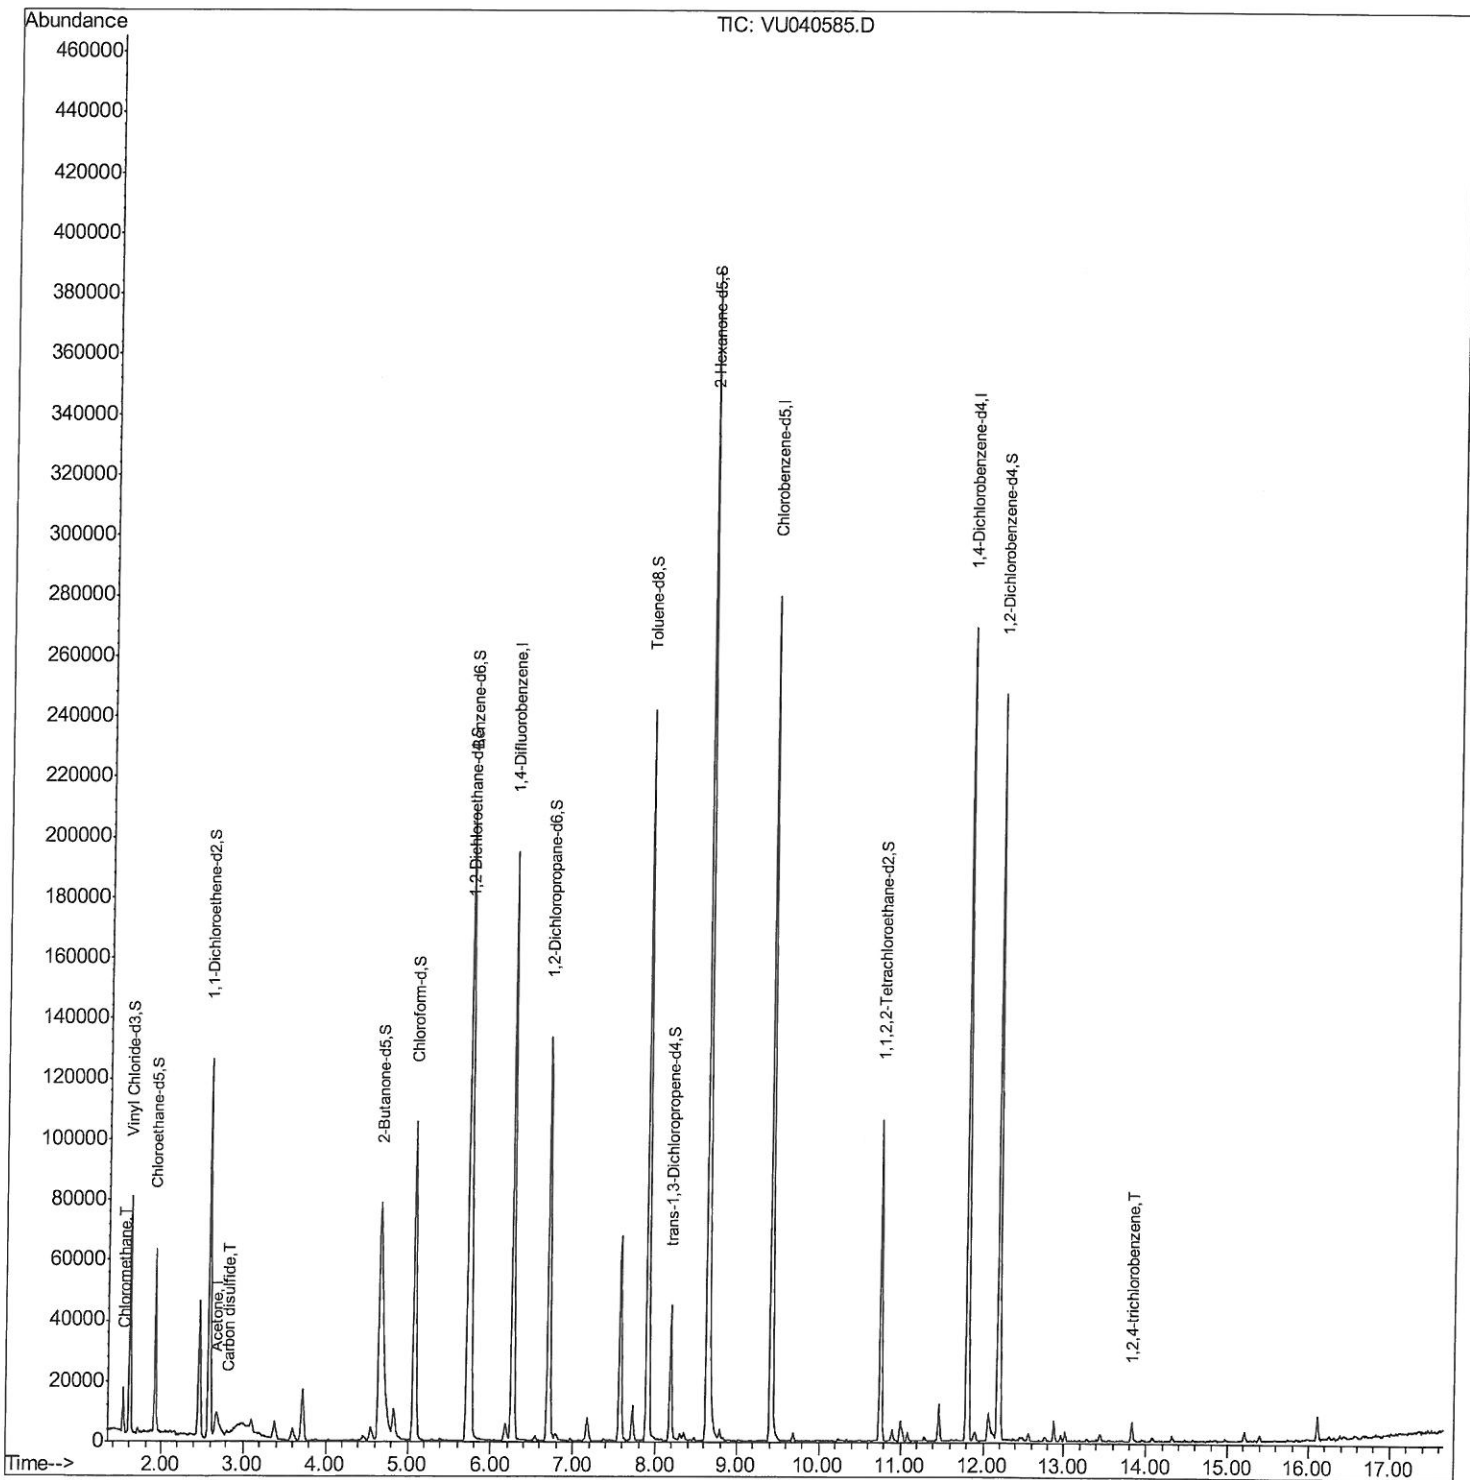




Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100920\  
 Data File : VU040585.D  
 Acq On : 09 Oct 2020 15:43  
 Operator : SY/MD  
 Sample : L4349-11  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_U  
**ClientSampled :**  
 BG189

**Manual Integrations**  
**APPROVED**  
 MMDadoda  
 10/12/2020 11:50:56 AM

Quant Time: Oct 10 04:21:49 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Sat Oct 10 04:13:39 2020  
 Response via : Initial Calibration

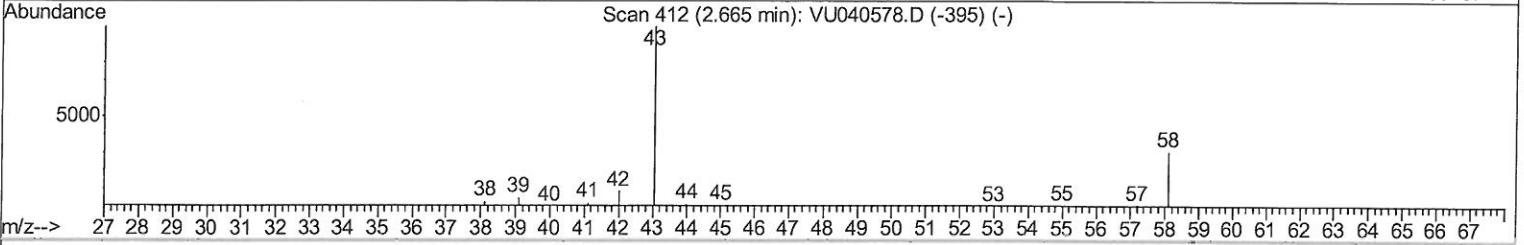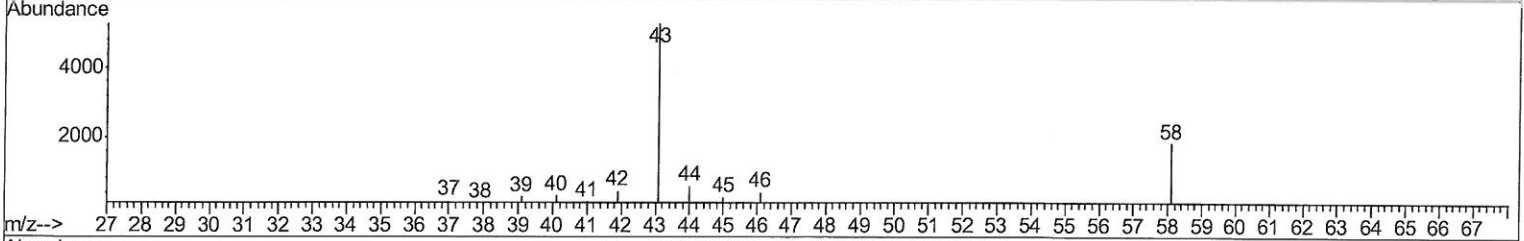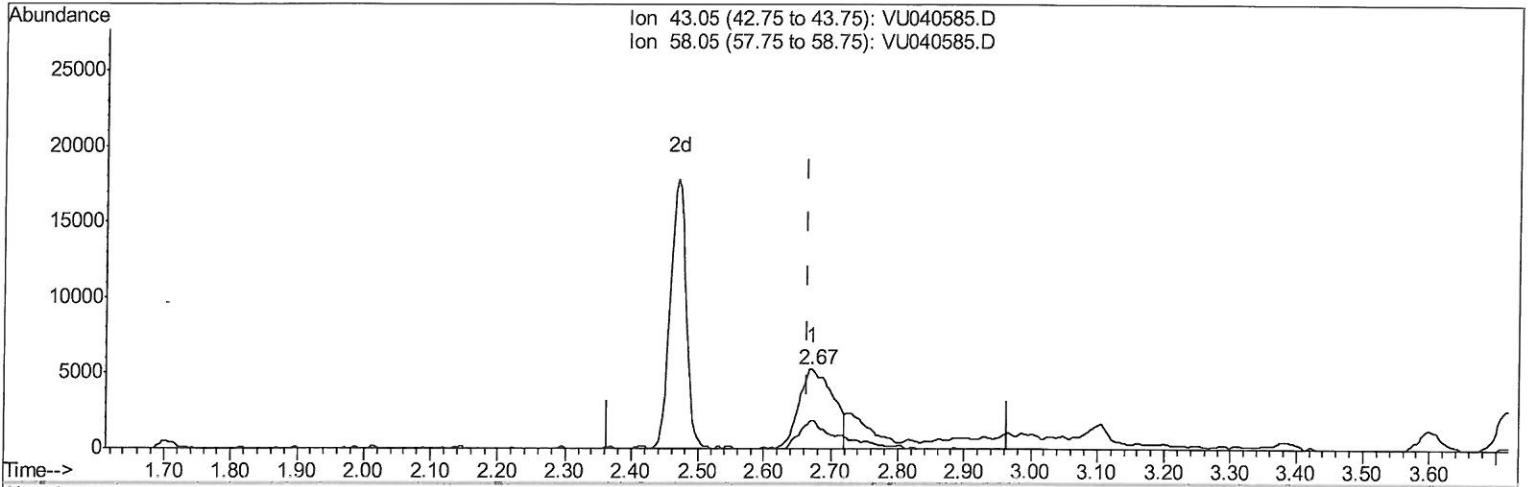

TIC: VU040585.D

(13) Acetone (T)  
 2.671min (+0.006) 6.06ug/L  
 response 18648

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	27.07
0.00	0.00	0.00
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100920\  
 Data File : VU040585.D  
 Acq On : 09 Oct 2020 15:43  
 Operator : SY/MD  
 Sample : L4349-11  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_U  
**ClientSampled :**  
 BG189

**Manual Integrations**  
**APPROVED**  
 MMDadoda  
 10/12/2020 11:50:56 AM

Quant Time: Oct 10 04:21:49 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Sat Oct 10 04:13:39 2020  
 Response via : Initial Calibration

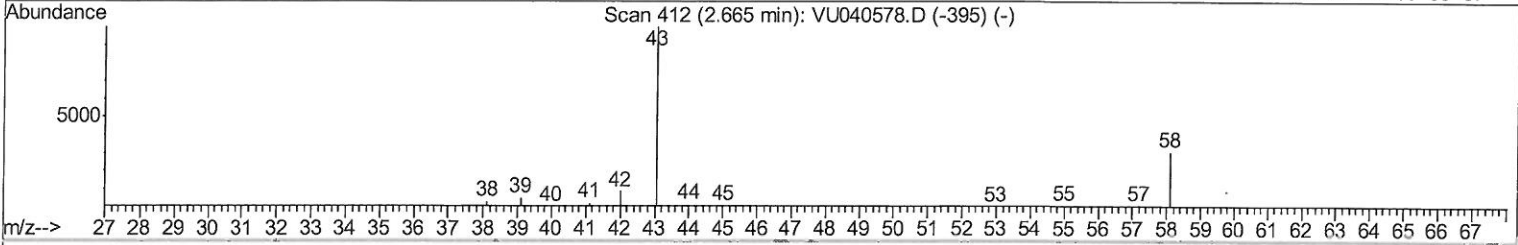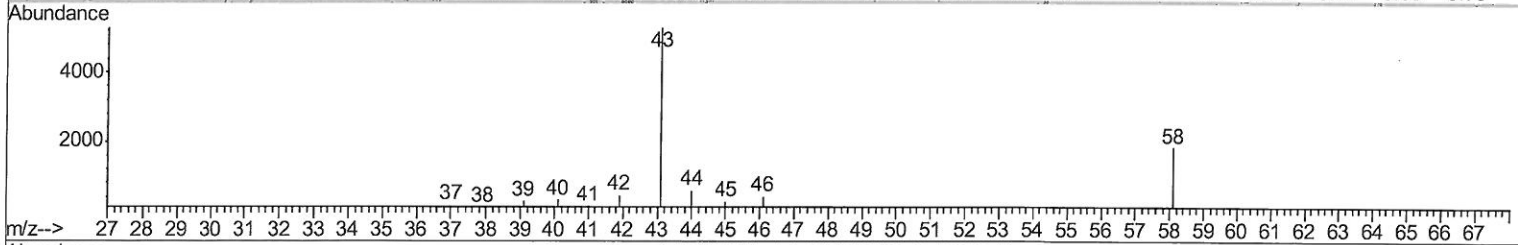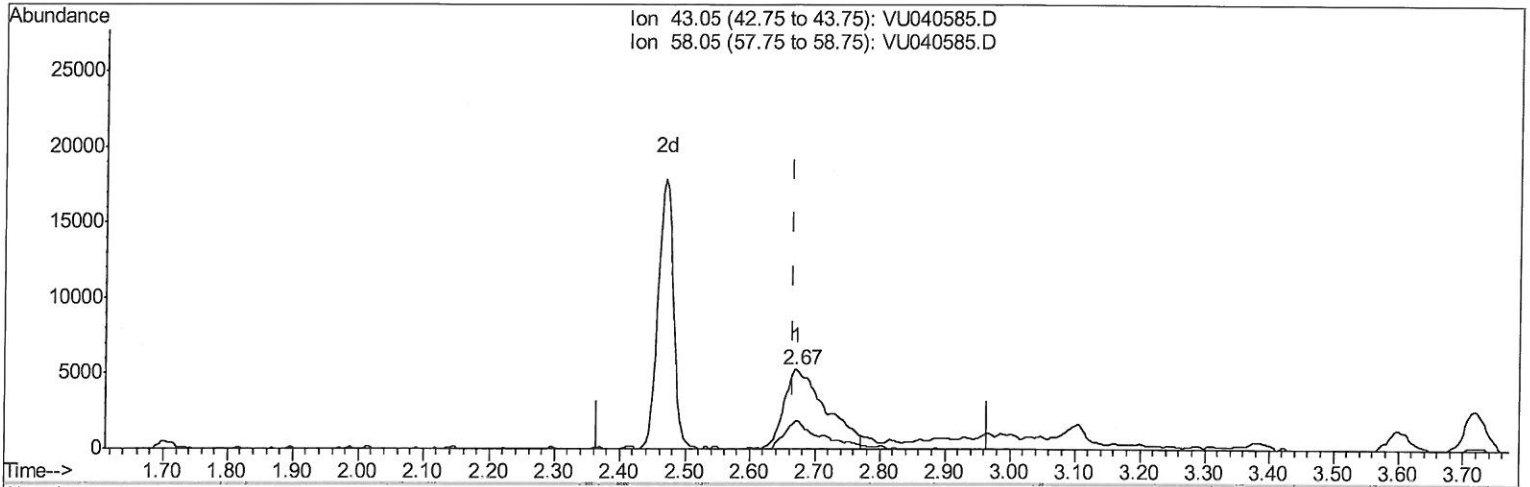

TIC: VU040585.D

(13) Acetone (T)

2.671min (+0.006) 7.75ug/L m

response 23856

*7 mg*  
*10/10/20*

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	21.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100920\  
 Data File : VU040585.D  
 Acq On : 09 Oct 2020 15:43  
 Operator : SY/MD  
 Sample : L4349-11  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 Client Sampled :  
 BG189

Manual Integrations  
 APPROVED

MMDadoda  
 10/12/2020 11:50:56 AM

Quant Time: Oct 10 05:14:04 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Sat Oct 10 04:13:39 2020  
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	149715	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	145255	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	65566	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	53829	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.93	69	41677	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.58	63	76637	3.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.20%
20) 2-Butanone-d5	4.66	46	190910	48.09	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.18%
24) Chloroform-d	5.08	84	94399	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	5.72	65	59268	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
32) Benzene-d6	5.75	84	178490	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
36) 1,2-Dichloropropane-d6	6.70	67	59301	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.91	98	149171	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.00%
43) trans-1,3-Dichloropropene-	8.19	79	23794	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
46) 2-Hexanone-d5	8.64	63	135945	47.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.76%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	50942	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	60825	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%

Target Compounds

					Ovalue
3) Chloromethane	1.53	50	9634	0.759 ug/L	96
13) Acetone	2.67	43	23856m	7.753 ug/L	88
14) Carbon disulfide	2.81	76	2298	0.077 ug/L #	88
68) 1,2,4-trichlorobenzene	13.83	180	1852	0.157 ug/L	98

MD  
 10/10/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed