


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100920\
 Data File : VU040577.D
 Acq On : 09 Oct 2020 10:15
 Operator : SY/MD
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Oct 12 07:06:57 2020

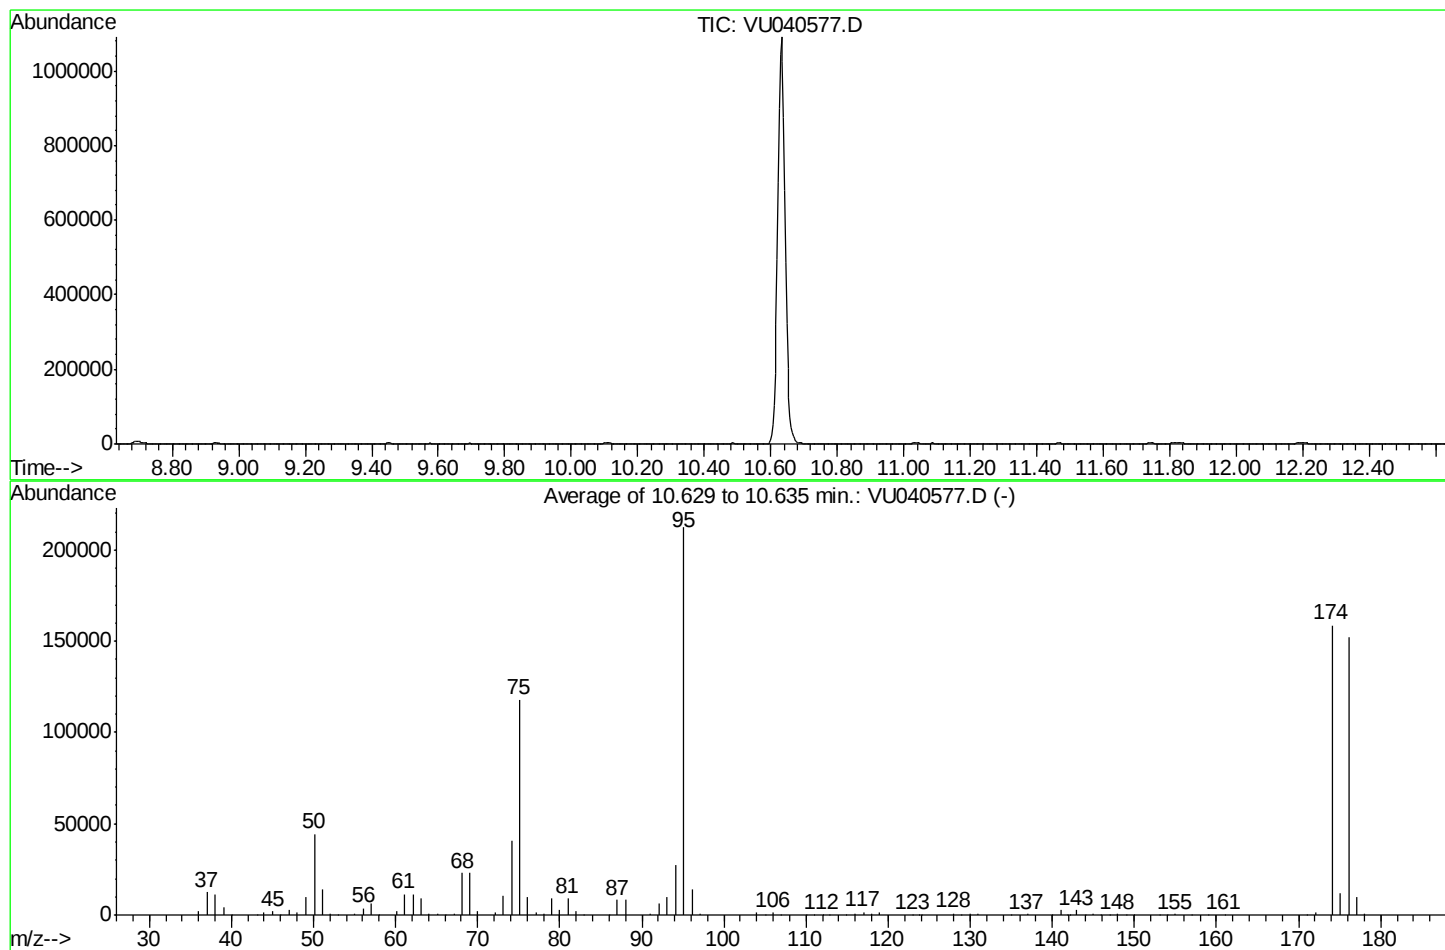

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	44213	PASS
75	95	30	80	55.6	118133	PASS
95	95	100	100	100.0	212437	PASS
96	95	5	9	6.7	14184	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.7	158720	PASS
175	174	5	9	7.5	11838	PASS
176	174	95	101	96.0	152298	PASS
177	176	5	9	6.3	9654	PASS

m/z	Abundance
36.00	2390.0
37.10	13001.0
38.00	11105.0
39.10	4508.0
40.00	447.0
43.20	132.0
44.00	1819.0
45.10	2057.0
46.10	203.0
47.00	2722.0
48.00	1762.0
49.00	9831.0
50.10	45808.0
51.10	13727.0
52.00	515.0
53.00	129.0
55.10	569.0
56.10	3772.0
57.10	6464.0
58.00	294.0
60.10	2115.0
61.00	11107.0
62.10	11603.0
63.10	8940.0
64.00	1215.0
65.10	1138.0
66.00	123.0
67.10	506.0
68.10	23000.0
69.10	23312.0
70.00	1893.0
72.10	1265.0
73.10	10768.0
74.10	40632.0
75.10	117624.0
76.10	10004.0
77.10	1329.0
78.00	916.0
79.00	9021.0
80.00	2417.0
81.00	9151.0
82.00	2065.0
82.90	220.0
86.00	322.0
87.00	7937.0
88.00	8248.0
91.00	1071.0
92.10	6529.0
93.10	9792.0
94.10	27144.0
95.10	211584.0
96.10	14126.0
97.00	482.0
104.00	1051.0
105.00	261.0
106.00	1082.0
106.90	198.0
110.00	190.0
111.00	259.0
112.00	200.0
112.90	334.0
114.90	215.0
116.00	824.0
117.00	1603.0
118.00	946.0
119.00	1199.0
123.00	102.0
124.00	171.0
128.00	868.0
129.00	308.0
130.00	763.0
131.00	352.0
135.00	372.0
136.90	421.0
140.00	138.0
141.00	2604.0
141.90	366.0
143.00	2690.0
144.00	174.0
145.00	527.0
146.00	346.0
147.00	128.0
148.00	547.0
149.00	145.0
150.00	233.0
153.00	155.0
154.00	144.0
155.00	538.0
157.00	296.0
159.00	238.0
160.90	128.0
171.00	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

172.10	1486.0
174.10	153856.0
175.10	11497.0
176.10	147840.0
177.10	8966.0
178.00	399.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	2296.0
37.10	13006.0
38.10	11336.0
39.10	4424.0
40.00	510.0
44.00	1941.0
45.00	2072.0
45.90	193.0
47.00	2825.0
48.00	1782.0
49.00	9905.0
50.10	45784.0
51.10	14371.0
52.00	566.0
53.00	122.0
55.00	589.0
56.10	3861.0
57.10	6843.0
58.00	271.0
60.10	2299.0
61.10	11745.0
62.10	11686.0
63.10	9451.0
64.10	1079.0
65.10	1042.0
66.00	134.0
67.10	594.0
68.10	23856.0
69.10	23616.0
70.00	1952.0
72.10	1280.0
73.10	11214.0
74.10	42480.0
75.10	122176.0
76.10	10320.0
77.10	1341.0
78.00	996.0
79.00	9285.0
80.00	2659.0
81.00	9380.0
82.00	2162.0
82.90	238.0
85.90	357.0
87.00	8695.0
88.00	8595.0
91.00	1086.0
92.10	6801.0
93.10	9987.0
94.10	28464.0
95.10	219712.0
96.10	14758.0
97.10	433.0
104.00	1198.0
105.00	295.0
106.00	1185.0
106.90	243.0
110.00	169.0
111.00	217.0
112.00	225.0
112.90	352.0
114.90	226.0
116.00	891.0
117.00	1739.0
118.00	970.0
119.00	1247.0
123.00	120.0
124.00	145.0
128.00	988.0
129.00	285.0
129.90	820.0
131.00	407.0
135.00	352.0
137.00	499.0
140.00	128.0
141.00	2612.0
141.90	315.0
143.00	2745.0
144.00	173.0
145.00	533.0
146.00	291.0
147.00	138.0
148.00	620.0
148.90	145.0
150.00	257.0
153.00	142.0
153.90	148.0
155.00	512.0
157.00	298.0
159.00	315.0
160.90	131.0
171.10	210.0
172.10	1366.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

174.10	164352.0
175.10	12232.0
176.10	157696.0
177.10	9989.0
178.00	429.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	2074.0
37.00	11861.0
38.10	10371.0
39.10	3903.0
40.00	491.0
44.00	1755.0
45.00	1928.0
45.90	237.0
47.00	2792.0
48.00	1577.0
49.00	9093.0
50.10	41048.0
51.10	13396.0
52.00	588.0
53.00	114.0
55.00	594.0
56.10	3630.0
57.10	6650.0
58.00	193.0
60.10	2336.0
61.10	11315.0
62.10	10704.0
63.10	8981.0
64.10	898.0
65.10	936.0
66.00	128.0
67.10	623.0
68.10	22048.0
69.10	21936.0
70.00	1837.0
72.10	1143.0
73.10	10338.0
74.10	39560.0
75.10	114600.0
76.10	9455.0
77.10	1193.0
78.00	986.0
79.00	8642.0
80.00	2609.0
81.00	8785.0
82.00	2032.0
82.90	200.0
85.90	345.0
87.00	8445.0
88.00	7874.0
91.00	962.0
92.10	6399.0
93.10	9085.0
94.10	26520.0
95.10	206016.0
96.10	13670.0
97.10	402.0
104.00	1162.0
105.00	338.0
106.00	1158.0
106.90	246.0
110.00	143.0
110.90	217.0
112.00	284.0
112.90	315.0
114.90	213.0
116.00	834.0
117.00	1678.0
118.00	901.0
119.00	1153.0
123.70	103.0
128.00	984.0
128.90	282.0
129.90	818.0
131.00	396.0
135.00	339.0
137.00	453.0
139.90	115.0
141.00	2495.0
142.10	283.0
143.00	2682.0
143.90	152.0
145.00	485.0
145.90	258.0
147.10	132.0
148.00	594.0
148.90	124.0
150.00	243.0
153.00	125.0
153.90	148.0
155.00	496.0
156.90	279.0
159.00	304.0
161.00	139.0
172.10	1290.0
174.10	157952.0
175.10	11785.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

176.10	151360.0
177.10	10008.0
178.00	338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Scan 2874 (10.581 min): VU040577.D
BFB16

m/z	Abundance
40.00	318.0
44.00	353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16