

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045268.D
 Acq On : 09 Oct 2021 17:25
 Operator : SY/MD
 Sample : VU1009WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	196730	212931	15.92%	2.148%
2	1.915	170	179	195	rVB	143207	194750	14.56%	1.965%
3	2.568	369	382	400	rBV	283199	470263	35.16%	4.745%
4	2.739	432	435	439	rVB2	264	177	0.01%	0.002%
5	2.764	439	443	445	rBV3	302	282	0.02%	0.003%
6	2.796	447	453	456	rBV2	1270	1254	0.09%	0.013%
7	3.054	524	533	541	rBV3	1609	2422	0.18%	0.024%
8	3.359	619	628	637	rBV4	539	685	0.05%	0.007%
9	3.475	659	664	666	rBV	180	196	0.01%	0.002%
10	3.565	688	692	694	rBV	224	173	0.01%	0.002%
11	3.607	702	705	708	rBV	187	135	0.01%	0.001%
12	3.777	752	758	763	rBV2	181	286	0.02%	0.003%
13	4.050	839	843	844	rBV	180	131	0.01%	0.001%
14	4.182	877	884	885	rBV	224	278	0.02%	0.003%
15	4.558	996	1001	1004	rVV2	136	150	0.01%	0.002%
16	4.626	1008	1022	1063	rBV	147565	356609	26.66%	3.598%
17	5.070	1143	1160	1181	rBV	235719	514563	38.47%	5.192%
18	5.253	1213	1217	1219	rBV2	229	175	0.01%	0.002%
19	5.298	1223	1231	1238	rVB5	804	1327	0.10%	0.013%
20	5.427	1267	1271	1273	rVB2	263	171	0.01%	0.002%
21	5.449	1273	1278	1280	rBV3	185	184	0.01%	0.002%
22	5.581	1315	1319	1324	rVB	315	288	0.02%	0.003%
23	5.623	1327	1332	1335	rBV	230	231	0.02%	0.002%
24	5.732	1343	1366	1392	rBV2	490525	1337619	100.00%	13.496%
25	5.976	1439	1442	1445	rBV2	392	254	0.02%	0.003%
26	6.079	1472	1474	1479	rBV2	256	184	0.01%	0.002%
27	6.253	1513	1528	1546	rBV	344429	645647	48.27%	6.514%
28	6.427	1579	1582	1585	rBV3	290	204	0.02%	0.002%
29	6.536	1607	1616	1624	rVB6	3681	6522	0.49%	0.066%
30	6.603	1632	1637	1641	rVB3	367	397	0.03%	0.004%
31	6.697	1651	1666	1691	rBV	313440	606295	45.33%	6.117%
32	6.893	1722	1727	1730	rBV3	390	419	0.03%	0.004%
33	7.012	1760	1764	1769	rBV2	127	151	0.01%	0.002%
34	7.050	1769	1776	1781	rBV2	532	808	0.06%	0.008%
35	7.182	1811	1817	1828	rVB3	718	1101	0.08%	0.011%
36	7.279	1842	1847	1849	rBV2	163	177	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045268.D
 Acq On : 09 Oct 2021 17:25
 Operator : SY/MD
 Sample : VU1009WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.320	1855	1860	1863	rBV2	187	224	0.02%	0.002%
38	7.404	1883	1886	1889	rBV	213	169	0.01%	0.002%
39	7.420	1889	1891	1894	rVB	214	133	0.01%	0.001%
40	7.443	1894	1898	1901	rBV2	178	178	0.01%	0.002%
41	7.513	1918	1920	1925	rBV2	166	130	0.01%	0.001%
42	7.571	1925	1938	1957	rBV	173195	305434	22.83%	3.082%
43	7.748	1989	1993	1997	rVB3	307	244	0.02%	0.002%
44	7.799	2000	2009	2018	rBV5	2353	3685	0.28%	0.037%
45	7.902	2027	2041	2056	rBV	607912	1037266	77.55%	10.466%
46	8.182	2116	2128	2147	rBV	120784	203913	15.24%	2.057%
47	8.401	2193	2196	2198	rVV2	220	146	0.01%	0.001%
48	8.635	2256	2269	2314	rBV	395208	751749	56.20%	7.585%
49	8.851	2334	2336	2337	rBV	227	123	0.01%	0.001%
50	8.934	2357	2362	2367	rBV3	515	655	0.05%	0.007%
51	8.983	2374	2377	2381	rBV2	170	181	0.01%	0.002%
52	9.008	2381	2385	2390	rBV	154	218	0.02%	0.002%
53	9.137	2421	2425	2428	rBV2	195	174	0.01%	0.002%
54	9.250	2455	2460	2463	rBV	161	177	0.01%	0.002%
55	9.420	2499	2513	2535	rBV	481900	805032	60.18%	8.123%
56	9.578	2553	2562	2568	rVV	1120	1588	0.12%	0.016%
57	9.700	2590	2600	2608	rVB	2100	3065	0.23%	0.031%
58	9.758	2614	2618	2620	rBV	209	185	0.01%	0.002%
59	9.806	2629	2633	2637	rBV2	212	224	0.02%	0.002%
60	9.844	2642	2645	2647	rBV	168	145	0.01%	0.001%
61	9.902	2656	2663	2667	rBV2	201	337	0.03%	0.003%
62	9.967	2678	2683	2686	rBV	230	238	0.02%	0.002%
63	10.060	2708	2712	2715	rBV2	240	197	0.01%	0.002%
64	10.111	2718	2728	2739	rVB7	2470	4594	0.34%	0.046%
65	10.304	2786	2788	2796	rVB2	335	357	0.03%	0.004%
66	10.340	2796	2799	2802	rBV2	169	163	0.01%	0.002%
67	10.491	2831	2846	2852	rBV3	1362	2344	0.18%	0.024%
68	10.574	2866	2872	2875	rVB2	182	211	0.02%	0.002%
69	10.623	2881	2887	2890	rBV2	202	278	0.02%	0.003%
70	10.674	2895	2903	2914	rVB2	3777	5540	0.41%	0.056%
71	10.761	2917	2930	2946	rBV	411970	669286	50.04%	6.753%
72	10.870	2960	2964	2972	rBV4	649	899	0.07%	0.009%
73	11.092	3027	3033	3038	rBV3	1283	1698	0.13%	0.017%
74	11.147	3047	3050	3060	rVB4	506	562	0.04%	0.006%
75	11.468	3138	3150	3161	rVB4	4651	8257	0.62%	0.083%
76	11.516	3161	3165	3167	rBV	219	196	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045268.D
 Acq On : 09 Oct 2021 17:25
 Operator : SY/MD
 Sample : VU1009WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.581	3179	3185	3191	rBV3	734	939	0.07%	0.009%
78	11.700	3216	3222	3229	rVB4	1396	2020	0.15%	0.020%
79	11.748	3229	3237	3246	rBV4	2813	4113	0.31%	0.041%
80	11.815	3246	3258	3276	rBV	466460	732847	54.79%	7.394%
81	11.938	3292	3296	3300	rBV4	942	1094	0.08%	0.011%
82	11.976	3304	3308	3316	rVB4	2248	2971	0.22%	0.030%
83	12.108	3344	3349	3350	rBV2	245	237	0.02%	0.002%
84	12.198	3355	3377	3397	rBV	542133	883603	66.06%	8.915%
85	12.327	3414	3417	3419	rBV3	599	407	0.03%	0.004%
86	12.372	3428	3431	3432	rBV	224	129	0.01%	0.001%
87	12.397	3437	3439	3440	rBV	351	143	0.01%	0.001%
88	12.430	3445	3449	3453	rBV2	300	305	0.02%	0.003%
89	12.857	3580	3582	3587	rBV2	184	152	0.01%	0.002%
90	12.999	3621	3626	3637	rVB4	1669	2419	0.18%	0.024%
91	13.150	3666	3673	3676	rBV3	370	515	0.04%	0.005%
92	13.224	3688	3696	3706	rVB2	5492	7949	0.59%	0.080%
93	13.266	3706	3709	3712	rBV	260	201	0.02%	0.002%
94	13.764	3861	3864	3865	rBV	246	167	0.01%	0.002%
95	13.844	3880	3889	3899	rBV4	12141	17918	1.34%	0.181%
96	14.092	3946	3966	3979	rBV	34797	60200	4.50%	0.607%
97	14.333	4032	4041	4053	rVB3	15746	24049	1.80%	0.243%
98	14.590	4117	4121	4124	rBV2	297	307	0.02%	0.003%
99	14.719	4159	4161	4167	rBV2	354	395	0.03%	0.004%
100	16.648	4759	4761	4763	rBV2	666	381	0.03%	0.004%




Sum of corrected areas: 9911095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045268.D
Acq On : 09 Oct 2021 17:25
Operator : SY/MD
Sample : VU1009WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

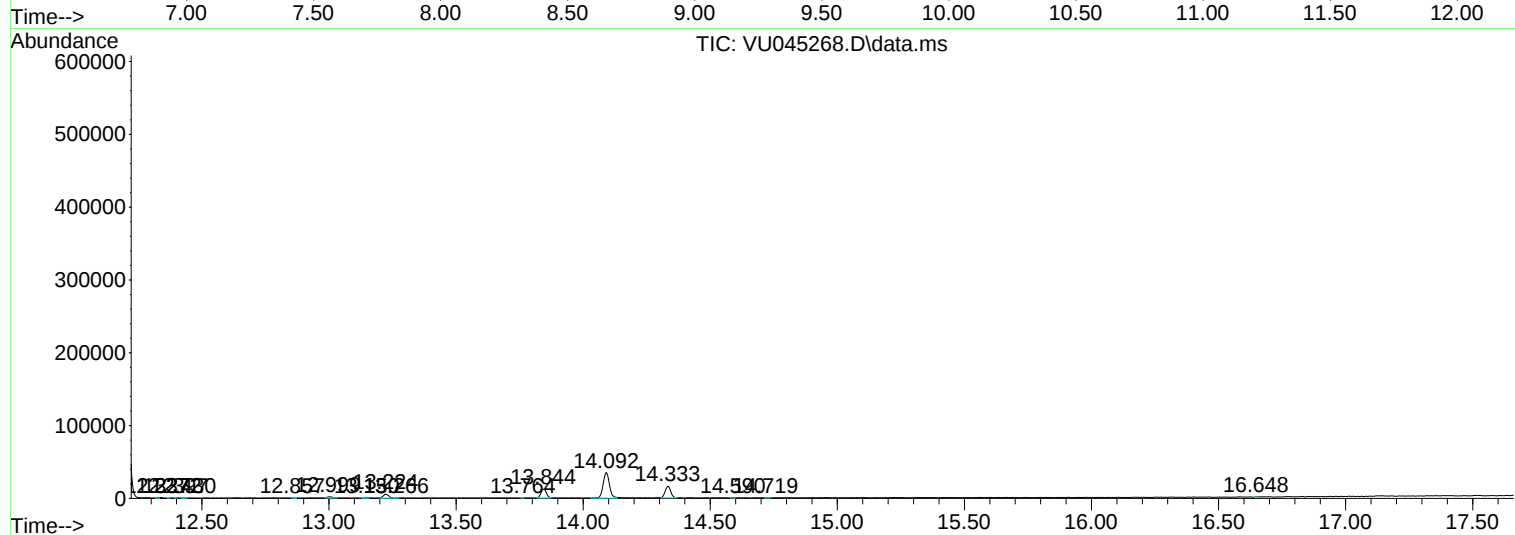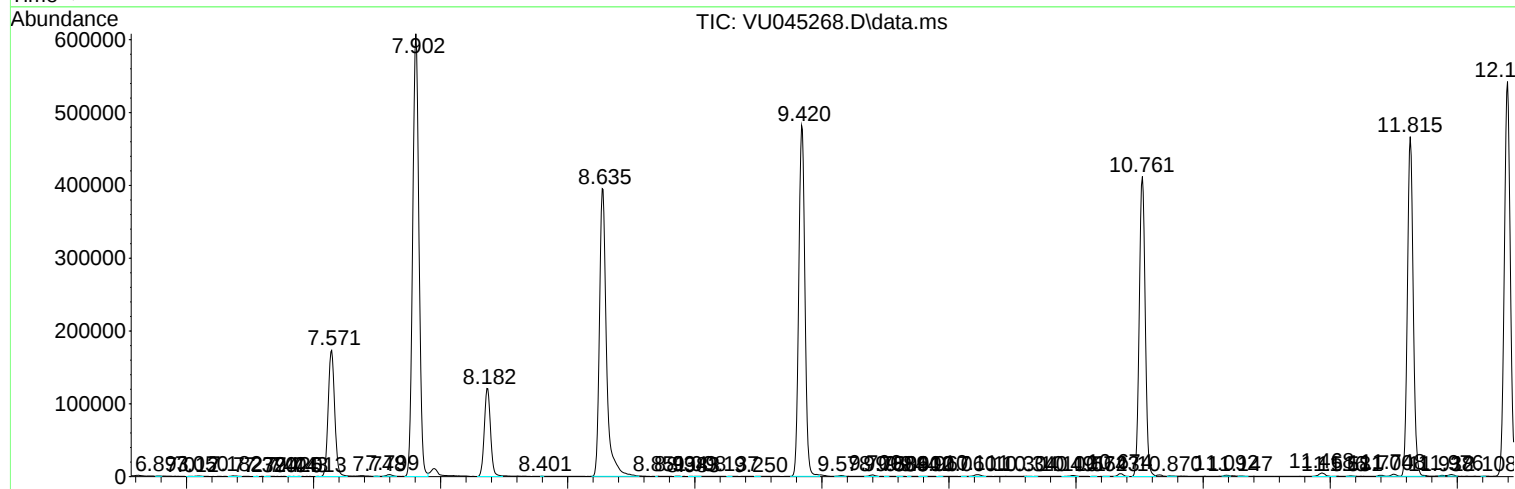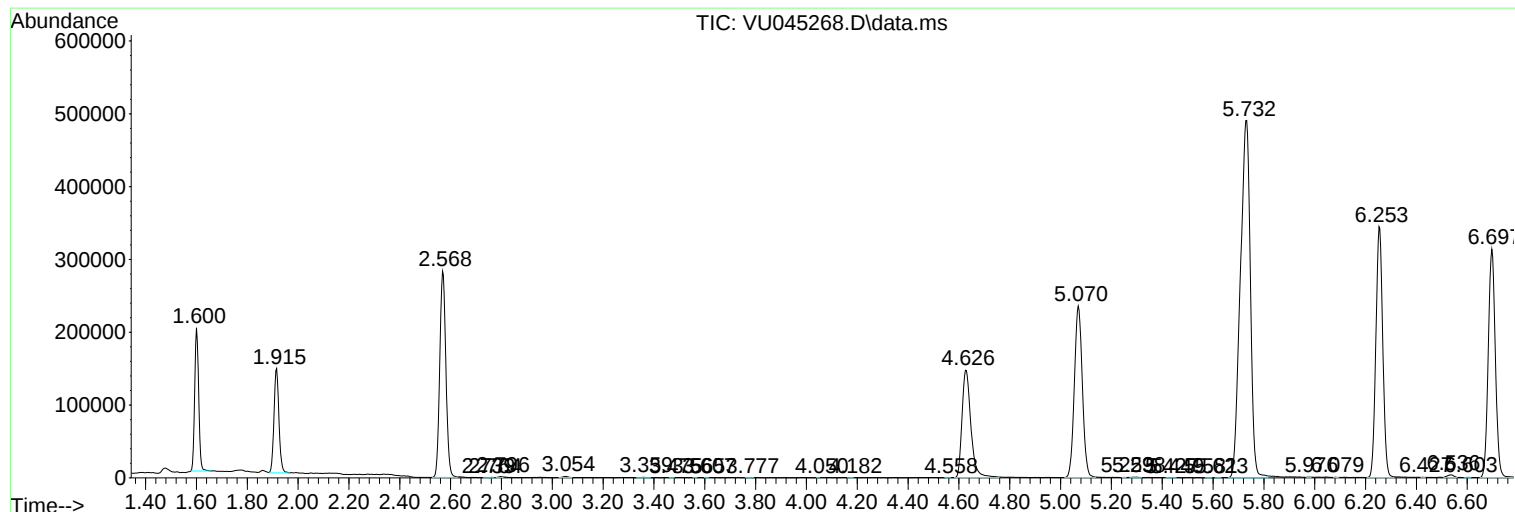

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045268.D
Acq On : 09 Oct 2021 17:25
Operator : SY/MD
Sample : VU1009WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045268.D
Acq On : 09 Oct 2021 17:25
Operator : SY/MD
Sample : VU1009WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
