

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045269.D
 Acq On : 09 Oct 2021 17:49
 Operator : SY/MD
 Sample : M4027-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	35	41	53	rBV2	11959	20301	1.51%	0.208%
2	1.601	74	81	92	rVB	211290	219391	16.37%	2.253%
3	1.903	166	175	195	rVB	144351	199386	14.88%	2.048%
4	2.565	368	381	400	rBV	274407	462258	34.49%	4.747%
5	2.794	443	452	460	rVB2	1066	1615	0.12%	0.017%
6	2.916	483	490	491	rBV	231	249	0.02%	0.003%
7	2.954	497	502	504	rBV2	487	475	0.04%	0.005%
8	3.051	522	532	542	rVB2	3773	6251	0.47%	0.064%
9	3.121	551	554	558	rBV2	226	205	0.02%	0.002%
10	3.189	567	575	587	rVB2	885	1961	0.15%	0.020%
11	3.298	605	609	613	rVB2	189	186	0.01%	0.002%
12	3.324	613	617	618	rBV	199	156	0.01%	0.002%
13	3.356	624	627	630	rBV3	178	158	0.01%	0.002%
14	3.462	655	660	663	rVB2	177	181	0.01%	0.002%
15	3.514	672	676	679	rBV2	213	186	0.01%	0.002%
16	3.568	691	693	697	rVV2	191	156	0.01%	0.002%
17	3.774	754	757	760	rBV	160	158	0.01%	0.002%
18	3.925	797	804	806	rBV2	237	269	0.02%	0.003%
19	3.977	816	820	821	rBV	191	139	0.01%	0.001%
20	4.067	845	848	852	rBV2	148	161	0.01%	0.002%
21	4.141	867	871	876	rVV	172	209	0.02%	0.002%
22	4.507	982	985	988	rBV	184	139	0.01%	0.001%
23	4.626	1007	1022	1050	rBV	150806	353592	26.38%	3.631%
24	4.951	1118	1123	1133	rBV2	241	380	0.03%	0.004%
25	5.070	1142	1160	1180	rBV	234309	510247	38.07%	5.240%
26	5.202	1197	1201	1203	rBV2	236	184	0.01%	0.002%
27	5.260	1216	1219	1222	rBV2	190	182	0.01%	0.002%
28	5.295	1224	1230	1233	rVV2	480	571	0.04%	0.006%
29	5.311	1233	1235	1239	rVB	299	175	0.01%	0.002%
30	5.401	1260	1263	1268	rBV	111	143	0.01%	0.001%
31	5.649	1337	1340	1343	rBV2	166	170	0.01%	0.002%
32	5.729	1343	1365	1396	rVV2	499669	1340247	100.00%	13.763%
33	5.864	1405	1407	1409	rBV	229	154	0.01%	0.002%
34	6.073	1467	1472	1476	rBV3	243	314	0.02%	0.003%
35	6.096	1476	1479	1482	rBV	167	161	0.01%	0.002%
36	6.115	1482	1485	1489	rBV2	247	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045269.D
 Acq On : 09 Oct 2021 17:49
 Operator : SY/MD
 Sample : M4027-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.253	1512	1528	1551	rBV	346016	646666	48.25%	6.641%
38	6.453	1587	1590	1593	rVB	236	171	0.01%	0.002%
39	6.533	1606	1615	1624	rVB4	3692	7124	0.53%	0.073%
40	6.578	1624	1629	1632	rVB3	194	174	0.01%	0.002%

41	6.697	1651	1666	1695	rBV	311100	608533	45.40%	6.249%
42	6.871	1716	1720	1724	rVB	242	158	0.01%	0.002%
43	7.051	1767	1776	1782	rBV3	515	780	0.06%	0.008%
44	7.182	1809	1817	1829	rVB6	1204	2190	0.16%	0.022%
45	7.231	1829	1832	1835	rBV2	179	168	0.01%	0.002%

46	7.501	1913	1916	1919	rBV	181	157	0.01%	0.002%
47	7.568	1924	1937	1954	rBV	155506	268995	20.07%	2.762%
48	7.658	1963	1965	1969	rBV	258	211	0.02%	0.002%
49	7.690	1969	1975	1985	rVB4	992	1719	0.13%	0.018%
50	7.800	2001	2009	2019	rBV2	1123	1485	0.11%	0.015%

51	7.903	2026	2041	2056	rBV	598971	1024497	76.44%	10.521%
52	7.973	2058	2063	2074	rVB	8999	13483	1.01%	0.138%
53	8.182	2116	2128	2143	rBV	107941	178828	13.34%	1.836%
54	8.465	2210	2216	2217	rBV	269	218	0.02%	0.002%
55	8.514	2227	2231	2237	rBV2	332	428	0.03%	0.004%

56	8.636	2255	2269	2300	rBV	427609	764379	57.03%	7.850%
57	8.890	2344	2348	2351	rVB2	240	162	0.01%	0.002%
58	8.932	2357	2361	2364	rBV2	296	294	0.02%	0.003%
59	9.086	2406	2409	2412	rBV	190	172	0.01%	0.002%
60	9.340	2485	2488	2492	rBV	174	161	0.01%	0.002%

61	9.420	2499	2513	2547	rBV	490017	807867	60.28%	8.296%
62	9.571	2555	2560	2572	rVB2	605	905	0.07%	0.009%
63	9.694	2592	2598	2610	rVB3	1649	2401	0.18%	0.025%
64	9.796	2625	2630	2633	rBV2	163	165	0.01%	0.002%
65	9.957	2677	2680	2685	rBV2	244	253	0.02%	0.003%

66	10.038	2700	2705	2708	rBV	162	159	0.01%	0.002%
67	10.057	2708	2711	2716	rBV	143	183	0.01%	0.002%
68	10.163	2741	2744	2749	rBV2	152	160	0.01%	0.002%
69	10.253	2768	2772	2774	rBV2	190	174	0.01%	0.002%
70	10.423	2822	2825	2827	rBV2	192	145	0.01%	0.001%

71	10.485	2840	2844	2853	rVB3	404	661	0.05%	0.007%
72	10.571	2868	2871	2874	rBV2	257	180	0.01%	0.002%
73	10.632	2887	2890	2893	rBV2	218	163	0.01%	0.002%
74	10.674	2893	2903	2910	rVV5	1967	2873	0.21%	0.030%
75	10.761	2916	2930	2948	rBV	430634	691410	51.59%	7.100%

76	10.861	2958	2961	2967	rBV3	311	409	0.03%	0.004%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045269.D
 Acq On : 09 Oct 2021 17:49
 Operator : SY/MD
 Sample : M4027-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.012	3005	3008	3012	rVB2	263	213	0.02%	0.002%
78	11.121	3038	3042	3044	rVB	274	142	0.01%	0.001%
79	11.147	3049	3050	3057	rVB	192	177	0.01%	0.002%
80	11.192	3062	3064	3066	rBV2	191	137	0.01%	0.001%
81	11.468	3141	3150	3159	rBV2	1863	3240	0.24%	0.033%
82	11.697	3217	3221	3227	rVV3	750	948	0.07%	0.010%
83	11.755	3231	3239	3244	rBV3	954	1170	0.09%	0.012%
84	11.816	3245	3258	3275	rBV	436636	697499	52.04%	7.163%
85	11.944	3294	3298	3301	rBV3	420	451	0.03%	0.005%
86	11.973	3303	3307	3316	rVB4	1161	1659	0.12%	0.017%
87	12.073	3331	3338	3339	rBV	205	275	0.02%	0.003%
88	12.195	3361	3376	3397	rBV	520061	850140	63.43%	8.730%
89	12.272	3397	3400	3404	rVV2	351	287	0.02%	0.003%
90	12.648	3514	3517	3519	rVB2	259	139	0.01%	0.001%
91	13.002	3625	3627	3631	rVB	298	190	0.01%	0.002%
92	13.086	3649	3653	3655	rBV2	259	221	0.02%	0.002%
93	13.224	3689	3696	3704	rBV3	1760	2257	0.17%	0.023%
94	13.845	3883	3889	3900	rVB3	3414	4891	0.36%	0.050%
95	13.906	3905	3908	3911	rVB	434	303	0.02%	0.003%
96	13.928	3911	3915	3918	rBV2	178	185	0.01%	0.002%
97	14.092	3958	3966	3978	rBV	10463	16489	1.23%	0.169%
98	14.333	4034	4041	4051	rVB3	4299	6236	0.47%	0.064%
99	14.578	4113	4117	4118	rBV	316	217	0.02%	0.002%
100	14.655	4138	4141	4144	rBV2	230	196	0.01%	0.002%




Sum of corrected areas: 9737862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045269.D
Acq On : 09 Oct 2021 17:49
Operator : SY/MD
Sample : M4027-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

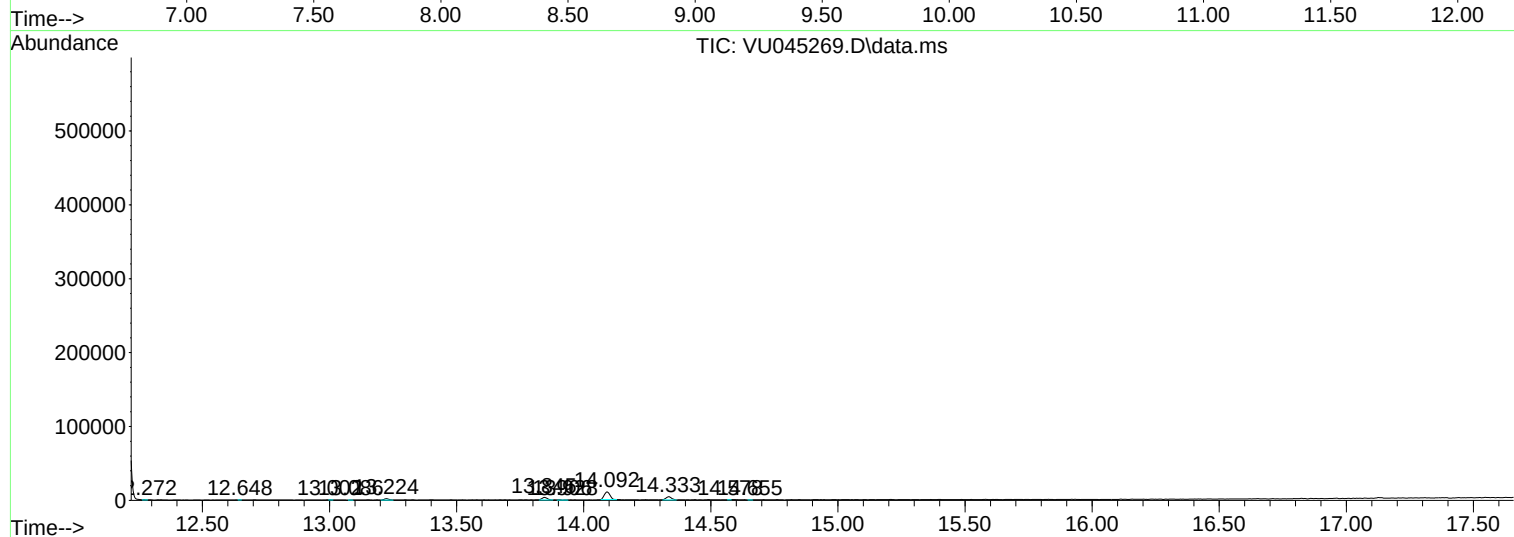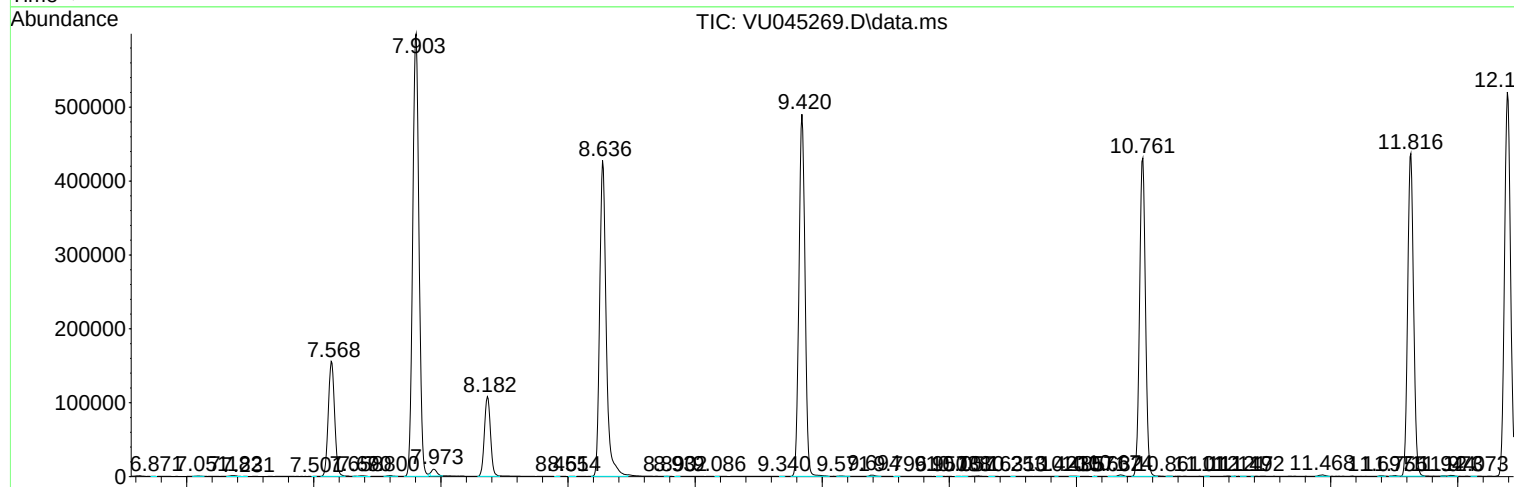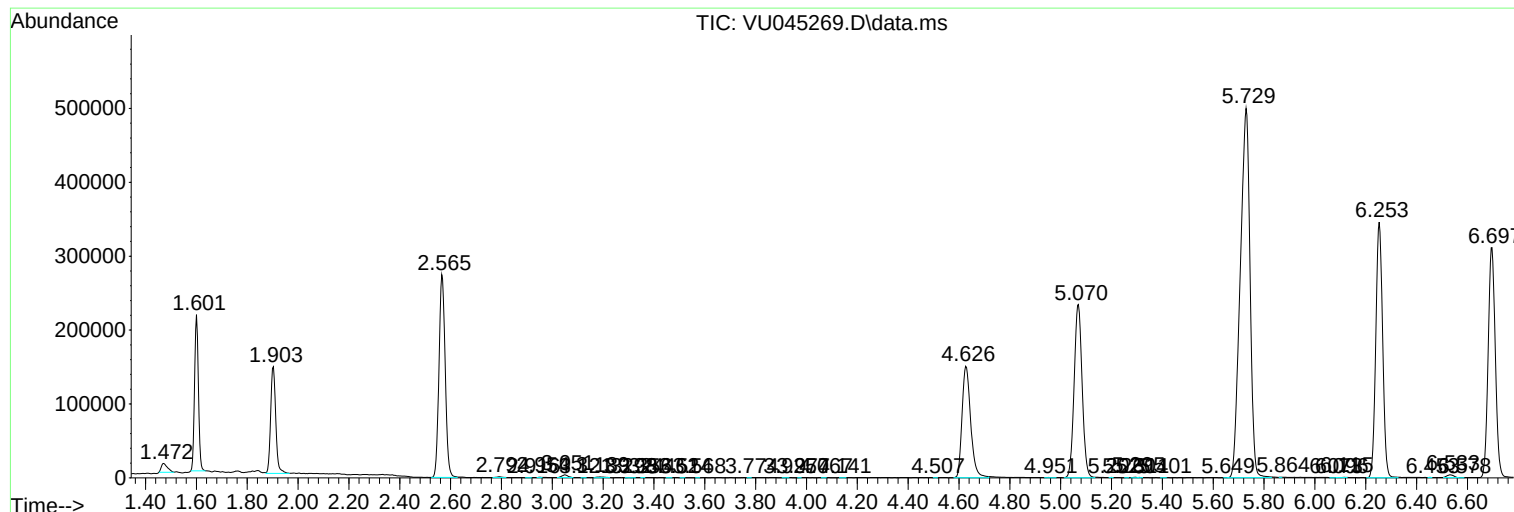

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045269.D
Acq On : 09 Oct 2021 17:49
Operator : SY/MD
Sample : M4027-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
Data File : VU045269.D
Acq On : 09 Oct 2021 17:49
Operator : SY/MD
Sample : M4027-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
