
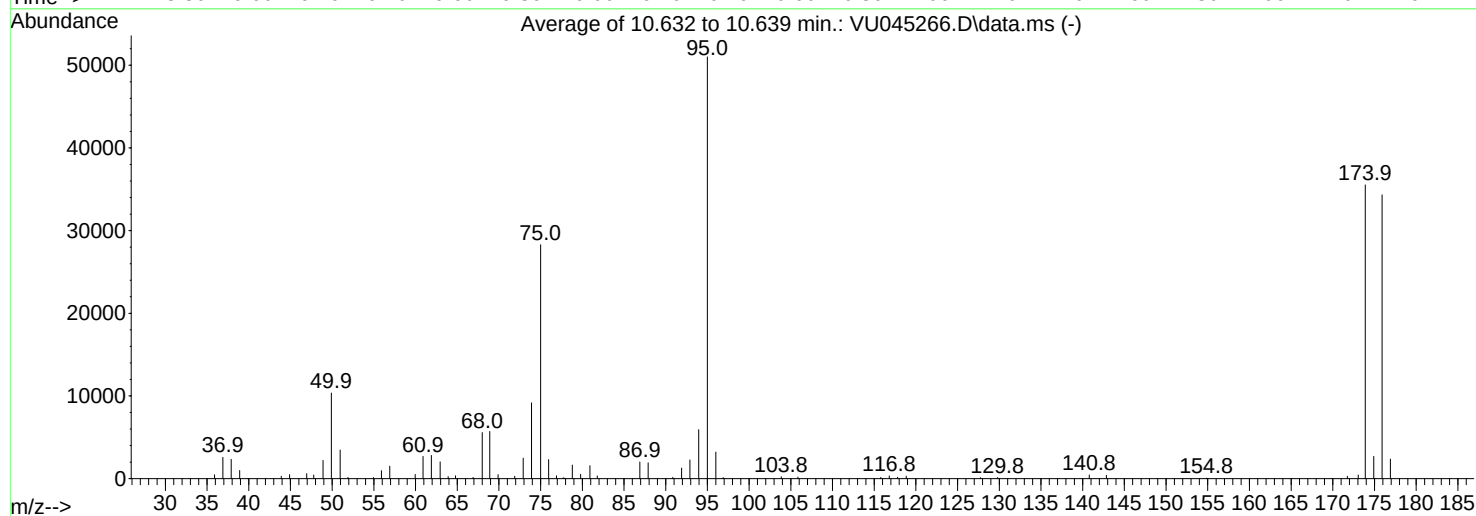


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100921\
 Data File : VU045266.D
 Acq On : 09 Oct 2021 16:31
 Operator : SY/MD
 Sample : BFB010
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB010

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 13 02:48:52 2021

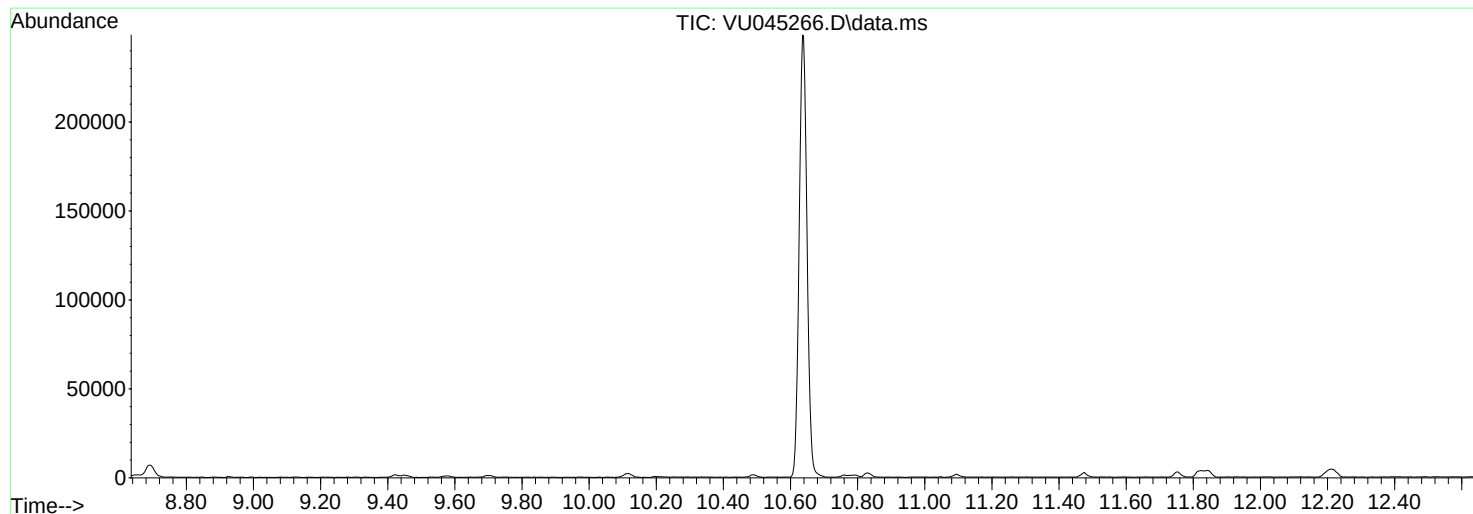

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	10359	PASS
75	95	30	80	55.5	28301	PASS
95	95	100	100	100.0	51019	PASS
96	95	5	9	6.3	3214	PASS
173	174	0.00	2	1.2	438	PASS
174	95	50	120	69.6	35525	PASS
175	174	5	9	7.6	2701	PASS
176	174	95	101	96.6	34333	PASS
177	176	5	9	6.9	2370	PASS

Scan 2878 (10.594 min): VU045266.D\data.ms
BFB010

m/z	Abundance
39.90	112.0
43.90	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	413.0
36.90	2506.0
37.90	2129.0
38.90	892.0
39.90	139.0
43.90	592.0
44.90	489.0
46.90	563.0
47.80	443.0
48.90	2193.0
49.90	9741.0
50.90	3298.0
51.90	191.0
54.90	135.0
55.90	904.0
56.90	1452.0
60.00	444.0
60.90	2525.0
61.90	2622.0
63.00	2033.0
63.90	288.0
64.80	373.0
66.90	159.0
68.00	5340.0
68.90	5573.0
69.90	488.0
71.90	267.0
72.90	2329.0
73.90	8880.0
75.00	27088.0
76.00	2195.0
76.90	366.0
77.70	178.0
78.80	1592.0
79.80	468.0
80.90	1557.0
81.80	336.0
86.90	1833.0
87.90	1760.0
90.80	121.0
91.90	1228.0
92.90	2119.0
93.90	5684.0
95.00	48216.0
96.00	2928.0
96.90	113.0
103.90	228.0
105.80	189.0
115.80	150.0
116.80	325.0
117.80	142.0
118.80	279.0
127.80	111.0
129.80	121.0
140.80	439.0
142.90	407.0
171.80	249.0
173.10	419.0
173.90	32696.0
174.90	2599.0
175.90	31200.0
176.90	2156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	466.0
36.90	2652.0
37.90	2366.0
38.90	999.0
39.80	139.0
43.90	641.0
44.90	497.0
47.00	625.0
47.80	470.0
48.90	2273.0
49.90	10593.0
50.90	3622.0
51.90	165.0
54.90	137.0
55.90	993.0
56.90	1560.0
60.00	528.0
60.90	2753.0
61.90	2950.0
63.00	2092.0
63.90	277.0
64.80	359.0
66.90	154.0
68.00	5740.0
68.90	5927.0
69.90	517.0
71.90	299.0
72.90	2537.0
73.90	9449.0
75.00	29400.0
76.00	2357.0
76.90	357.0
77.70	178.0
78.80	1703.0
79.80	536.0
80.90	1609.0
81.80	331.0
86.90	2010.0
87.90	1986.0
90.80	153.0
91.90	1309.0
92.90	2376.0
93.90	6059.0
95.00	52464.0
96.00	3308.0
96.90	152.0
103.90	248.0
105.80	206.0
115.80	157.0
116.80	340.0
117.80	175.0
118.90	322.0
127.80	131.0
129.80	149.0
140.80	456.0
142.80	422.0
154.90	102.0
171.80	303.0
173.00	459.0
173.90	36624.0
174.90	2786.0
175.90	35392.0
176.90	2490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	506.0
36.90	2583.0
37.90	2534.0
38.90	1049.0
39.80	137.0
43.90	627.0
44.90	482.0
47.00	632.0
47.80	400.0
48.90	2149.0
49.90	10743.0
51.00	3474.0
51.90	129.0
55.00	142.0
55.90	992.0
56.90	1523.0
59.90	528.0
60.90	2782.0
61.90	2840.0
62.90	1995.0
63.90	203.0
64.80	300.0
66.90	124.0
68.00	5635.0
68.90	5641.0
69.90	470.0
71.90	312.0
72.90	2570.0
73.90	9211.0
75.00	28416.0
75.90	2354.0
76.90	322.0
77.90	181.0
78.80	1644.0
79.80	570.0
80.90	1560.0
81.80	306.0
86.90	2174.0
87.90	1994.0
90.90	187.0
91.90	1325.0
92.90	2279.0
94.00	6039.0
95.00	52376.0
96.00	3406.0
96.90	147.0
103.80	222.0
105.90	215.0
115.80	155.0
116.80	349.0
117.80	180.0
118.90	304.0
127.70	133.0
129.80	162.0
140.80	421.0
142.80	419.0
154.80	100.0
171.70	324.0
173.00	435.0
173.90	37256.0
174.90	2717.0
175.90	36408.0
176.90	2465.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010