

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
 Data File : VU051302.D
 Acq On : 09 Oct 2022 16:02
 Operator : JC/MD
 Sample : N5013-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA38

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 10 01:27:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 10 01:25:26 2022
 Response via : Initial Calibration

10/10/2022
 Supervised By :Mahesh
 Dadoda

10/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	218627	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	228814	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	133731	5.000	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.594	65	64319	3.647	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.000%
7) Chloroethane-d5	1.909	69	61607	4.066	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.562	65	25061	3.595	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.800%
20) 2-Butanone-d5	4.626	46	212423	54.710	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.420%
24) Chloroform-d	5.060	84	140776	4.282	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
26) 1,2-Dichloroethane-d4	5.703	65	76612	4.518	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
32) Benzene-d6	5.729	84	273116	4.339	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	6.690	67	94337	4.413	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.899	98	230191	4.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	8.179	79	33233	4.732	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%
46) 2-Hexanone-d5	8.632	63	124653	52.661	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.320%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	85551	5.010	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	108297	4.659	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%

Target Compounds

						Qvalue
5) Vinyl chloride	1.601	62	259820	10.578	ug/L	95
8) Chloroethane	1.932	64	350869	22.399	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.575	101	5891	0.347	ug/L	97
12) 1,1-Dichloroethene	2.575	96	3788	0.238	ug/L #	1
13) Acetone	2.636	43	208971	71.758	ug/L	93
18) trans-1,2-Dichloroethene	3.353	96	3487	0.208	ug/L #	84
19) 1,1-Dichloroethane	3.867	63	118198	3.415	ug/L	99
21) 2-Butanone	4.713	43	77140	16.808	ug/L	99
22) cis-1,2-Dichloroethene	4.665	96	1457563	78.451	ug/L	98
29) 1,1,1-Trichloroethane	5.314	97	7617	0.278	ug/L	97
30) Cyclohexane	5.385	56	59942	2.578	ug/L	99
33) Benzene	5.761	78	24649849m	322.691	ug/L	
35) Methylcyclohexane	6.761	83	66193	2.753	ug/L	92
40) 4-Methyl-2-pentanone	7.793	43	98468	8.964	ug/L	97
42) Toluene	7.960	91	25548813m	315.099	ug/L	
47) Tetrachloroethene	8.552	164	3373	0.241	ug/L	90
51) Chlorobenzene	9.446	112	5604315	115.679	ug/L	98
52) Ethylbenzene	9.571	91	8575491	117.691	ug/L	98
53) m,p-Xylene	9.693	106	8548880	302.515	ug/L	69

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
 Data File : VU051302.D
 Acq On : 09 Oct 2022 16:02
 Operator : JC/MD
 Sample : N5013-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA38

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 10 01:27:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 10 01:25:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
54) o-Xylene	10.099	106	2455035	91.816	ug/L	98	
60) Isopropylbenzene	10.484	105	1754430	20.713	ug/L	99	
62) 1,3,5-Trimethylbenzene	11.086	105	488220	21.728	ug/L	99	
63) 1,2,4-Trimethylbenzene	11.465	105	2321547	36.534	ug/L	100	
64) 1,3-Dichlorobenzene	11.745	146	44039	1.051	ug/L	95	
65) 1,4-Dichlorobenzene	11.835	146	222899	5.398	ug/L	99	
67) 1,2-Dichlorobenzene	12.211	146	280568	6.888	ug/L	99	
70) 1,2,4-trichlorobenzene	13.838	180	6138	0.299	ug/L #	87	

10/10/2022

Supervised By :Mahesh
 Dadoda

10/11/2022

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
Data File : VU051302.D
Acq On : 09 Oct 2022 16:02
Operator : JC/MD
Sample : N5013-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA38


Quant Time: Oct 10 01:27:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 10 01:25:26 2022
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022

10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

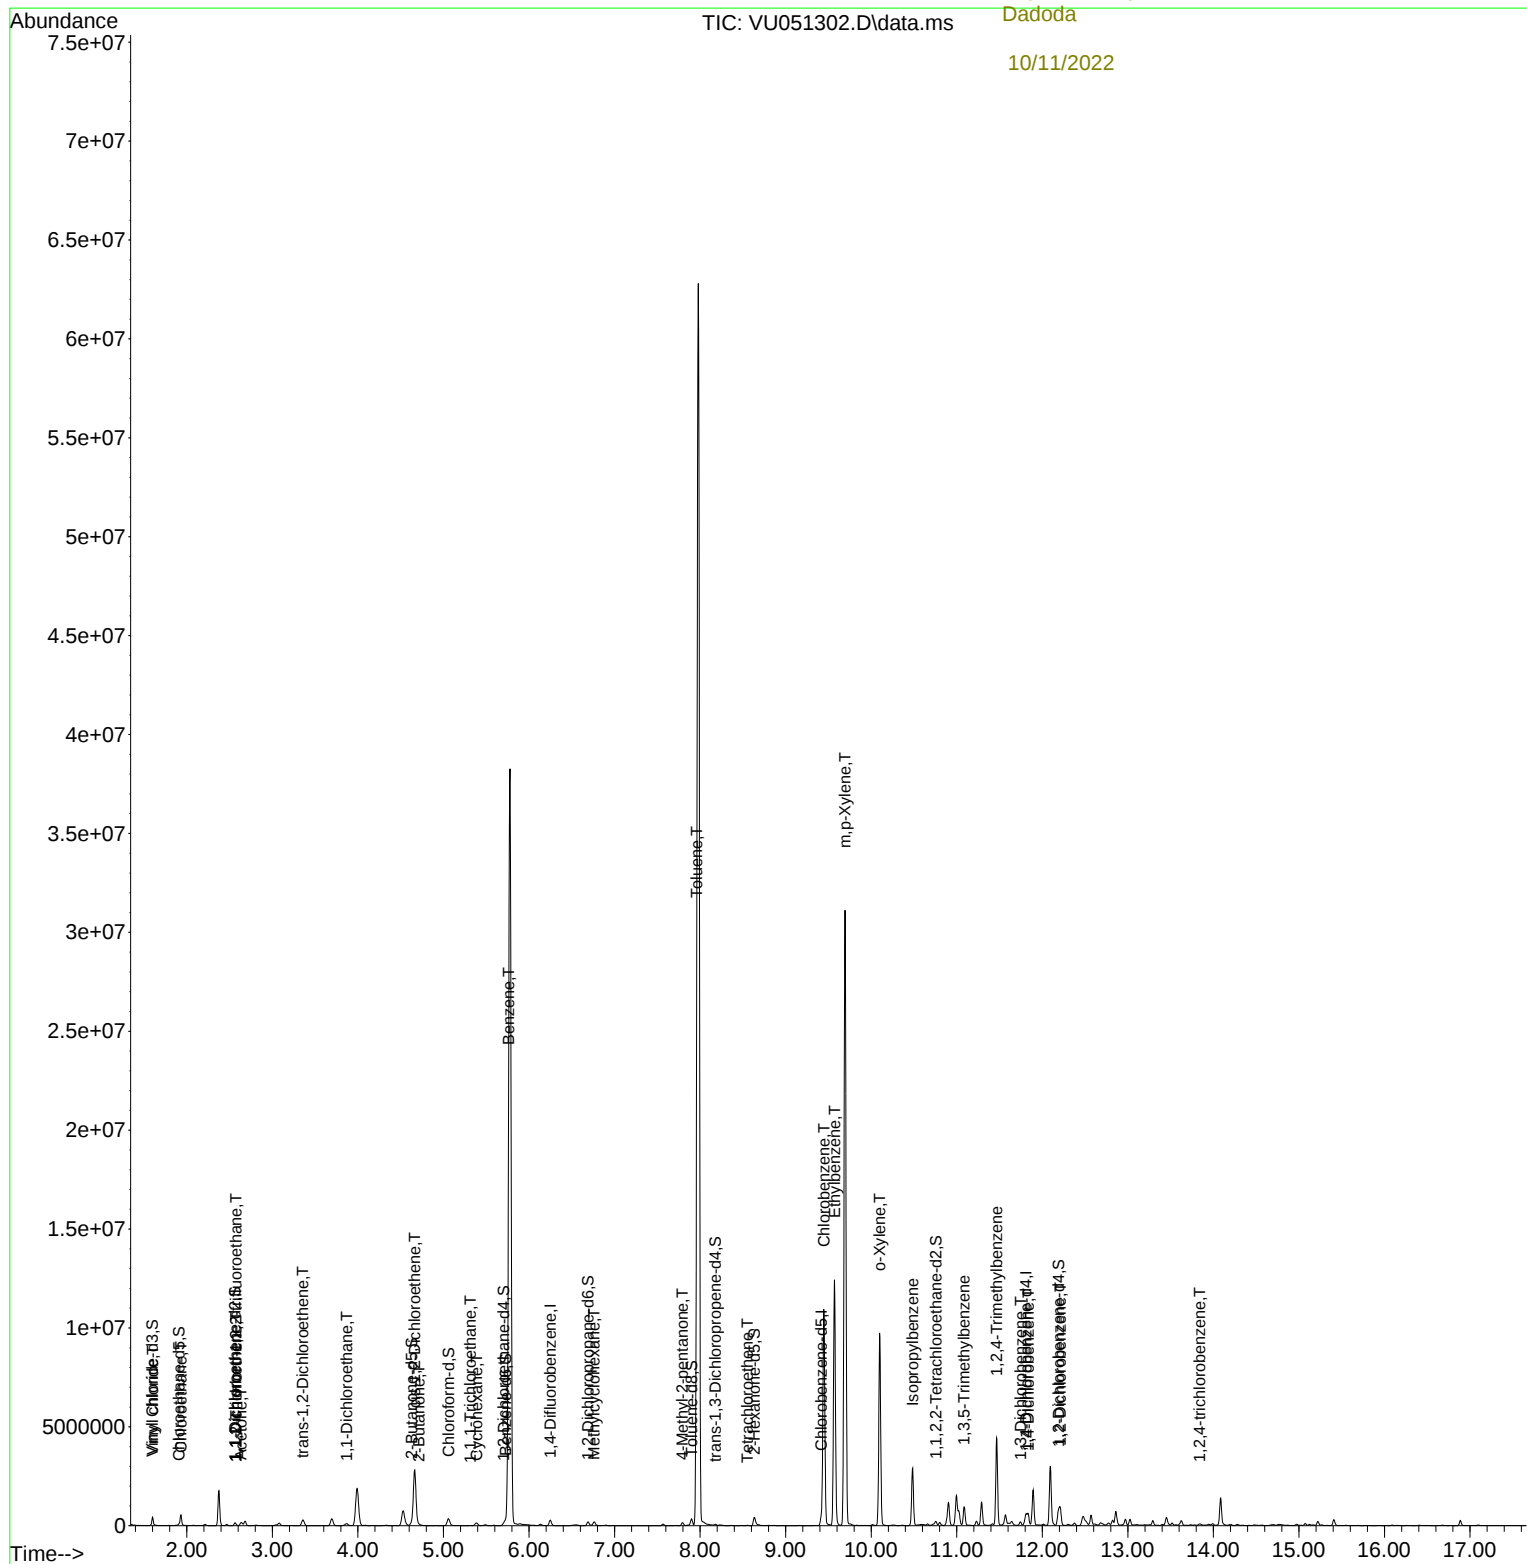

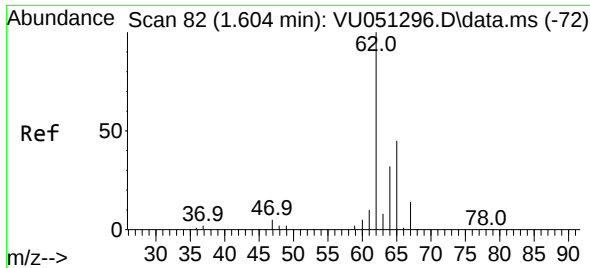

#5
 Vinyl chloride
 Concen: 10.578 ug/L
 RT: 1.601 min Scan# 81
 Delta R.T. -0.003 min
 Lab File: VU051302.D
 Acq: 09 Oct 2022 16:02



Instrument :
 MSVOA_U
 ClientSampleId :
 BHA38

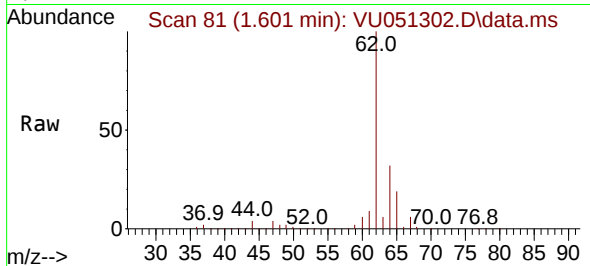

Tgt Ion: 62 Resp: 259820
 Ion Ratio Lower Upper
 62 100
 64 31.6 24.0 44.6


Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/11/2022

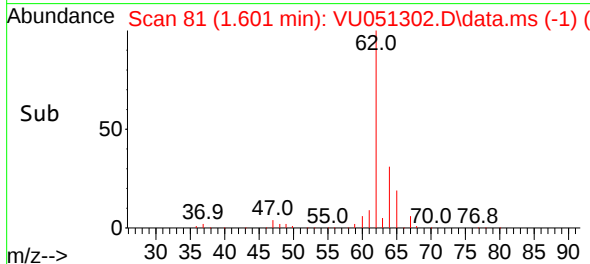




10/10/2022
 Supervised By :Mahesh
 Dadoda


10/11/2022

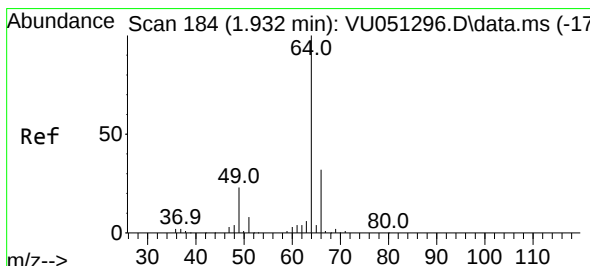

#8
 Chloroethane
 Concen: 22.399 ug/L
 RT: 1.932 min Scan# 184
 Delta R.T. -0.000 min
 Lab File: VU051302.D
 Acq: 09 Oct 2022 16:02

Tgt Ion: 64 Resp: 350869
 Ion Ratio Lower Upper
 64 100
 66 31.9 22.3 41.3

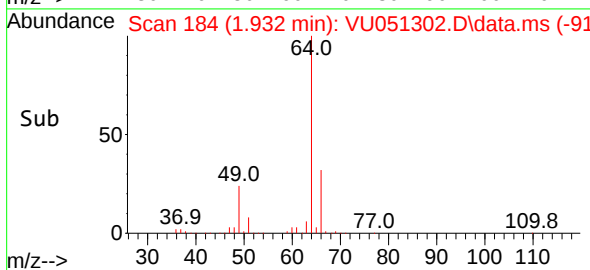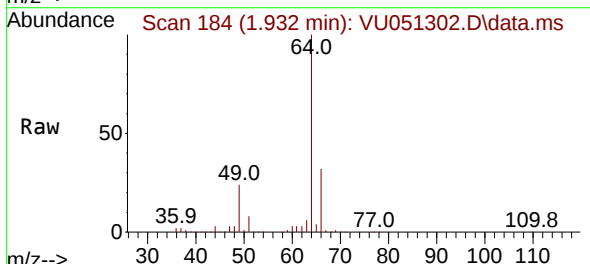



#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.347 ug/L
 RT: 2.575 min Scan# 384
 Delta R.T. -0.003 min
 Lab File: VU051302.D
 Acq: 09 Oct 2022 16:02

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA38





Tgt Ion: 101 Resp: 589
 Ion Ratio Lower Upper
 101 100
 85 43.0 34.6 51.8
 151 67.3 56.5 84.7

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/10/2022
 Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
 Supervised By :Mahesh
 Dadoda


10/11/2022

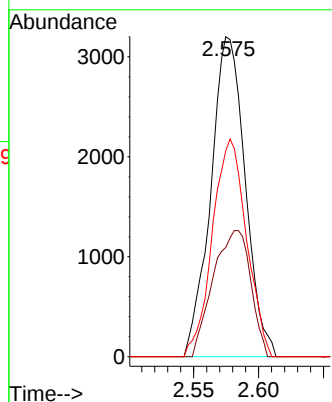

#12
 1,1-Dichloroethene
 Concen: 0.238 ug/L
 RT: 2.575 min Scan# 384
 Delta R.T. -0.003 min
 Lab File: VU051302.D
 Acq: 09 Oct 2022 16:02


Tgt Ion: 96 Resp: 3788
 Ion Ratio Lower Upper
 96 100
 61 305.0 117.6 218.4#
 63 1373.9 85.2 158.2#

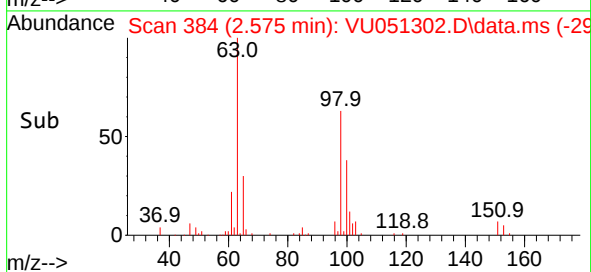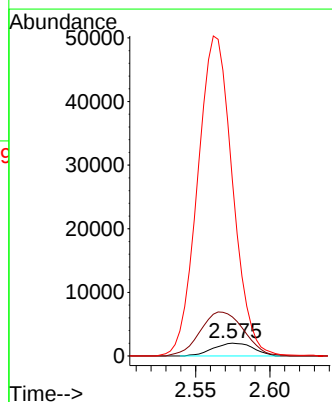



#13
Acetone
Concen: 71.758 ug/L
RT: 2.636 min Scan# 405
Delta R.T. -0.007 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02


Instrument :
MSVOA_U
ClientSampleId :
BHA38



Tgt Ion: 43 Resp: 20897
Ion Ratio Lower Upper
43 100
58 38.2 0.0 68.8


Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022

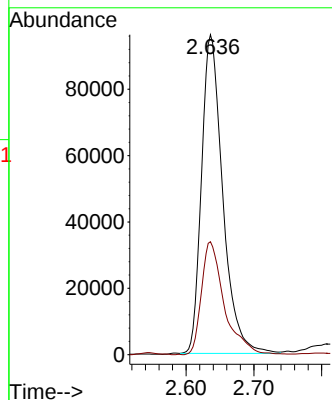




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022



#18
trans-1,2-Dichloroethene
Concen: 0.208 ug/L
RT: 3.353 min Scan# 626
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Tgt Ion: 96 Resp: 3487
Ion Ratio Lower Upper
96 100
61 159.4 101.4 188.2
98 84.9 44.9 83.5#

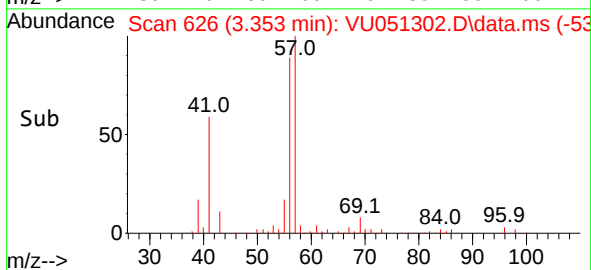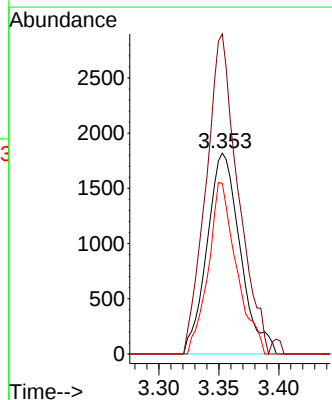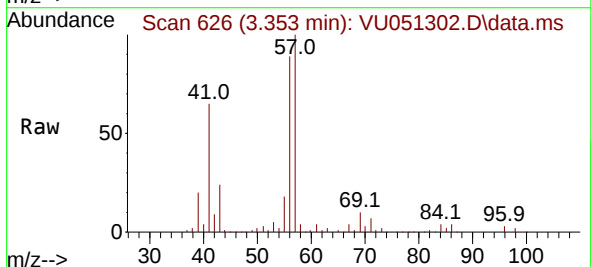



#19
1,1-Dichloroethane
Concen: 3.415 ug/L
RT: 3.867 min Scan# 786
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38





Tgt Ion: 63 Resp: 118198
Ion Ratio Lower Upper
63 100
65 31.3 22.0 41.0
83 12.1 9.0 16.6

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

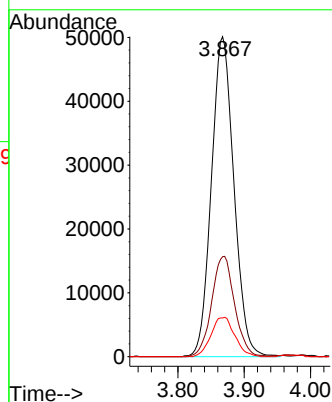

#21
2-Butanone
Concen: 16.808 ug/L
RT: 4.713 min Scan# 1049
Delta R.T. 0.003 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Tgt Ion: 43 Resp: 77140
Ion Ratio Lower Upper
43 100
72 26.8 13.8 41.4

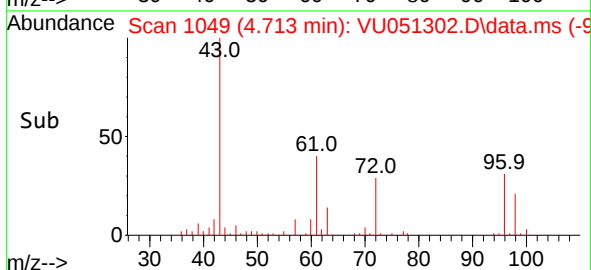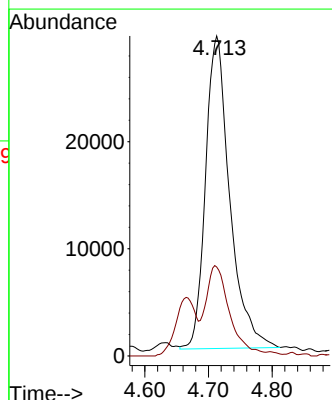

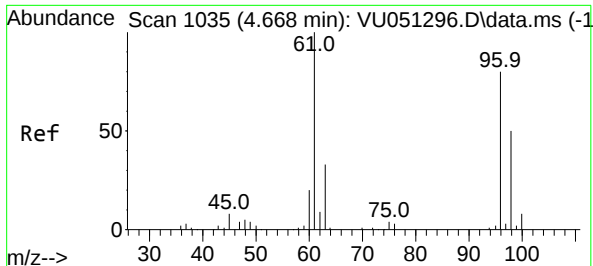

#22

cis-1,2-Dichloroethene

Concen: 78.451 ug/L

RT: 4.665 min Scan# 1035

Delta R.T. -0.003 min

Lab File: VU051302.D

Acq: 09 Oct 2022 16:02

Instrument :

MSVOA_U

ClientSampleId :

BHA38

Tgt Ion: 96 Resp: 145756

Ion Ratio Lower Upper

96 100

61 130.7 90.6 168.2

98 64.2 47.5 88.3

Manual Integrations

APPROVED





Reviewed By :Krupa Patel 10/10/2022

Supervised By :Mahesh Dadoda 10/11/2022

10/10/2022

Supervised By :Mahesh
Dadoda

10/11/2022

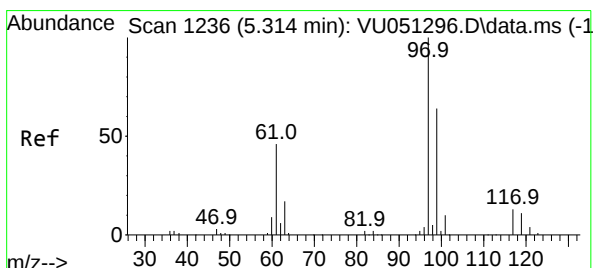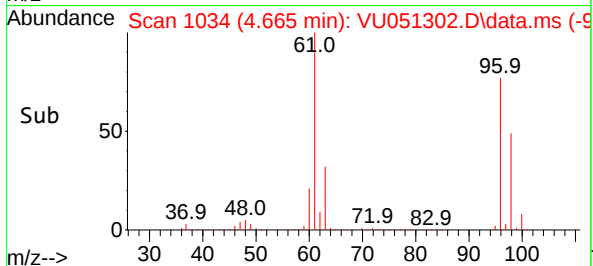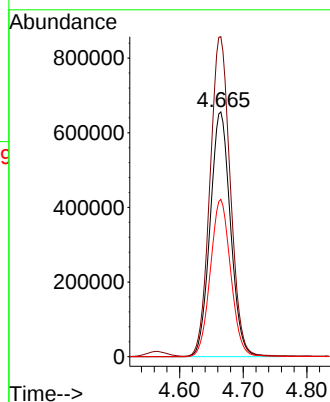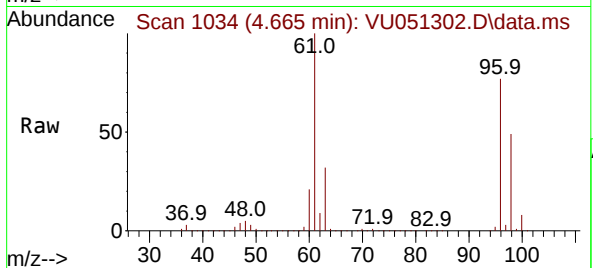

#29

1,1,1-Trichloroethane

Concen: 0.278 ug/L

RT: 5.314 min Scan# 1236

Delta R.T. -0.000 min

Lab File: VU051302.D

Acq: 09 Oct 2022 16:02




Tgt Ion: 97 Resp: 7617


Ion Ratio Lower Upper

97 100

99 63.5 50.2 75.4


61 52.6 38.7 58.1

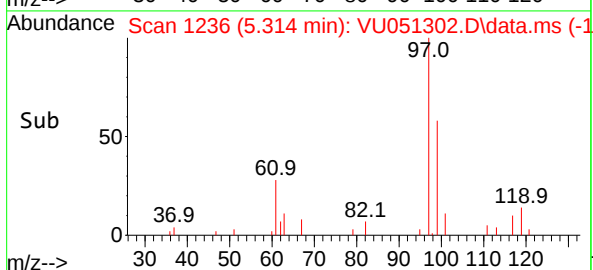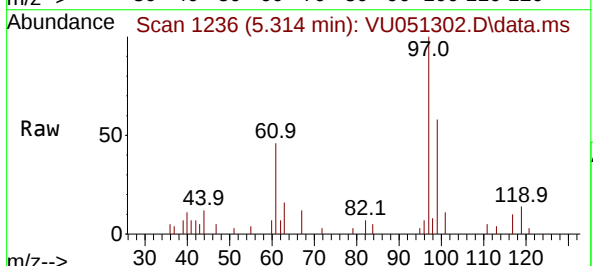

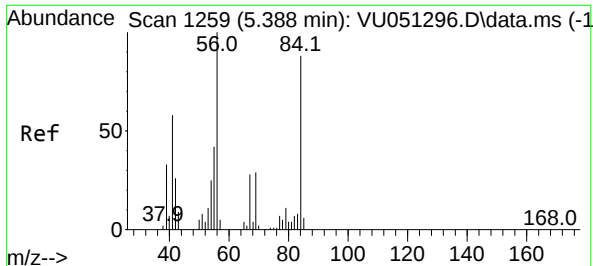

#30
Cyclohexane
Concen: 2.578 ug/L
RT: 5.385 min Scan# 1259
Delta R.T. -0.003 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38

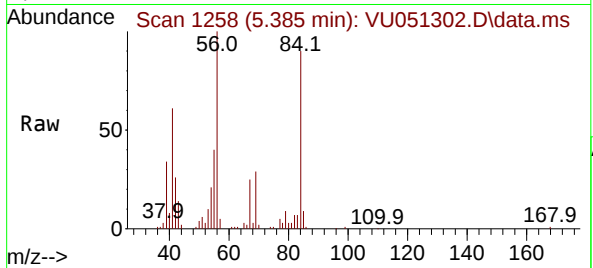




Tgt Ion: 56 Resp: 5994
Ion Ratio Lower Upper
56 100
69 31.8 25.1 37.7
84 87.0 70.9 106.3

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

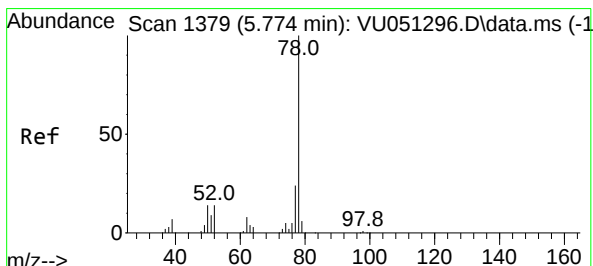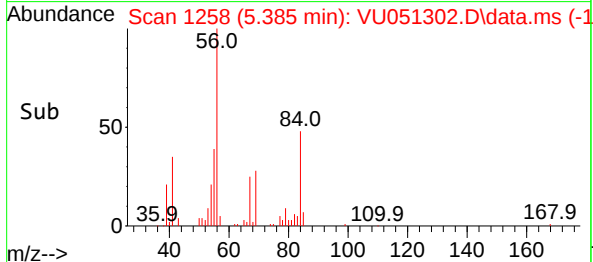

#33
Benzene
Concen: 322.691 ug/L m
RT: 5.761 min Scan# 1375
Delta R.T. -0.013 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Tgt Ion: 78 Resp:24649849

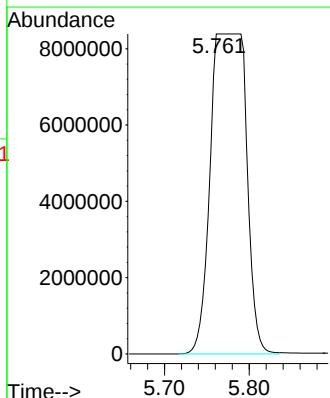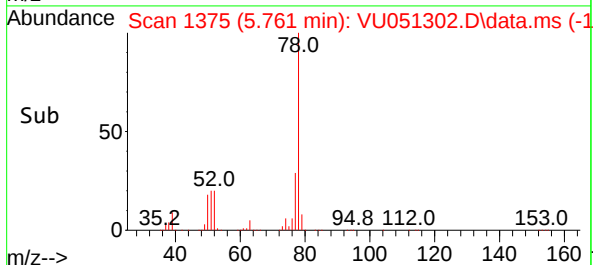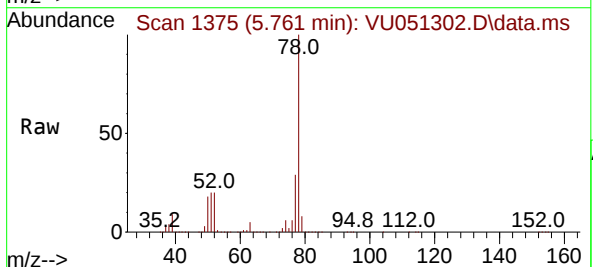

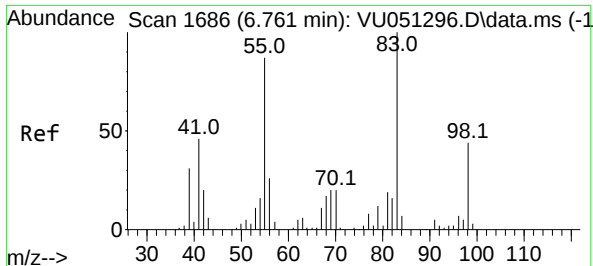

#35

Methylcyclohexane

Concen: 2.753 ug/L

RT: 6.761 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU051302.D

Acq: 09 Oct 2022 16:02

Instrument :

MSVOA_U

ClientSampleId :

BHA38

Tgt Ion: 83	Resp: 6619
Ion Ratio	Lower Upper
83 100	
55 93.9	65.8 98.6
98 44.8	35.9 53.9

Manual Integrations

APPROVED





Reviewed By :Krupa Patel 10/10/2022

Supervised By :Mahesh Dadoda 10/11/2022

10/10/2022

Supervised By :Mahesh
Dadoda

10/11/2022

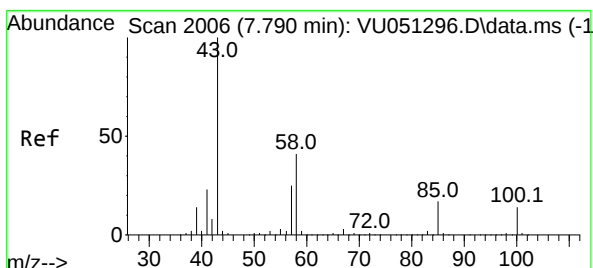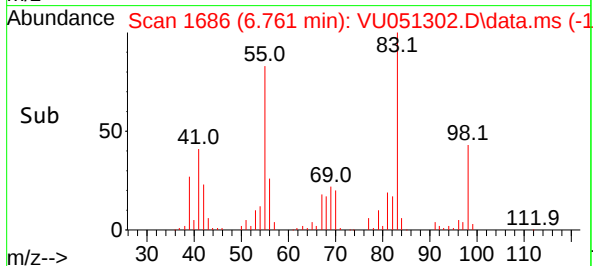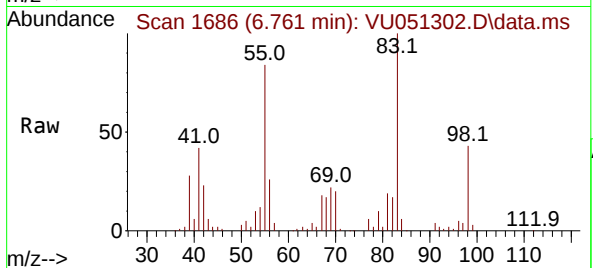

#40

4-Methyl-2-pentanone

Concen: 8.964 ug/L




RT: 7.793 min Scan# 2007


Delta R.T. 0.003 min

Lab File: VU051302.D

Acq: 09 Oct 2022 16:02


Tgt Ion: 43	Resp: 98468
Ion Ratio	Lower Upper
43 100	
58 38.7	33.0 49.6
100 14.4	11.8 17.6

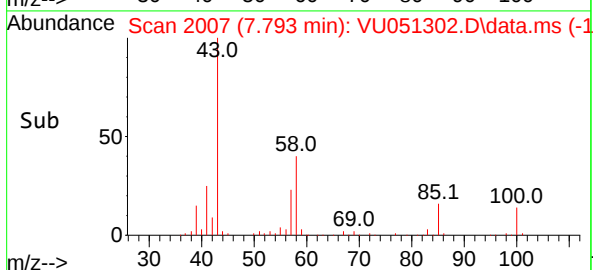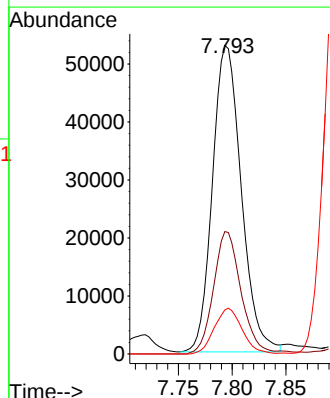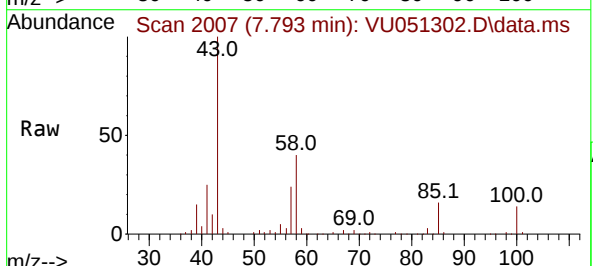



#42
Toluene
Concen: 315.099 ug/L m
RT: 7.960 min Scan# 2062
Delta R.T. -0.010 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38






Tgt Ion: 91 Resp: 2554881
Ion Ratio Lower Upper
91 100
92 84.2 39.9 74.1

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

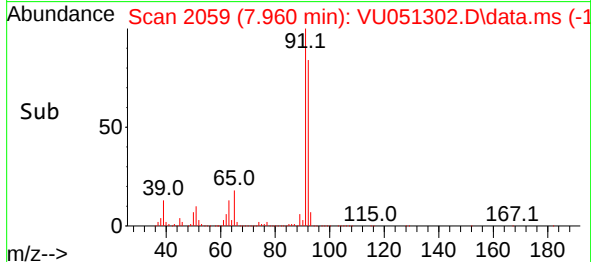

#47
Tetrachloroethene
Concen: 0.241 ug/L
RT: 8.552 min Scan# 2243
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02


Tgt Ion: 164 Resp: 3373
Ion Ratio Lower Upper
164 100
129 102.0 71.3 132.3
131 114.7 66.9 124.3
166 142.1 90.9 168.7

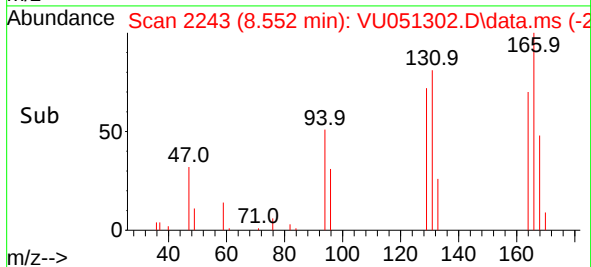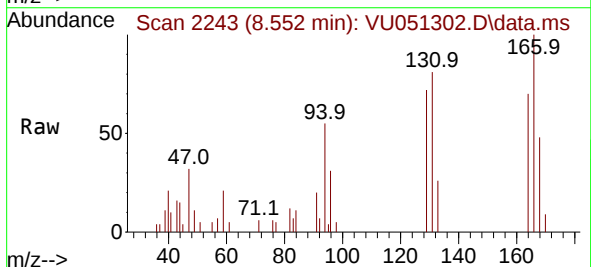



#51
Chlorobenzene
Concen: 115.679 ug/L
RT: 9.446 min Scan# 2521
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38






Tgt Ion:112 Resp: 560431
Ion Ratio Lower Upper
112 100
114 31.9 22.3 41.5
77 62.1 48.1 72.1

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022



#52
Ethylbenzene
Concen: 117.691 ug/L
RT: 9.571 min Scan# 2560
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Tgt Ion: 91 Resp: 8575491
Ion Ratio Lower Upper
91 100
106 30.6 20.9 38.7

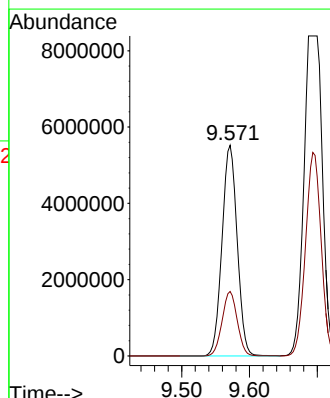







#53
m,p-Xylene
Concen: 302.515 ug/L
RT: 9.693 min Scan# 2598
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38

Tgt Ion:106 Resp: 8548880
Ion Ratio Lower Upper
106 100
91 157.2 143.9 267.3




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022

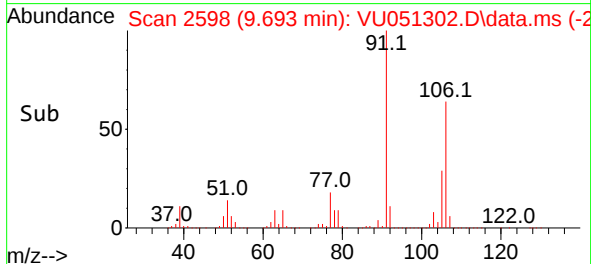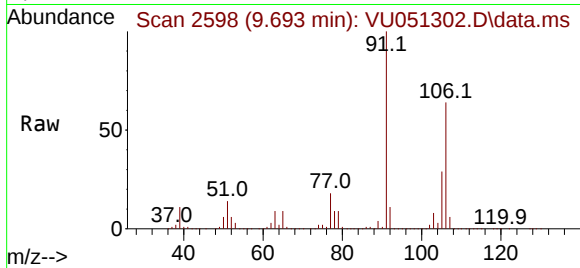

#54
o-Xylene
Concen: 91.816 ug/L
RT: 10.099 min Scan# 2724
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02


Tgt Ion:106 Resp: 2455035
Ion Ratio Lower Upper
106 100
91 217.6 154.4 286.8

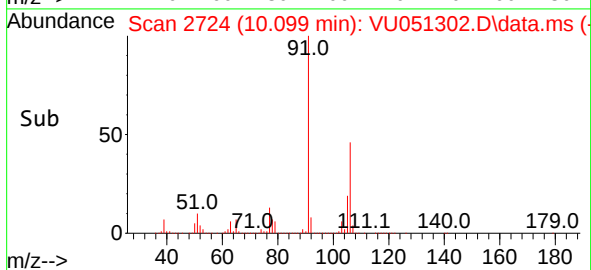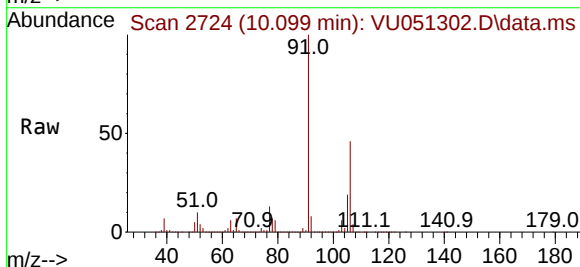

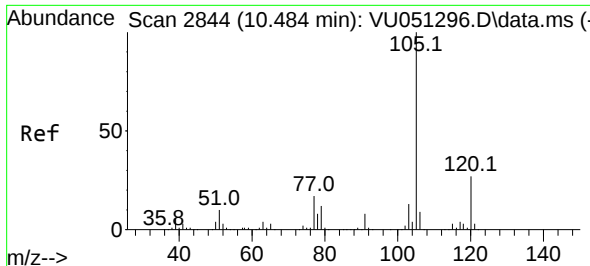

#60
Isopropylbenzene
Concen: 20.713 ug/L
RT: 10.484 min Scan# 2844
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38

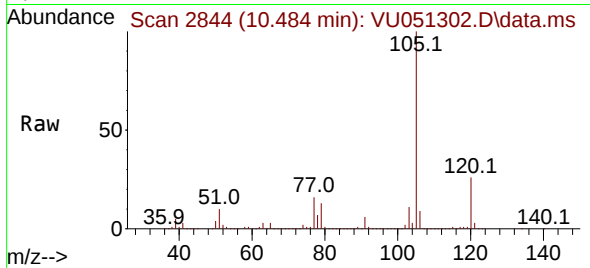



Tgt Ion:105 Resp: 1754430
Ion Ratio Lower Upper
105 100
120 26.1 20.6 30.8
77 16.4 13.5 20.3

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

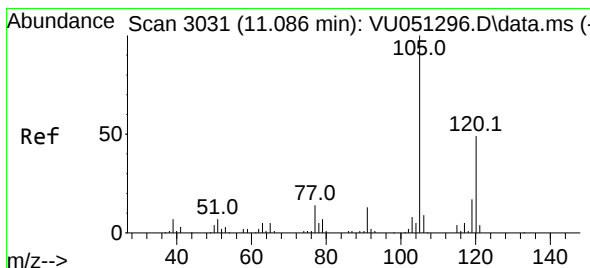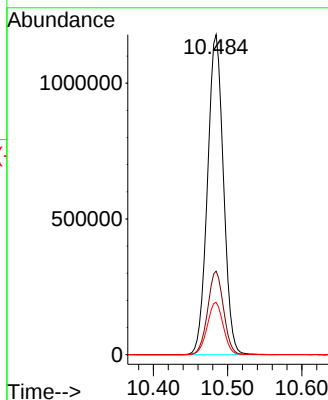

#62
1,3,5-Trimethylbenzene
Concen: 21.728 ug/L
RT: 11.086 min Scan# 3031
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02


Tgt Ion:105 Resp: 488220
Ion Ratio Lower Upper
105 100
120 47.7 37.7 56.5

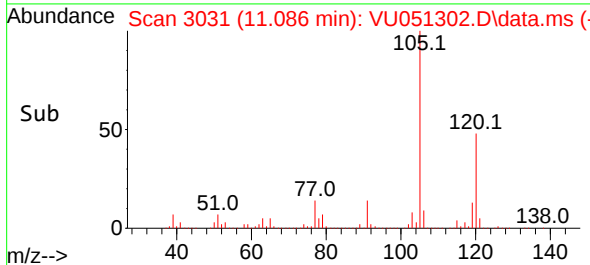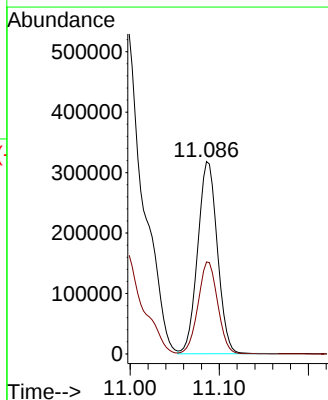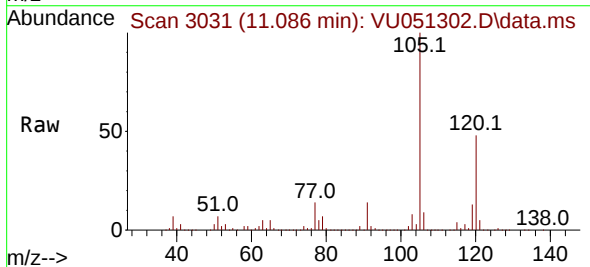

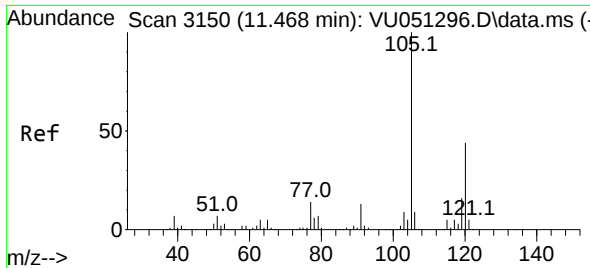

#63
1,2,4-Trimethylbenzene
Concen: 36.534 ug/L
RT: 11.465 min Scan# 3150
Delta R.T. -0.003 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02



Instrument :
MSVOA_U
ClientSampleId :
BHA38

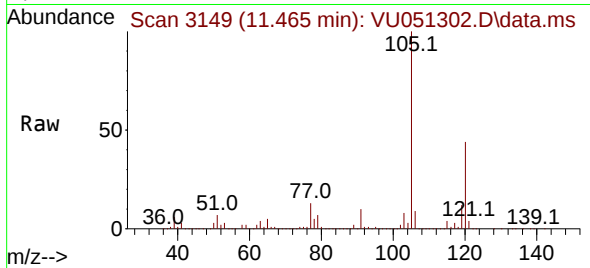

Tgt Ion:105 Resp: 232154
Ion Ratio Lower Upper
105 100
120 44.4 35.6 53.4


Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022

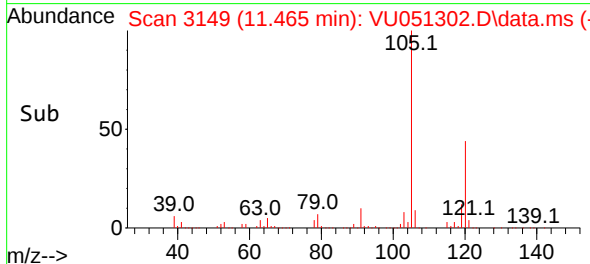


10/10/2022
Supervised By :Mahesh
Dadoda



10/11/2022

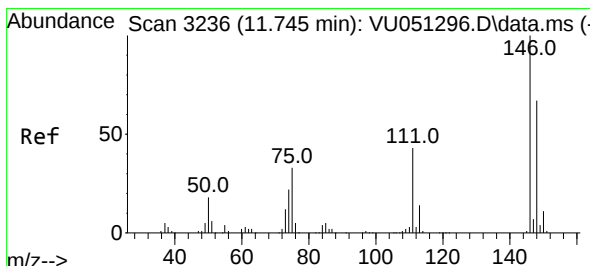


#64
1,3-Dichlorobenzene
Concen: 1.051 ug/L
RT: 11.745 min Scan# 3236
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

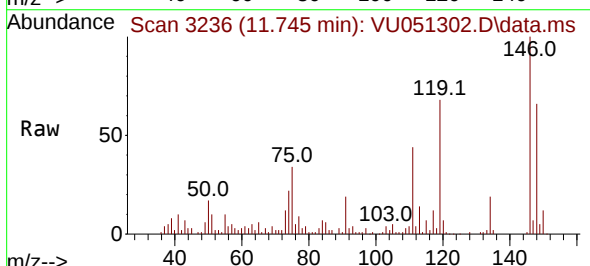


Tgt Ion:146 Resp: 44039
Ion Ratio Lower Upper
146 100
111 43.7 28.3 52.7
148 66.3 43.8 81.4

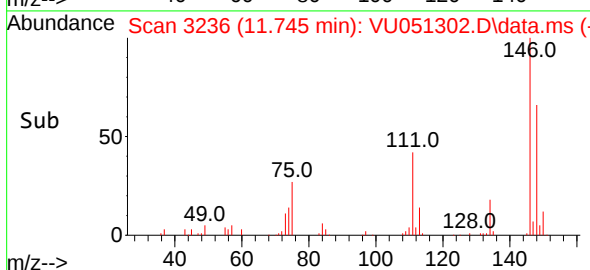

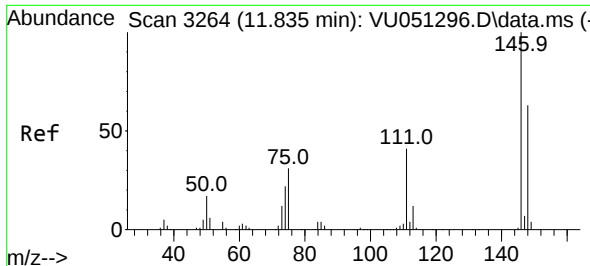

#65
1,4-Dichlorobenzene
Concen: 5.398 ug/L
RT: 11.835 min Scan# 3264
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02

Instrument :
MSVOA_U
ClientSampleId :
BHA38

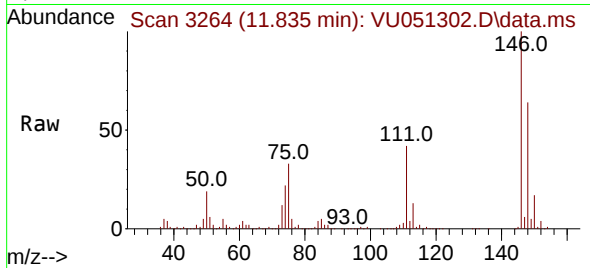




Tgt Ion:146 Resp: 222899
Ion Ratio Lower Upper
146 100
111 41.6 29.1 54.1
148 63.8 44.2 82.0

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022




10/10/2022
Supervised By :Mahesh
Dadoda


10/11/2022

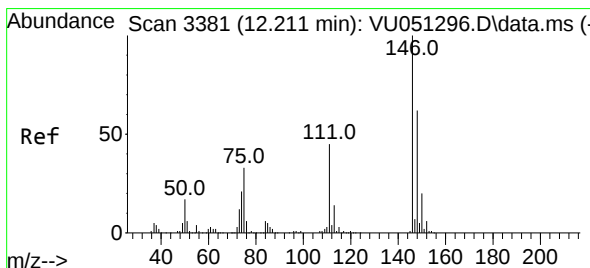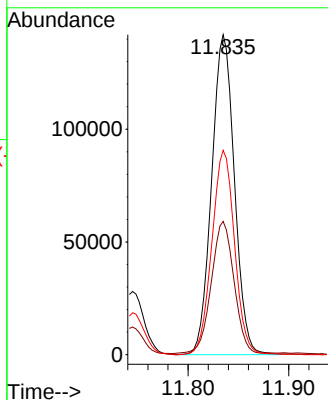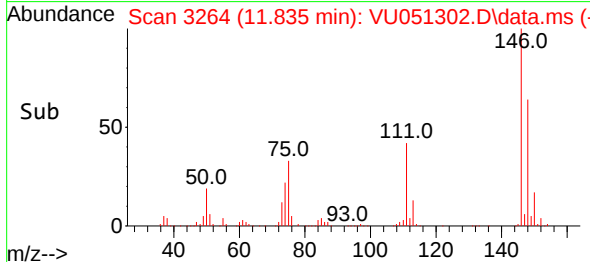

#67
1,2-Dichlorobenzene
Concen: 6.888 ug/L
RT: 12.211 min Scan# 3381
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02


Tgt Ion:146 Resp: 280568
Ion Ratio Lower Upper
146 100
111 44.3 35.5 53.3
148 65.3 50.9 76.3

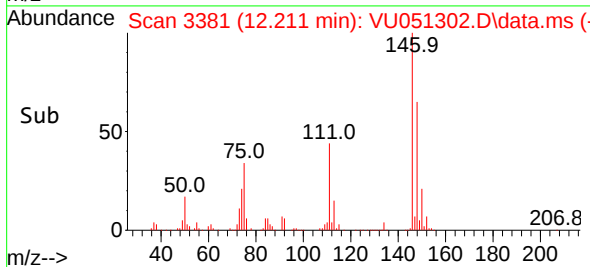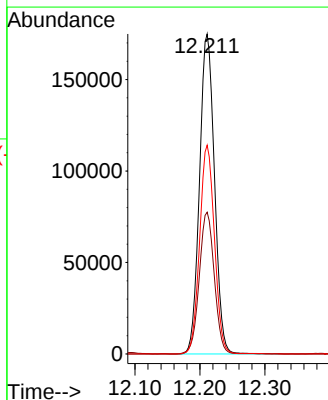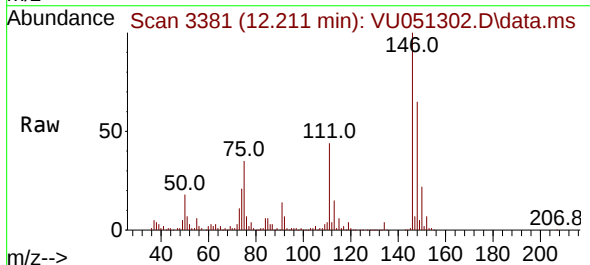

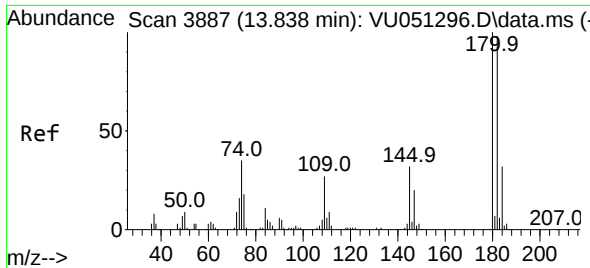

#70
1,2,4-trichlorobenzene
Concen: 0.299 ug/L
RT: 13.838 min Scan# 3887
Delta R.T. -0.000 min
Lab File: VU051302.D
Acq: 09 Oct 2022 16:02



Instrument :
MSVOA_U
ClientSampleId :
BHA38

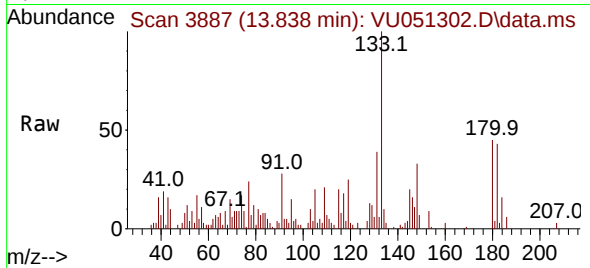

Tgt Ion:180 Resp: 6138
Ion Ratio Lower Upper
180 100
182 99.7 78.7 118.1
145 59.8 25.0 37.4

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/10/2022
Supervised By :Mahesh Dadoda 10/11/2022

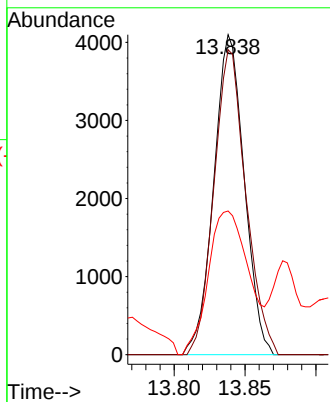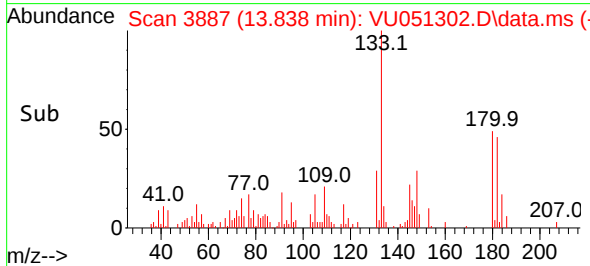

10/10/2022
Supervised By :Mahesh
Dadoda
10/11/2022