

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
 Data File : VU051312.D
 Acq On : 09 Oct 2022 20:10
 Operator : JC/MD
 Sample : N5064-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	12	16	27	rVB2	6237	8982	1.08%	0.132%
2	1.597	73	80	90	rBV	110784	126993	15.33%	1.869%
3	1.912	170	178	188	rBV	93964	119206	14.39%	1.755%
4	2.565	367	381	396	rBV	166540	273481	33.00%	4.025%
5	3.044	516	530	548	rVB2	31646	60719	7.33%	0.894%
6	3.186	560	574	588	rBV2	16090	37231	4.49%	0.548%
7	4.623	1005	1021	1059	rBV2	139855	371740	44.86%	5.472%
8	5.063	1140	1158	1177	rBV	159799	349811	42.22%	5.149%
9	5.726	1343	1364	1397	rBV2	310719	828627	100.00%	12.196%
10	6.250	1513	1527	1556	rBV	255948	490673	59.22%	7.222%
11	6.690	1650	1664	1689	rBV	203909	401341	48.43%	5.907%
12	7.565	1924	1936	1957	rBV	72769	131115	15.82%	1.930%
13	7.896	2026	2039	2054	rBV	357270	614279	74.13%	9.041%
14	7.970	2054	2062	2073	rVB	26864	45802	5.53%	0.674%
15	8.179	2116	2127	2145	rBV2	44376	77246	9.32%	1.137%
16	8.632	2256	2268	2302	rBV3	350276	788711	95.18%	11.609%
17	9.417	2498	2512	2541	rBV	375667	653624	78.88%	9.621%
18	9.690	2587	2597	2610	rBV3	12142	20044	2.42%	0.295%
19	10.755	2914	2928	2942	rBV	158100	254342	30.69%	3.744%
20	11.812	3244	3257	3274	rBV	351475	572914	69.14%	8.433%
21	12.192	3361	3375	3393	rBV	349602	567127	68.44%	8.347%




Sum of corrected areas: 6794008

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
Data File : VU051312.D
Acq On : 09 Oct 2022 20:10
Operator : JC/MD
Sample : N5064-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

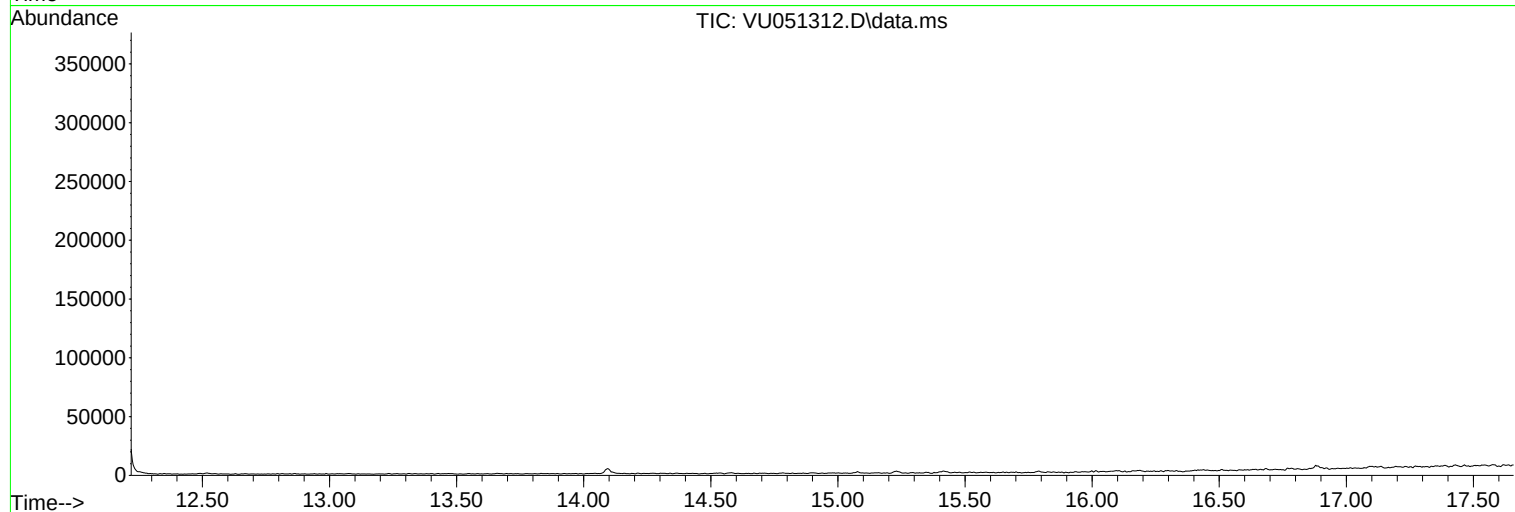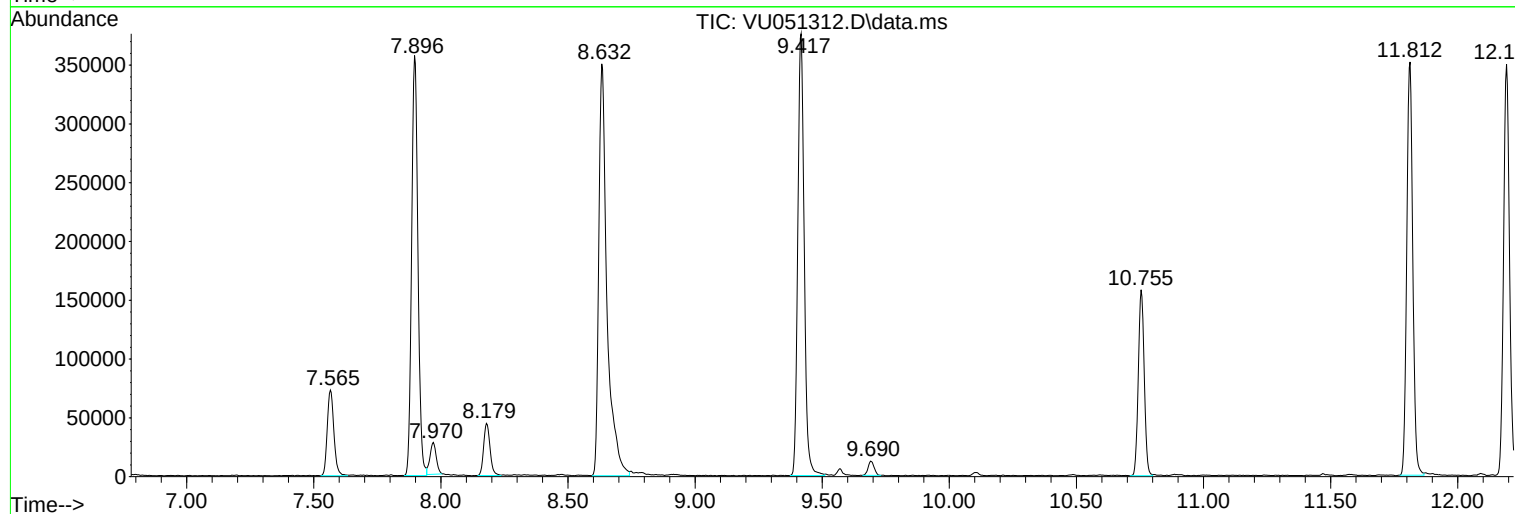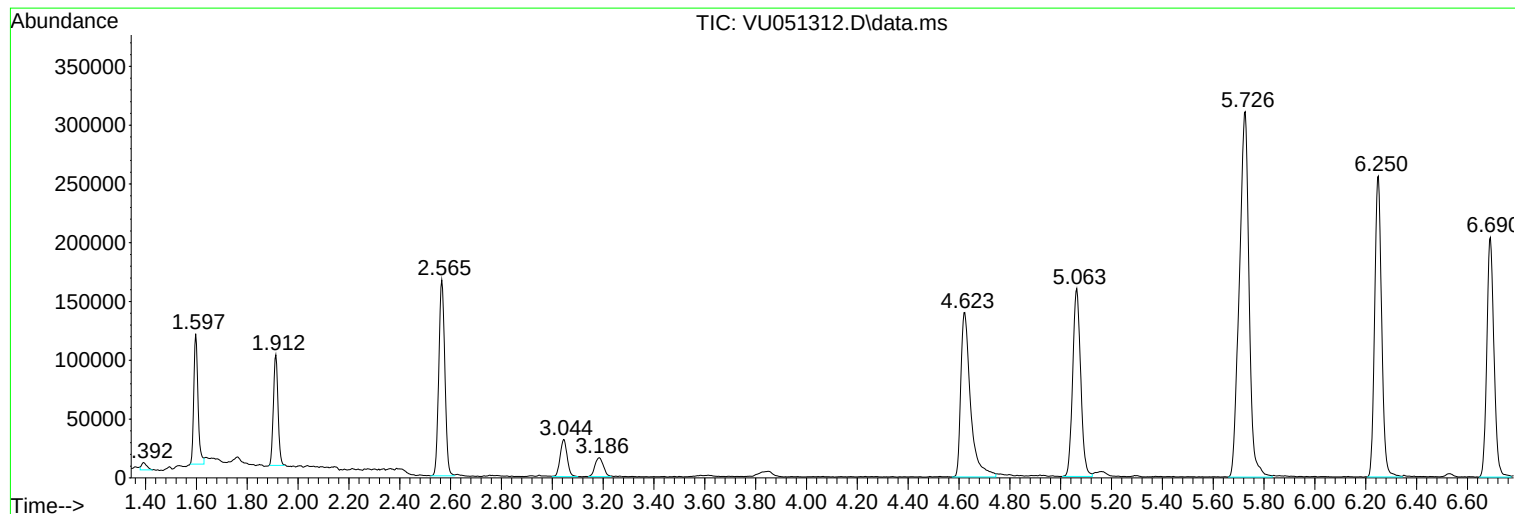

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
Data File : VU051312.D
Acq On : 09 Oct 2022 20:10
Operator : JC/MD
Sample : N5064-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
Data File : VU051312.D
Acq On : 09 Oct 2022 20:10
Operator : JC/MD
Sample : N5064-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc