


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100922\
 Data File : VU051295.D
 Acq On : 09 Oct 2022 12:04
 Operator : JC/MD
 Sample : BFB152
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB152

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 11 02:38:56 2022

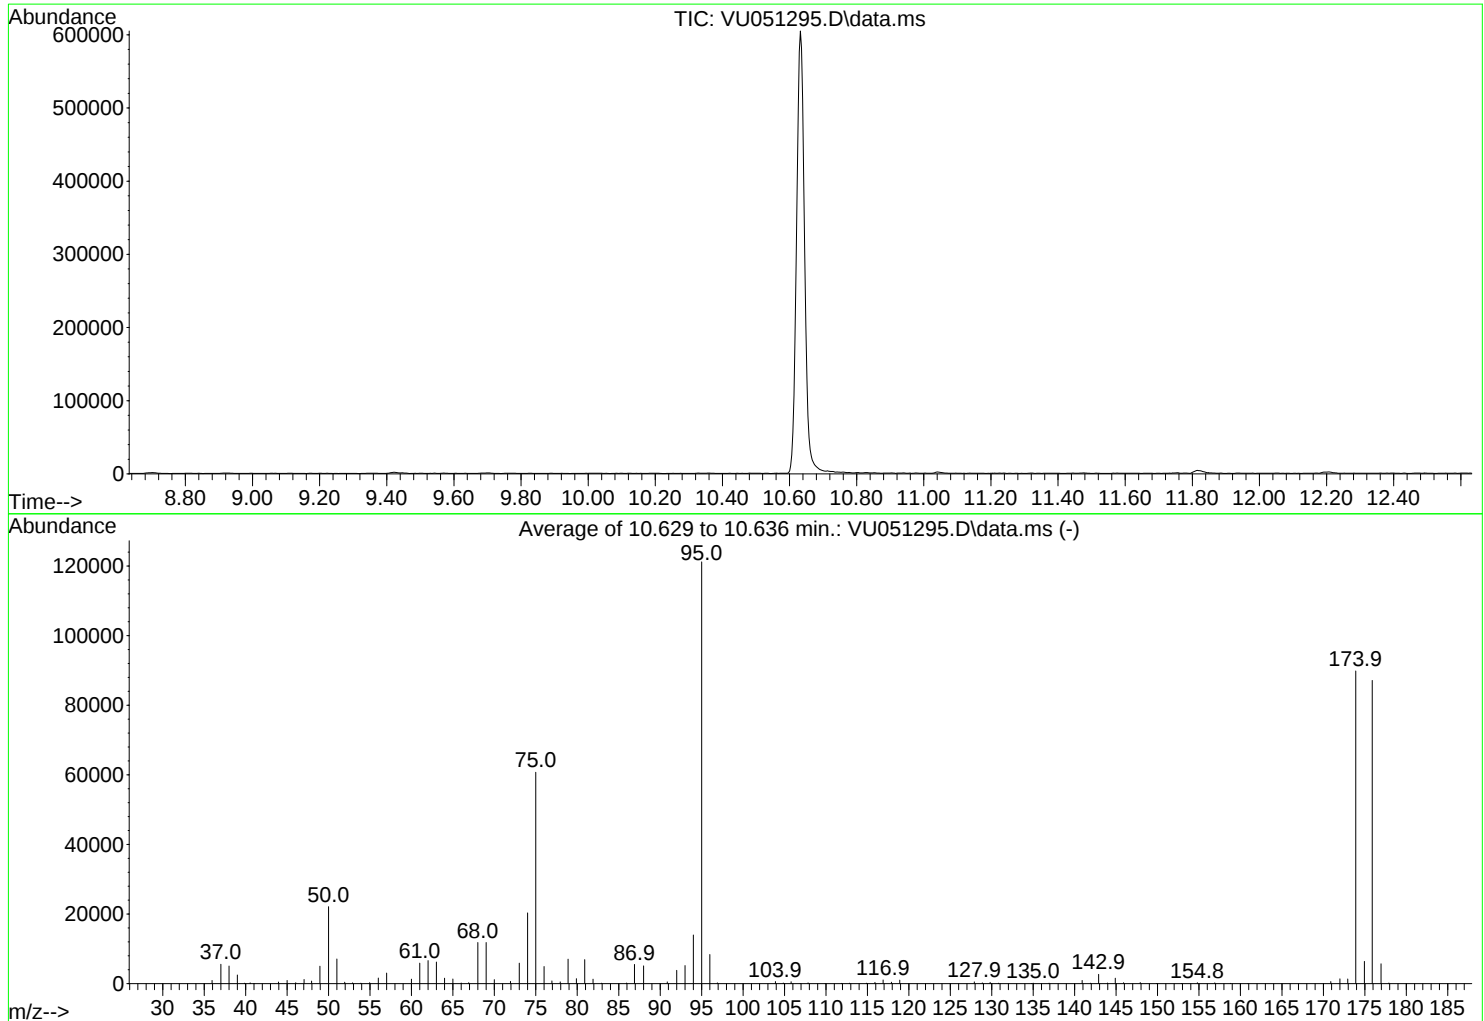

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	22115	PASS
75	95	30	80	50.1	60723	PASS
95	95	100	100	100.0	121211	PASS
96	95	5	9	6.9	8371	PASS
173	174	0.00	2	1.5	1351	PASS
174	95	50	120	74.1	89827	PASS
175	174	5	9	7.1	6377	PASS
176	174	95	101	97.0	87128	PASS
177	176	5	9	6.6	5720	PASS

m/z	Abundance
39.80	277.0
43.90	654.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
35.90	773.0
37.00	5615.0
38.00	5110.0
39.00	2577.0
39.90	389.0
40.60	250.0
44.00	1001.0
45.00	930.0
46.00	258.0
47.00	1219.0
48.00	767.0
48.90	4673.0
50.00	22128.0
51.00	7066.0
52.00	407.0
52.90	241.0
53.90	152.0
55.00	302.0
56.00	1665.0
57.00	3066.0
60.00	1350.0
61.00	5754.0
62.00	6694.0
63.00	6379.0
64.00	1664.0
65.00	1369.0
66.00	216.0
66.80	259.0
68.00	11912.0
69.00	11718.0
70.00	1190.0
72.00	657.0
73.00	5653.0
74.00	20096.0
75.00	59816.0
76.00	4937.0
76.90	765.0
77.90	503.0
78.90	6763.0
79.90	1387.0
80.90	6803.0
81.90	1086.0
83.00	146.0
86.00	171.0
86.90	5417.0
88.00	4938.0
90.90	491.0
92.00	3639.0
93.00	5191.0
94.00	13521.0
95.00	119360.0
96.00	8496.0
96.90	300.0
103.90	565.0
104.80	210.0
105.80	577.0
106.90	107.0
108.00	205.0
111.90	141.0
112.80	116.0
114.90	131.0
115.90	366.0
116.90	944.0
117.90	360.0
118.90	1031.0
127.90	513.0
128.80	201.0
129.80	385.0
130.80	119.0
134.80	168.0
136.90	154.0
140.90	908.0
141.90	149.0
142.90	2598.0
144.00	222.0
144.90	1595.0
145.90	263.0
147.90	285.0
154.80	278.0
156.90	239.0
160.90	115.0
170.90	609.0
172.00	1274.0
172.90	1413.0
173.90	86064.0
174.90	6232.0
175.90	84968.0
176.90	5560.0
177.90	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
36.00	925.0
37.00	5764.0
38.00	5242.0
39.00	2553.0
39.90	411.0
40.60	267.0
44.00	1160.0
45.00	944.0
46.10	299.0
47.10	1210.0
47.90	712.0
49.00	5143.0
50.00	22768.0
51.00	7290.0
52.00	410.0
52.90	269.0
53.90	124.0
55.00	255.0
56.00	1661.0
57.00	3120.0
60.00	1345.0
61.00	6079.0
62.00	6857.0
63.00	6410.0
64.00	1645.0
65.00	1404.0
66.00	178.0
66.90	289.0
68.00	12120.0
69.00	12126.0
70.00	1190.0
72.00	680.0
73.00	6033.0
74.00	20992.0
75.00	62688.0
76.00	5043.0
77.00	783.0
77.90	522.0
78.90	7275.0
79.90	1459.0
80.90	7104.0
81.90	1330.0
83.00	180.0
85.90	173.0
86.90	5768.0
88.00	5243.0
90.90	513.0
92.00	3905.0
93.00	5374.0
94.00	14397.0
95.00	124936.0
96.00	8665.0
96.90	240.0
103.90	595.0
104.90	201.0
105.80	577.0
106.90	102.0
107.80	251.0
109.90	108.0
111.90	116.0
112.80	163.0
114.90	116.0
115.90	353.0
116.90	1064.0
117.90	415.0
118.90	1028.0
127.90	532.0
128.80	248.0
129.80	384.0
130.80	110.0
135.00	208.0
136.90	163.0
140.90	940.0
141.90	171.0
142.90	2753.0
143.90	196.0
144.90	1586.0
145.90	277.0
147.90	319.0
149.90	101.0
154.80	296.0
156.90	250.0
158.80	125.0
170.90	583.0
172.00	1427.0
173.00	1353.0
173.90	92456.0
174.90	6431.0
175.90	89464.0
177.00	6013.0
177.90	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
36.00	1001.0
37.00	5293.0
38.00	4790.0
39.00	2291.0
39.90	395.0
40.50	246.0
41.00	133.0
44.00	1248.0
45.00	897.0
46.10	298.0
47.10	1190.0
47.90	681.0
49.00	5243.0
50.00	21448.0
51.00	6850.0
51.90	395.0
52.90	238.0
53.90	145.0
54.90	231.0
56.00	1539.0
57.00	2950.0
60.00	1190.0
61.00	5896.0
62.00	6378.0
63.00	5777.0
64.00	1452.0
65.00	1304.0
66.00	136.0
67.00	343.0
68.00	11428.0
69.00	11595.0
70.00	1028.0
71.90	595.0
73.00	5923.0
74.00	19920.0
75.00	59664.0
76.00	4795.0
77.00	864.0
78.00	544.0
78.90	7036.0
79.90	1446.0
80.90	6828.0
81.90	1458.0
82.90	152.0
85.90	171.0
86.90	5354.0
88.00	5170.0
90.80	517.0
92.00	3869.0
93.00	5052.0
94.00	13976.0
95.00	119336.0
96.00	7953.0
96.90	210.0
103.90	579.0
104.90	164.0
105.80	539.0
107.80	273.0
109.90	103.0
112.90	161.0
114.90	119.0
115.90	376.0
116.90	1115.0
117.90	474.0
118.90	968.0
127.90	531.0
128.90	226.0
129.80	346.0
130.80	135.0
135.00	213.0
136.90	122.0
140.90	885.0
141.90	152.0
142.90	2683.0
143.90	176.0
144.90	1495.0
145.90	267.0
147.90	312.0
152.90	105.0
154.80	295.0
156.90	244.0
158.80	141.0
170.90	579.0
172.00	1499.0
173.00	1287.0
173.90	90960.0
175.00	6467.0
175.90	86952.0
177.00	5586.0
177.90	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152