




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055701.D
 Acq On : 09 Oct 2023 15:15
 Operator : MD/SY
 Sample : 04744-01RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH578RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/10/2023
 Supervised By :Mahesh Dadoda 10/11/2023

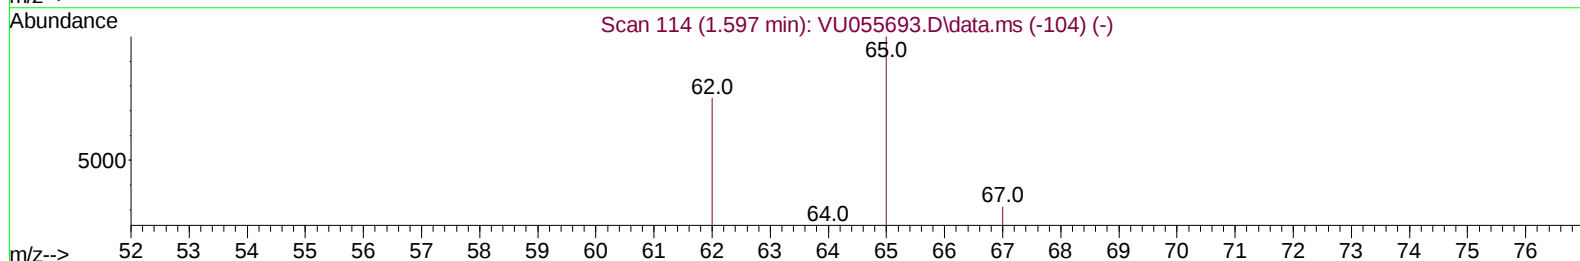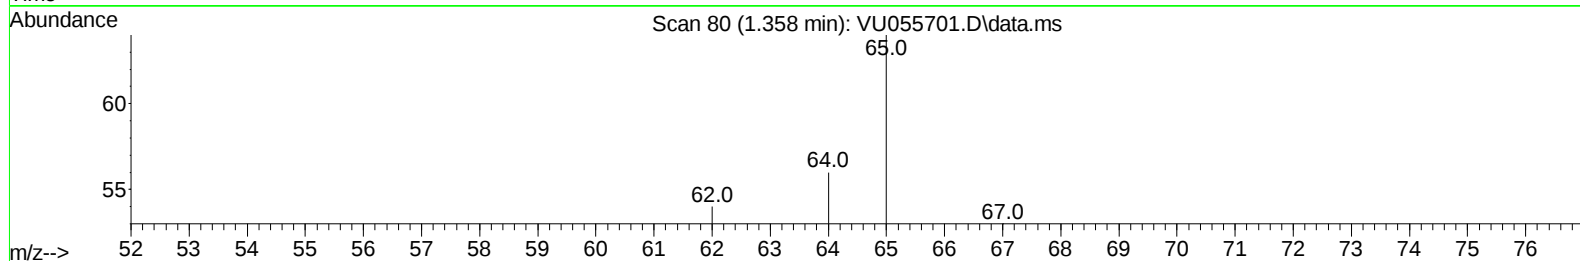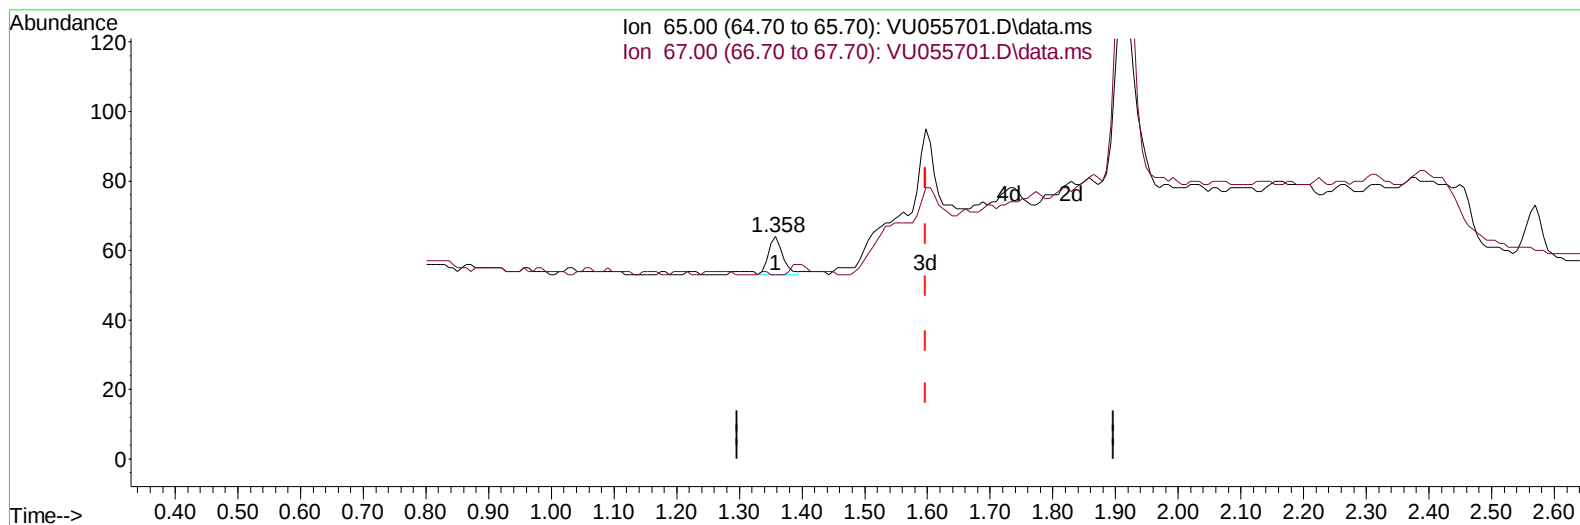

TIC: VU055701.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.358min (-0.239) 0.00 ug/L

response 17

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	35.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055701.D
 Acq On : 09 Oct 2023 15:15
 Operator : MD/SY
 Sample : 04744-01RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH578RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/10/2023
 Supervised By :Mahesh Dadoda 10/11/2023

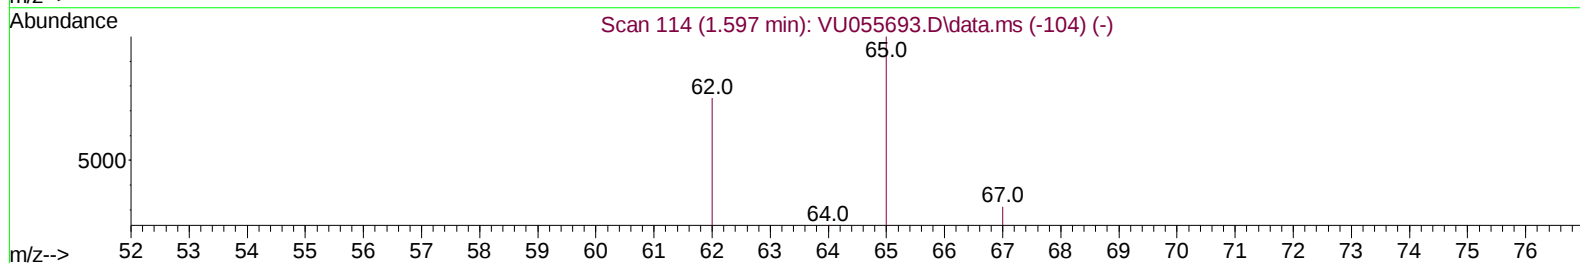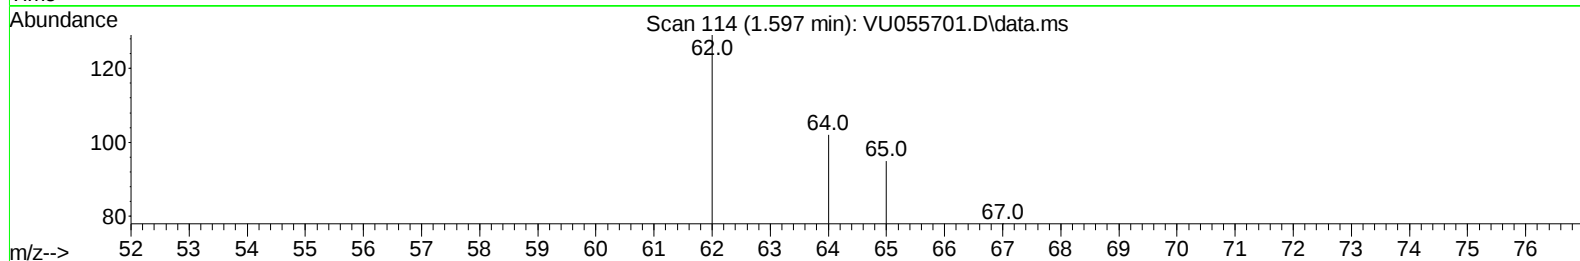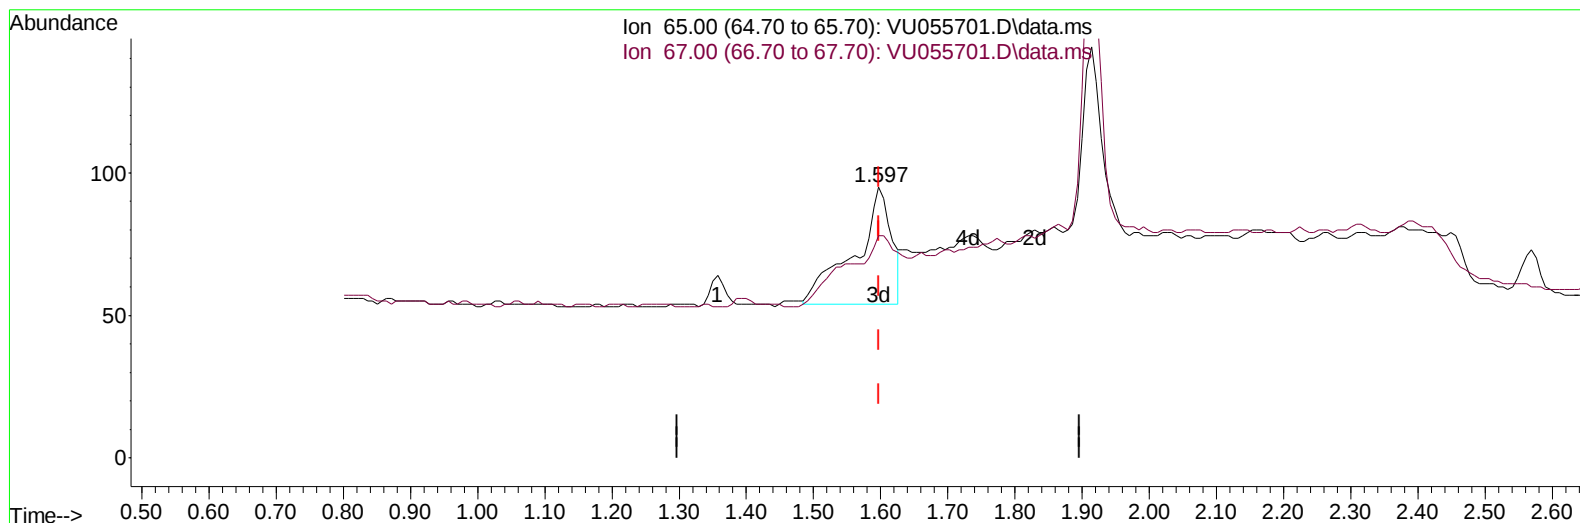

TIC: VU055701.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.597min (+ 0.000) 0.01 ug/L m

response 155

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	3.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055701.D
 Acq On : 09 Oct 2023 15:15
 Operator : MD/SY
 Sample : 04744-01RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH578RE

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 10/10/2023
 Supervised By : Mahesh Dadoda 10/11/2023

Quant Time: Oct 10 01:31:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	10241	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	17999	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	5516	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	155m	0.010	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	2.000%#	
4) 1,2-Dichloroethane-d4	5.685	65	7105	0.546	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	110.000%	
7) 1,2-Dichloropropane-d6	6.687	67	7787	0.462	ug/L	0.00
Spiked Amount	0.500	Range 60 - 140	Recovery	=	92.000%	
8) Toluene-d8	7.903	98	221	0.006	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	2.000%#	
10) 1,1,2,2-Tetrachloroeth...	10.745	84	6151	0.489	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	98.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
Data File : VU055701.D
Acq On : 09 Oct 2023 15:15
Operator : MD/SY
Sample : 04744-01RE
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH578RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 10 01:10:06 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/10/2023
Supervised By :Mahesh Dadoda 10/11/2023

