




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055703.D
 Acq On : 09 Oct 2023 16:04
 Operator : MD/SY
 Sample : 04744-03RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH580RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

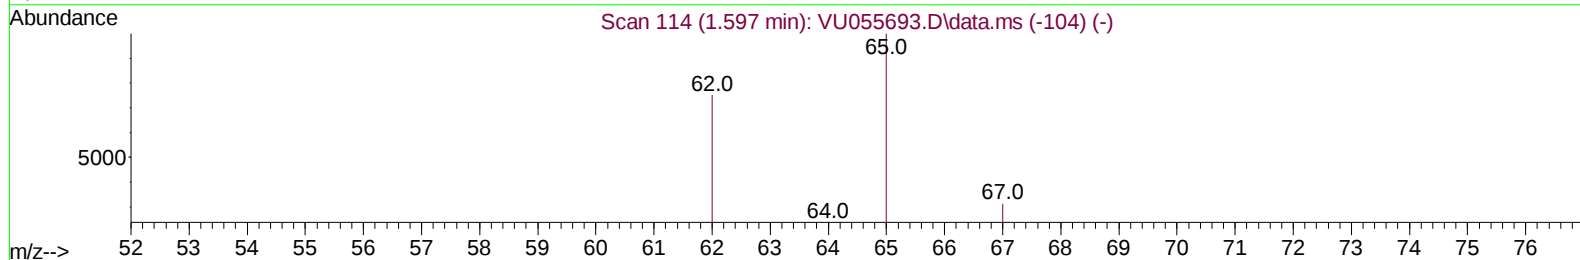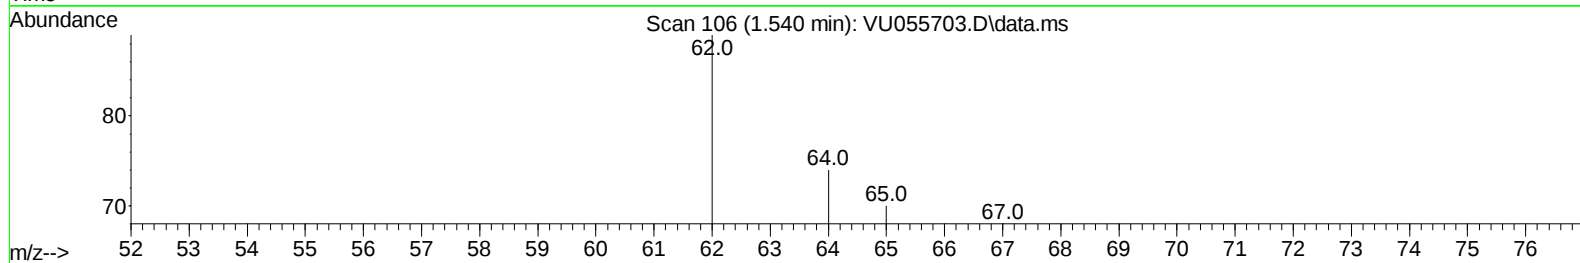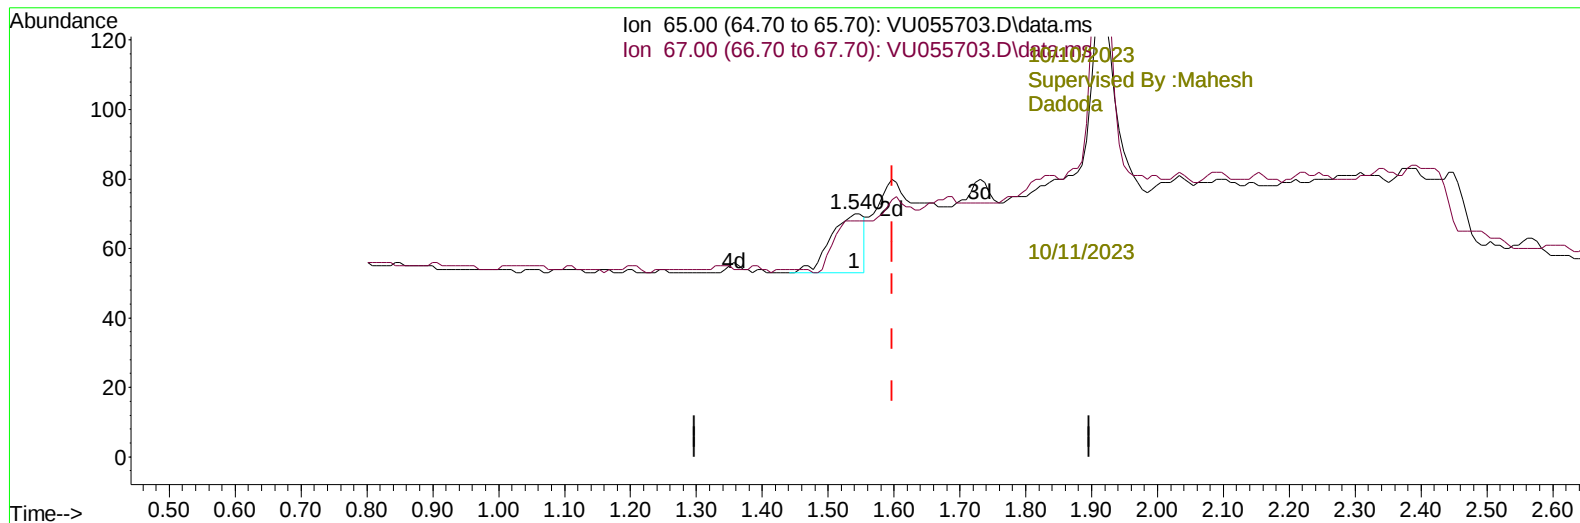

TIC: VU055703.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.540min (-0.057) 0.00 ug/L

response 60

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	28.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055703.D
 Acq On : 09 Oct 2023 16:04
 Operator : MD/SY
 Sample : 04744-03RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH580RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

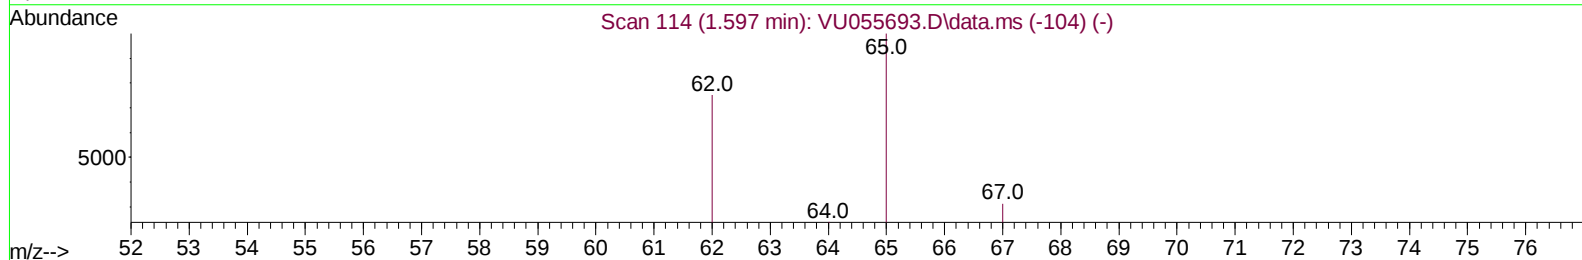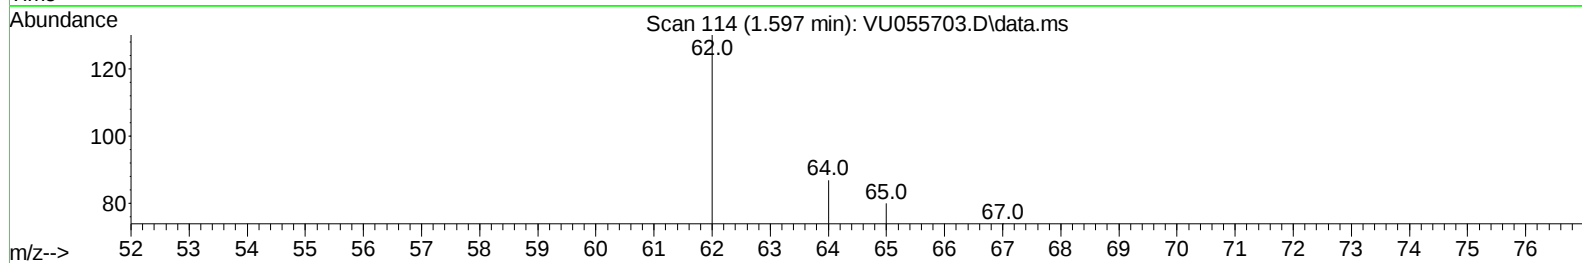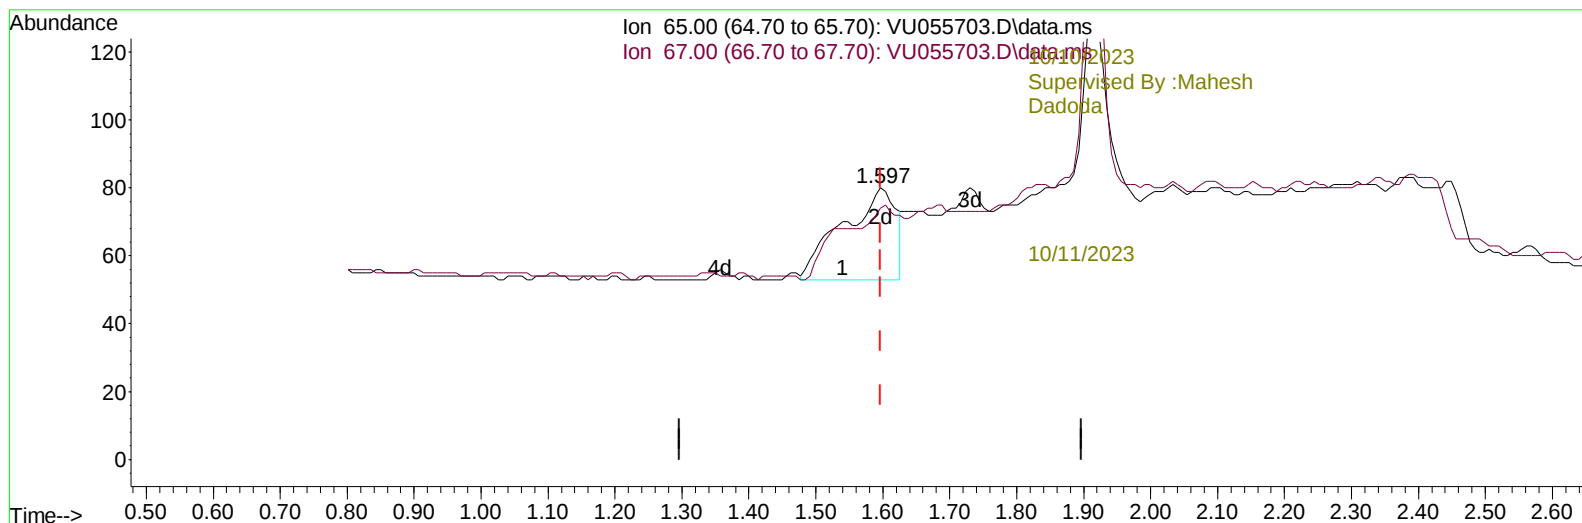

TIC: VU055703.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.597min (-0.000) 0.01 ug/L m

response 149

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	11.41#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
 Data File : VU055703.D
 Acq On : 09 Oct 2023 16:04
 Operator : MD/SY
 Sample : 04744-03RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH580RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 10 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----10/10/2023							
Internal Standards							
1) 1,4-Difluorobenzene	6.258	114		8672	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117		14433	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152		4209	0.500	ug/L	0.00
System Monitoring Compounds							
2) Vinyl Chloride-d3	1.597	65		149m	0.011	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	2.000%#	
4) 1,2-Dichloroethane-d4	5.685	65		6797	0.617	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	124.000%	
7) 1,2-Dichloropropane-d6	6.687	67		7207	0.533	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%	
8) Toluene-d8	7.903	98		87	0.003	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	0.000%#	
10) 1,1,2,2-Tetrachloroeth...	10.745	84		5961	0.591	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	118.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
Data File : VU055703.D
Acq On : 09 Oct 2023 16:04
Operator : MD/SY
Sample : 04744-03RE
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH580RE

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 10 01:10:06 2023
Response via : Initial Calibration

Reviewed By :John
Carlone

