
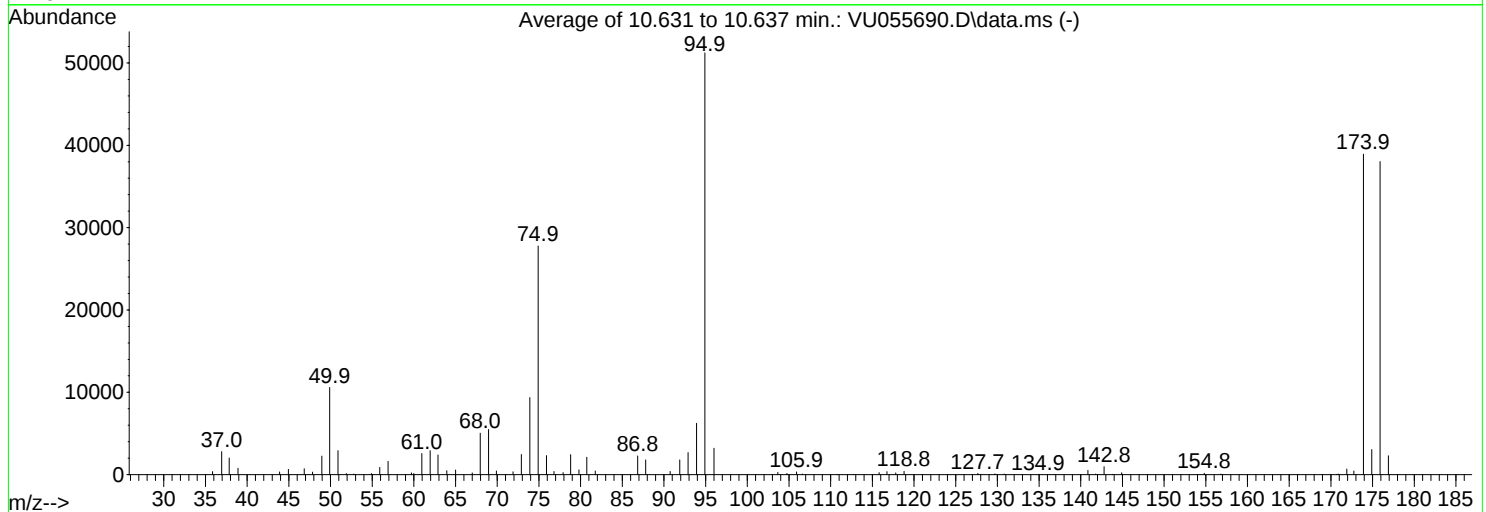


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100923\
Data File : VU055690.D
Acq On : 09 Oct 2023 09:12
Operator : MD/SY
Sample : BFB042
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB042

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100923.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 10 01:10:06 2023

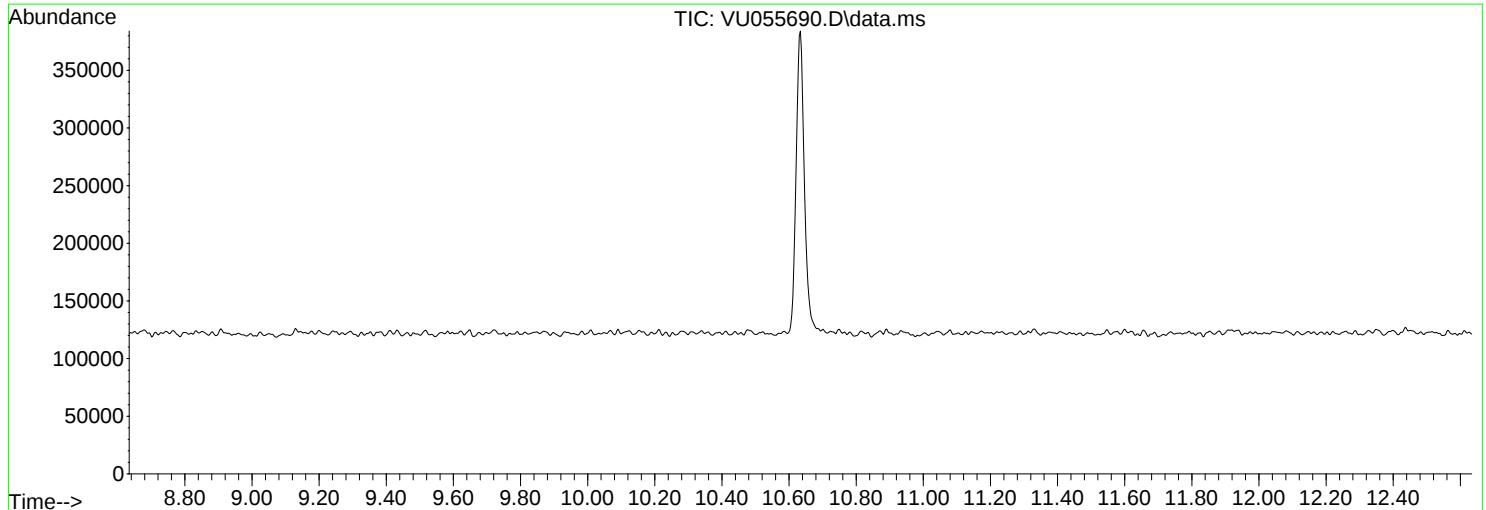

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	10582	PASS
75	95	30	80	54.2	27760	PASS
95	95	100	100	100.0	51227	PASS
96	95	5	9	6.3	3210	PASS
173	174	0.00	2	1.1	447	PASS
174	95	50	120	76.0	38925	PASS
175	174	5	9	7.8	3047	PASS
176	174	95	101	97.7	38035	PASS
177	176	5	9	6.0	2301	PASS

m/z	Abundance
35.80	370.0
37.80	164.0
38.30	147.0
38.90	258.0
39.90	121680.0
44.00	531.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	811.0
36.90	2873.0
37.90	2345.0
38.90	1065.0
39.90	120408.0
43.90	898.0
44.90	695.0
46.90	747.0
47.90	310.0
48.90	2462.0
49.90	10858.0
50.90	3274.0
51.90	130.0
54.90	266.0
55.90	922.0
56.90	1750.0
60.00	434.0
60.90	2661.0
61.90	2901.0
62.90	2509.0
64.00	509.0
65.00	651.0
67.00	244.0
68.00	5149.0
68.90	5635.0
69.90	484.0
71.90	339.0
72.90	2585.0
73.90	9492.0
74.90	28504.0
75.90	2445.0
76.80	377.0
77.90	274.0
78.80	2344.0
79.80	500.0
80.70	2199.0
81.80	410.0
86.80	2430.0
87.80	1910.0
90.70	347.0
91.90	1710.0
92.90	2753.0
93.90	6586.0
94.90	51880.0
96.00	3356.0
103.70	180.0
104.70	162.0
105.80	392.0
106.60	110.0
110.80	129.0
115.80	273.0
116.70	368.0
117.70	201.0
118.80	380.0
127.70	140.0
136.80	110.0
140.90	621.0
142.80	947.0
143.80	126.0
144.90	246.0
154.90	171.0
156.80	131.0
170.70	110.0
171.90	680.0
172.80	485.0
173.90	39136.0
174.90	3252.0
175.90	37728.0
176.90	2274.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	719.0
37.00	2912.0
37.90	2176.0
38.90	998.0
39.90	121696.0
43.90	842.0
44.90	684.0
46.90	765.0
47.80	324.0
49.00	2321.0
49.90	10882.0
50.90	2956.0
51.90	159.0
52.80	112.0
54.90	169.0
55.90	914.0
56.90	1679.0
59.70	325.0
60.90	2604.0
62.00	2968.0
62.90	2451.0
63.90	535.0
65.00	555.0
67.00	245.0
68.00	5125.0
68.90	5629.0
69.90	439.0
71.90	356.0
72.90	2500.0
73.90	9698.0
74.90	28544.0
75.90	2380.0
76.80	404.0
77.90	242.0
78.80	2480.0
79.80	599.0
80.80	2165.0
81.80	438.0
86.80	2306.0
87.80	1829.0
90.70	423.0
91.90	1863.0
92.90	2784.0
93.90	6337.0
94.90	52936.0
96.00	3260.0
103.60	289.0
104.70	162.0
105.90	326.0
106.60	111.0
115.80	267.0
116.80	365.0
117.80	214.0
118.80	433.0
127.60	161.0
129.70	132.0
130.80	133.0
140.80	552.0
141.80	120.0
142.80	1051.0
144.90	244.0
154.80	196.0
156.80	119.0
170.90	121.0
171.90	718.0
172.70	448.0
173.90	40296.0
174.90	3137.0
175.90	39352.0
176.90	2431.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
36.00	689.0
36.90	2606.0
37.90	2008.0
39.00	1040.0
39.90	122872.0
43.90	827.0
45.00	533.0
46.80	649.0
47.80	307.0
49.00	1972.0
49.90	10005.0
50.90	2503.0
51.90	139.0
52.80	104.0
55.90	792.0
56.90	1438.0
59.70	340.0
61.00	2439.0
62.00	2864.0
62.90	2233.0
63.90	412.0
65.00	488.0
67.00	156.0
67.90	4814.0
69.00	5180.0
69.90	426.0
71.90	346.0
72.90	2238.0
73.90	8939.0
74.90	26232.0
75.90	2103.0
76.80	410.0
77.90	240.0
78.80	2437.0
79.80	660.0
80.80	2018.0
81.70	467.0
86.90	2085.0
87.80	1622.0
90.80	411.0
91.90	1814.0
92.90	2491.0
93.90	5816.0
94.90	48864.0
96.00	3013.0
103.60	366.0
104.80	128.0
106.00	264.0
112.70	106.0
115.80	201.0
116.80	353.0
117.90	240.0
118.80	434.0
127.60	157.0
128.00	113.0
129.70	155.0
130.80	114.0
134.90	106.0
140.90	431.0
141.80	107.0
142.80	946.0
144.90	214.0
154.70	174.0
170.90	111.0
171.90	666.0
172.80	408.0
173.90	37344.0
174.90	2753.0
175.90	37024.0
176.90	2199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042