

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U101018\
 Data File : VU027564.D
 Acq On : 10 Oct 2018 12:53
 Operator : MD/SY
 Sample : J5324-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 OILY-WATER

Quant Time: Oct 11 04:03:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 02 02:04:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	129508	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	212184	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	185061	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	85643	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	98865	45.72	ug/l	0.00
Spiked Amount			Recovery	=	91.44%	
35) Dibromofluoromethane	4.89	113	71206	48.97	ug/l	0.00
Spiked Amount			Recovery	=	97.94%	
50) Toluene-d8	7.57	98	267860	49.22	ug/l	0.00
Spiked Amount			Recovery	=	98.44%	
62) 4-Bromofluorobenzene	10.31	95	89838	44.42	ug/l	0.00
Spiked Amount			Recovery	=	88.84%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	2.83	59	2975	6.533	ug/l #	80
13) Acrolein	2.20	56	448	1.172	ug/l #	41
15) Acrylonitrile	2.95	53	368	0.310	ug/l #	82
16) Acetone	2.32	43	217558	170.292	ug/l	98
18) Methyl Acetate	2.45	43	14315	4.912	ug/l #	56
20) Methylene Chloride	2.70	84	969	0.545	ug/l #	80
25) 2-Butanone	4.27	43	27281	15.659	ug/l	100
30) Chloroform	4.68	83	4836	1.604	ug/l	94
31) Cyclohexane	4.99	56	2826	0.580	ug/l #	1
36) 1,1-Dichloropropene	4.99	75	11178	4.852	ug/l #	50
37) Ethyl Acetate	4.27	43	27281	9.162	ug/l #	70
38) Carbon Tetrachloride	4.99	117	12776	6.139	ug/l #	17
40) Benzene	5.40	78	1475	0.220	ug/l #	79
48) Methyl methacrylate	6.53	41	6852	2.980	ug/l #	46
51) 4-Methyl-2-Pentanone	7.47	43	4455	1.483	ug/l	91
52) Toluene	7.64	92	993	0.250	ug/l	100
56) Ethyl methacrylate	7.92	69	82	2.298	ug/l #	1
59) 2-Hexanone	8.37	43	5804	2.490	ug/l	98
76) 1,2,3-Trichloropropane	10.31	75	47825	21.542	ug/l #	37
81) trans-1,4-Dichloro-2-buten	10.31	75	47825	56.378	ug/l #	100
84) 1,2,4-Trimethylbenzene	11.15	105	1426	0.276	ug/l	81
86) p-Isopropyltoluene	11.48	119	5727	1.084	ug/l	95
89) n-Butylbenzene	11.89	91	520	2.039	ug/l #	73
95) Naphthalene	13.75	128	2612	2.050	ug/l #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101018\
Data File : VU027564.D
Acq On : 10 Oct 2018 12:53
Operator : MD/SY
Sample : J5324-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
OILY-WATER

Quant Time: Oct 11 04:03:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 02 02:04:34 2018
Response via : Initial Calibration

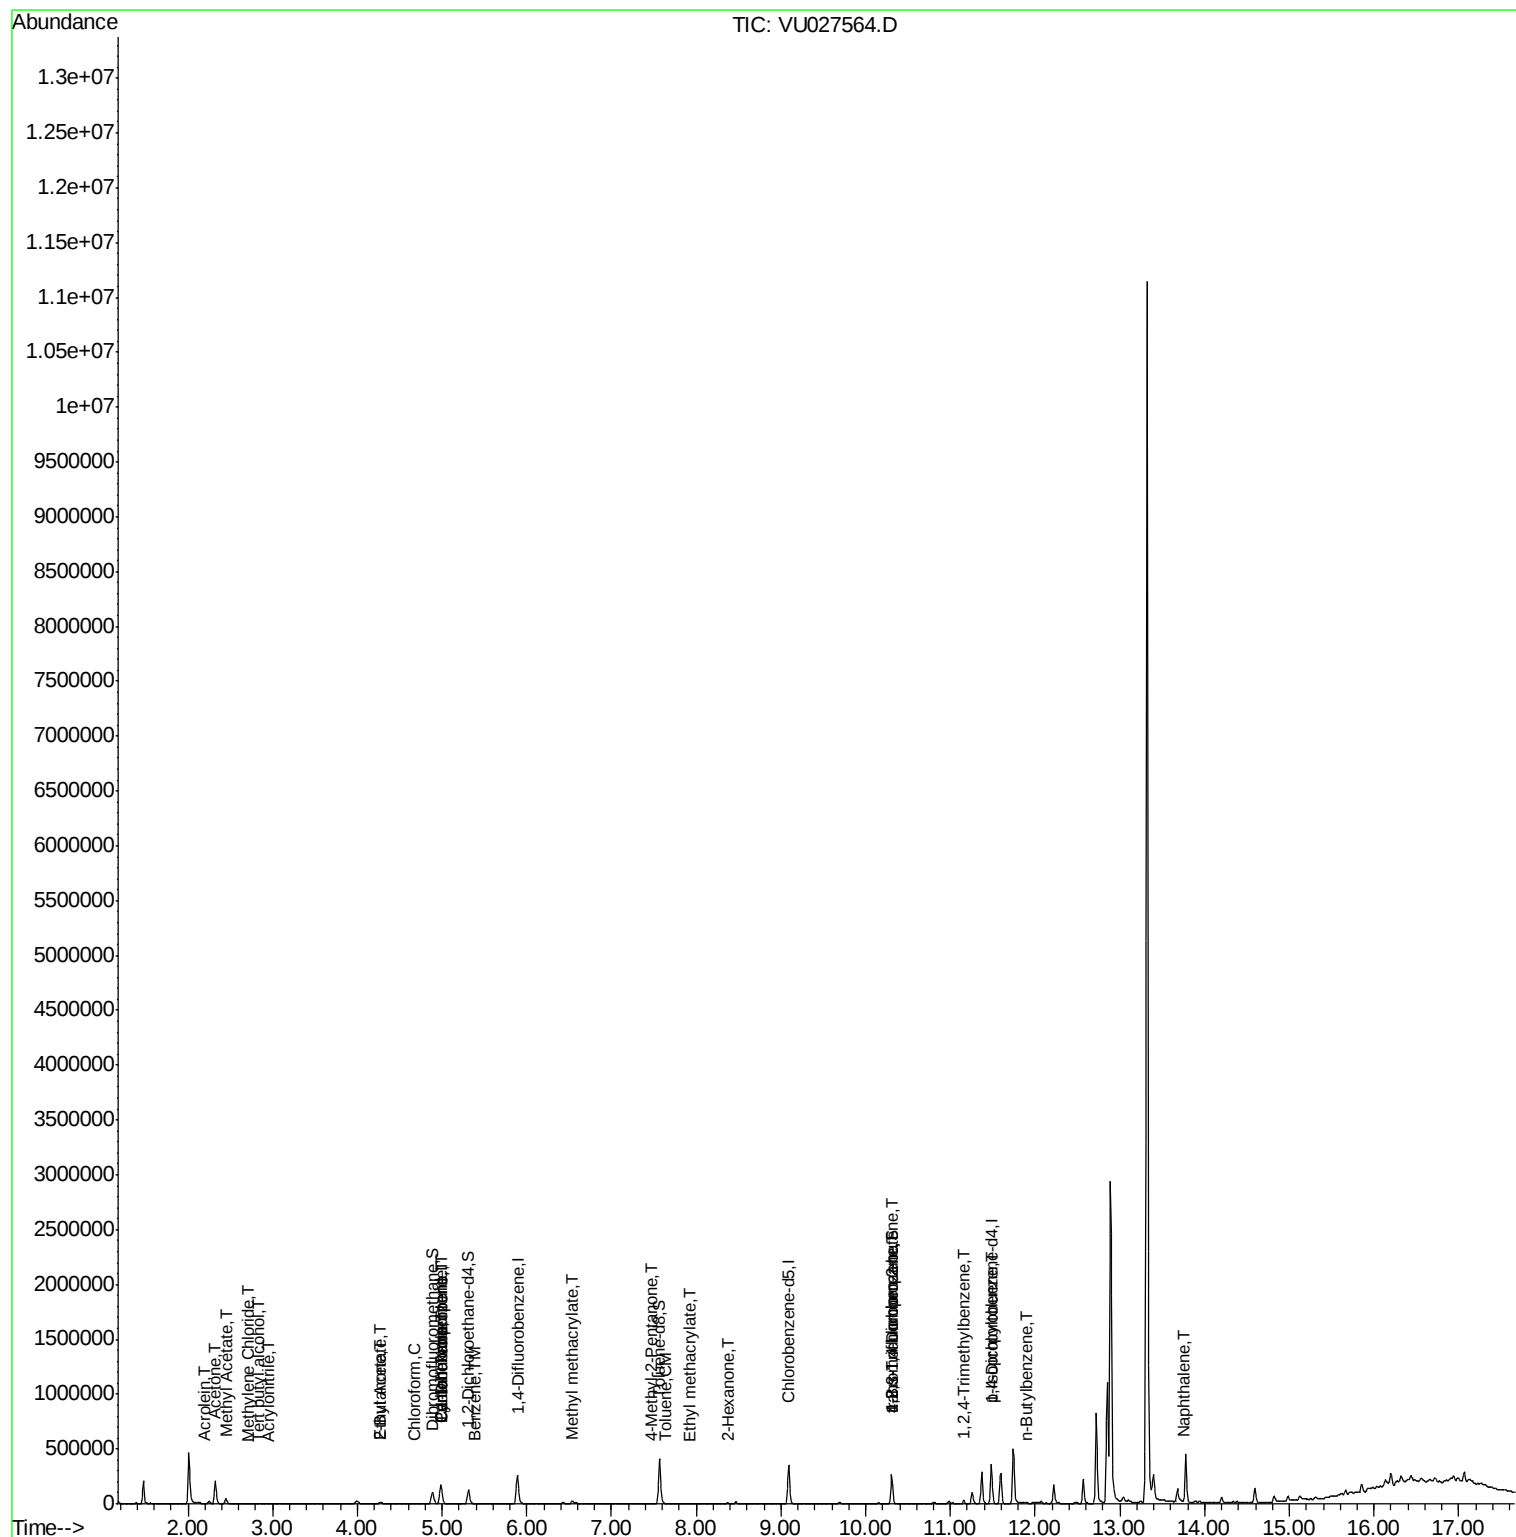



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion:168 Resp: 129508

Ion Ratio Lower Upper

168 100

99 60.9 50.8 76.2

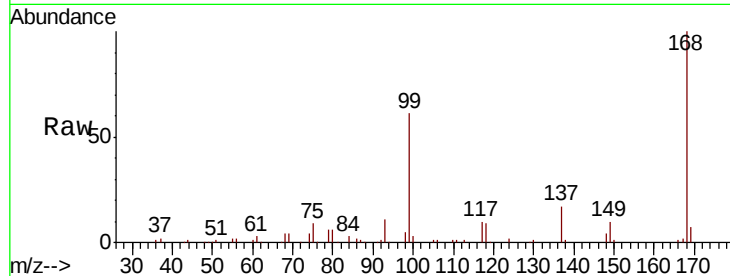

Abundance Ion 167.90 (167.60 to 168.60): VU027314.D (-1169) (-)

Ion 98.90 (98.60 to 99.60): VU027314.D (-1169) (-)

4.99

60000

50000

40000

30000



20000

10000

0

4.90 5.00 5.10 5.20

Time-->



#11

Tert butyl alcohol

Concen: 6.533 ug/l

RT: 2.83 min Scan# 516

Delta R.T. 0.01 min

Lab File: VU027564.D


Acq: 10 Oct 2018 12:53

Tgt Ion: 59 Resp: 2975

Ion Ratio Lower Upper

59 100

57 3.2 8.4 12.6#



Abundance Ion 59.00 (58.70 to 59.70): VU027314.D (-499) (-)

Ion 57.00 (56.70 to 57.70): VU027314.D (-499) (-)

2.83

1500


1000


500

0

2.80 2.85

Time-->



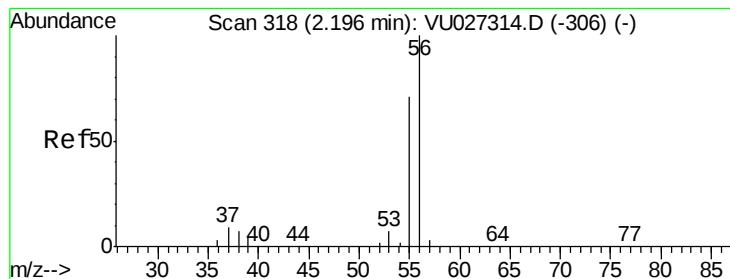

#13

Acrolein

Concen: 1.172 ug/l

RT: 2.20 min Scan# 318

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion: 56 Resp: 448

Ion Ratio Lower Upper

56 100

55 121.4 57.7 86.5#



Abundance Ion 56.00 (55.70 to 56.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

400

300



200

100

0

2.16 2.18 2.20 2.22

Time-->



#15

Acrylonitrile

Concen: 0.310 ug/l

RT: 2.95 min Scan# 554

Delta R.T. 0.02 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 53 Resp: 368

Ion Ratio Lower Upper

53 100

52 82.1 66.5 99.7

51 0.0 27.6 41.4#



Abundance Ion 53.00 (52.70 to 53.70): VU0

Ion 52.00 (51.70 to 52.70): VU0

Ion 51.00 (50.70 to 51.70): VU0

300

250

200

150


100


50

0

2.92 2.94 2.96 2.98

Time-->



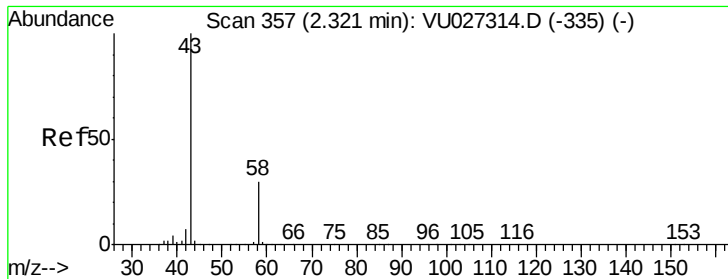

#16

Acetone

Concen: 170.292 ug/l

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :





OILY-WATER

Tgt Ion: 43 Resp: 217558

Ion Ratio Lower Upper

43 100

58 31.4 24.2 36.4

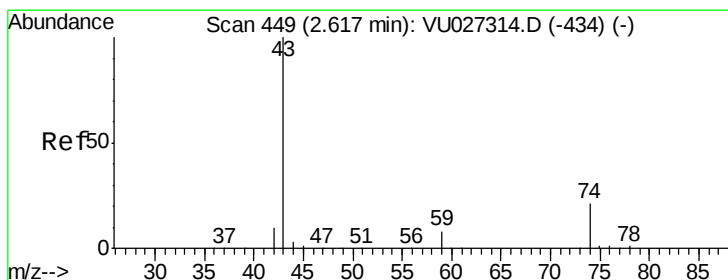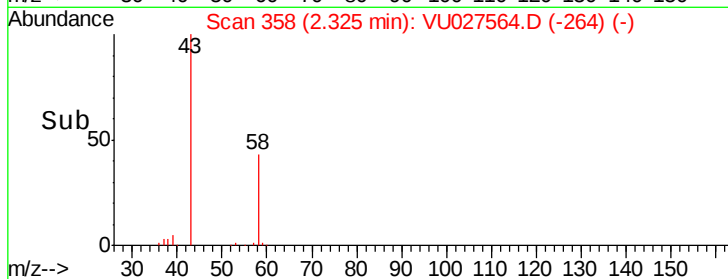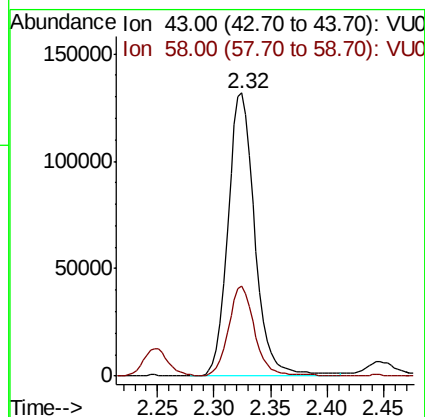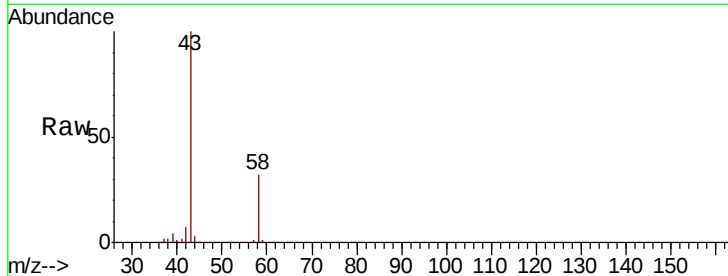

#18

Methyl Acetate

Concen: 4.912 ug/l

RT: 2.45 min Scan# 396

Delta R.T. -0.17 min

Lab File: VU027564.D




Acq: 10 Oct 2018 12:53


Tgt Ion: 43 Resp: 14315

Ion Ratio Lower Upper

43 100

74 0.0 16.5 24.7#


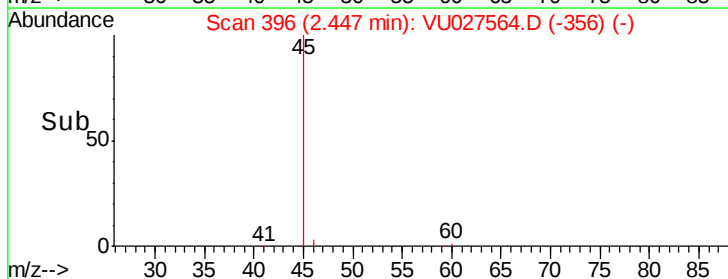
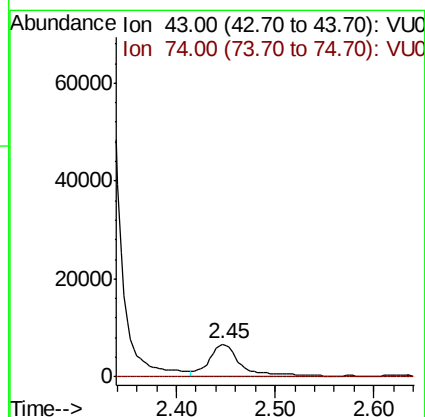
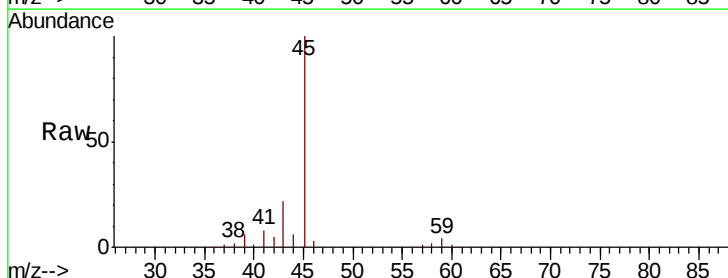


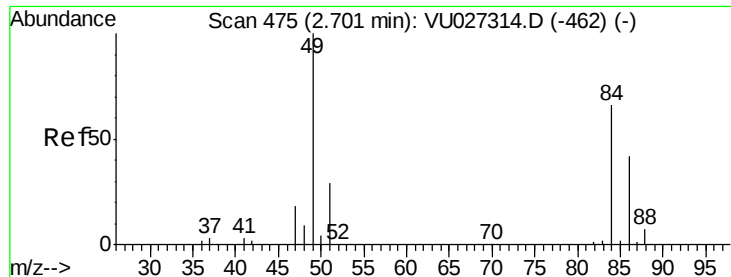

#20
Methylene Chloride
Concen: 0.545 ug/l
RT: 2.70 min Scan# 475
Delta R.T. 0.00 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53




Instrument :
MSVOA_U
ClientSampled :
OILY-WATER


Tgt Ion: 84 Resp: 969
Ion Ratio Lower Upper
84 100
49 114.7 120.5 180.7#
51 36.0 35.1 52.7
86 58.4 50.5 75.7

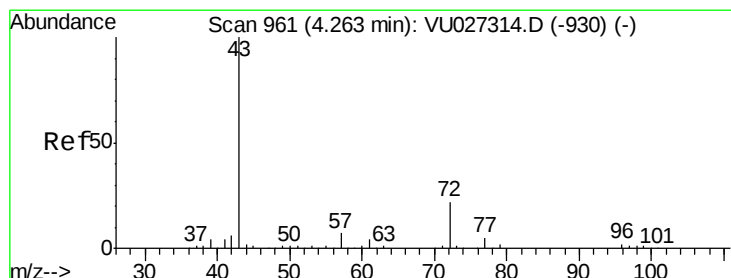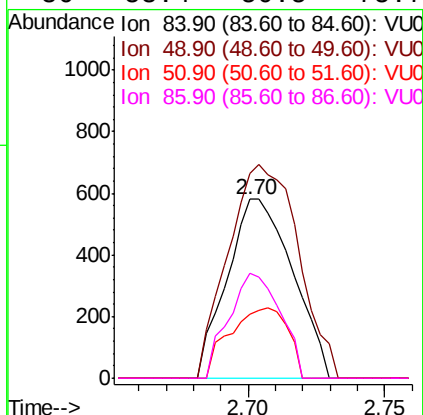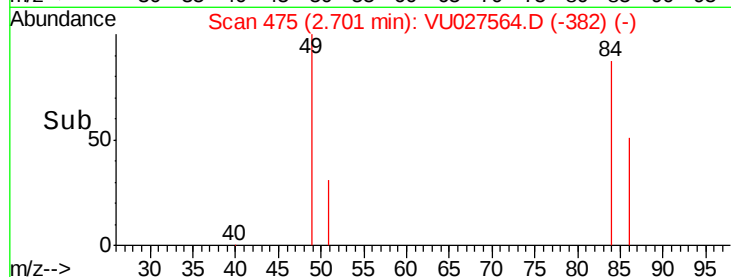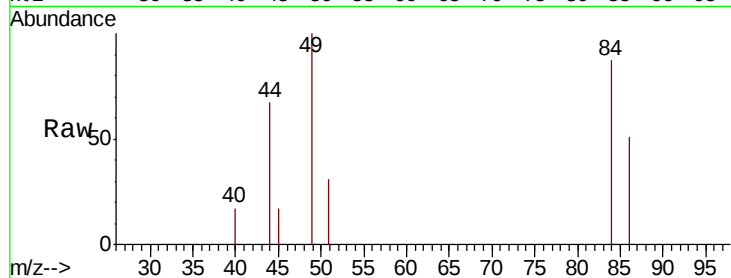

#25
2-Butanone
Concen: 15.659 ug/l
RT: 4.27 min Scan# 964
Delta R.T. 0.01 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Tgt Ion: 43 Resp: 27281
Ion Ratio Lower Upper
43 100
72 22.2 17.8 26.6

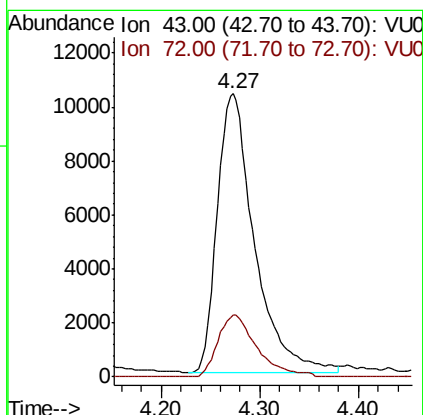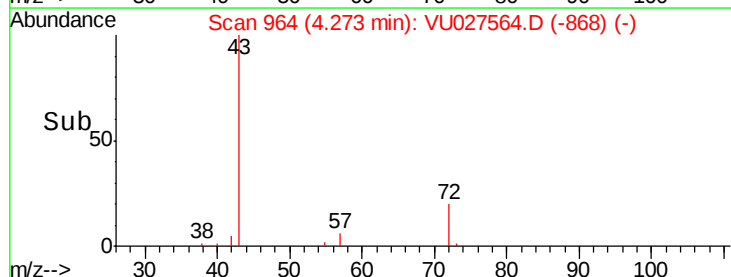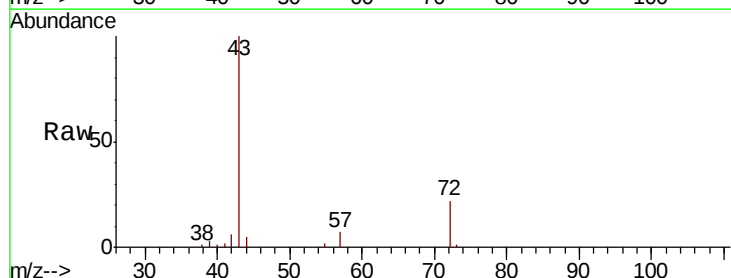



#30

Chloroform

Concen: 1.604 ug/l

RT: 4.68 min Scan# 1090

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion: 83 Resp: 4836

Ion Ratio Lower Upper




83 100

85 59.8 51.8 77.6

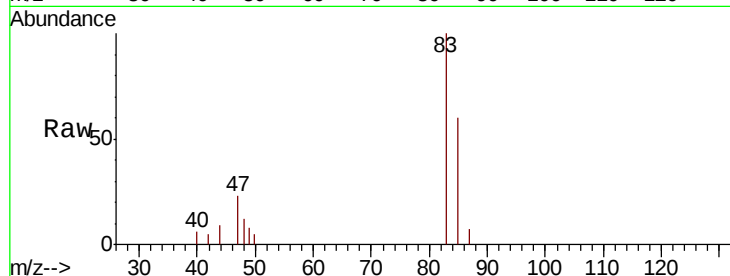

Abundance Ion 82.90 (82.60 to 83.60): VU0

Ion 84.90 (84.60 to 85.60): VU0

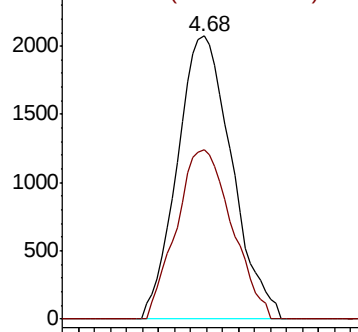

#31

Cyclohexane

Concen: 0.580 ug/l

RT: 4.99 min Scan# 1187

Delta R.T. -0.01 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 56 Resp: 2826

Ion Ratio Lower Upper

56 100

69 179.3 24.1 36.1#



84 126.1 59.1 88.7#




Abundance Ion 56.00 (55.70 to 56.70): VU0

Ion 69.00 (68.70 to 69.70): VU0

Ion 84.00 (83.70 to 84.70): VU0

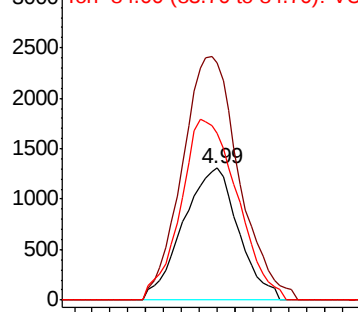

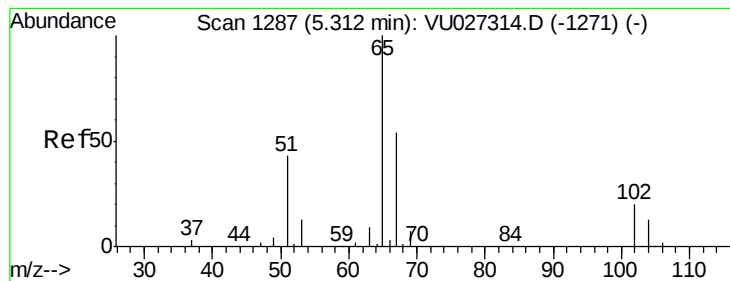

#33

1,2-Dichloroethane-d4

Concen: 45.717 ug/l

RT: 5.31 min Scan# 1287

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion: 65 Resp: 98865

Ion Ratio Lower Upper




65 100

67 53.4 0.0 107.8



Abundance Ion 64.90 (64.60 to 65.60): VU0

Ion 66.90 (66.60 to 67.60): VU0

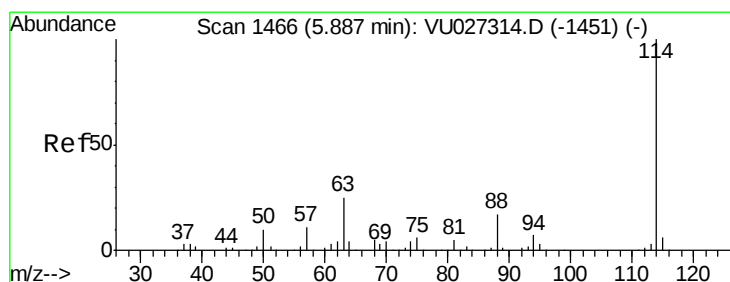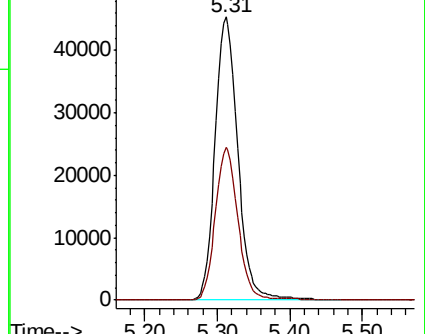

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.89 min Scan# 1467

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 114 Resp: 212184

Ion Ratio Lower Upper

114 100

63 25.4 0.0 50.2



88 17.1 0.0 33.8




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

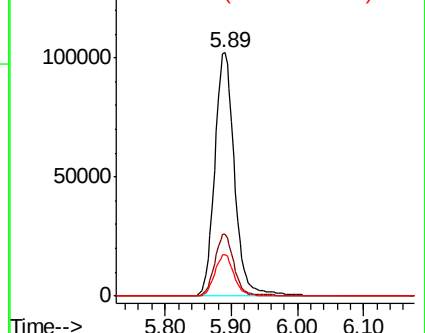







#35
 Dibromofluoromethane
 Concen: 48.967 ug/l
 RT: 4.89 min Scan# 1155
 Delta R.T. 0.00 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53

Instrument :
 MSVOA_U
 ClientSampleId :
 OILY-WATER

Tgt Ion:113 Resp: 71206
 Ion Ratio Lower Upper
 113 100
 111 102.4 83.1 124.7
 192 19.3 15.4 23.0

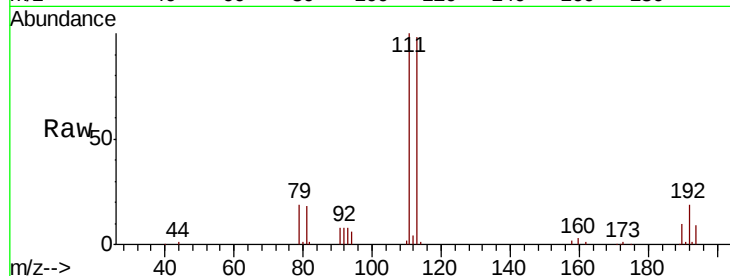


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V


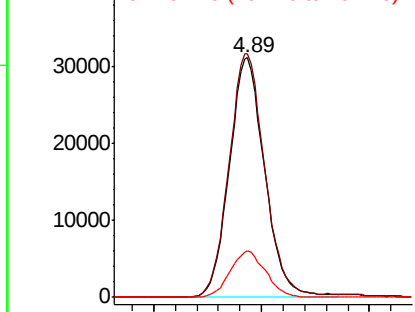



#36
 1,1-Dichloropropene
 Concen: 4.852 ug/l
 RT: 4.99 min Scan# 1186
 Delta R.T. -0.15 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53

Tgt Ion: 75 Resp: 11178
 Ion Ratio Lower Upper
 75 100
 110 7.5 15.5 46.5#
 77 0.0 25.4 38.0#



Abundance Ion 74.90 (74.60 to 75.60): VU0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VU0

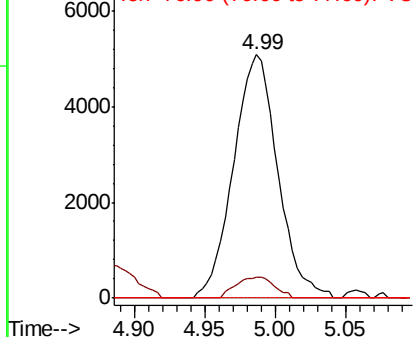


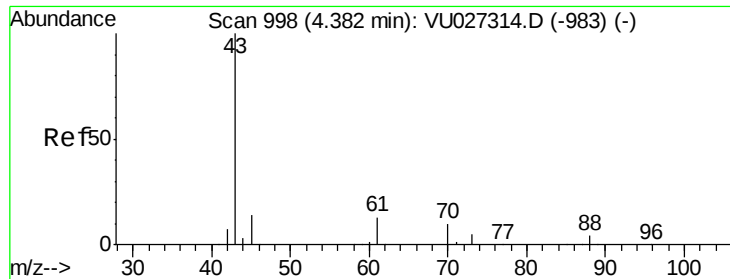




#37
Ethyl Acetate
Concen: 9.162 ug/l
RT: 4.27 min Scan# 964
Delta R.T. -0.11 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Instrument :
MSVOA_U
ClientSampled :
OILY-WATER

Tgt Ion: 43 Resp: 27281
Ion Ratio Lower Upper
43 100
61 0.0 10.7 16.1#
70 0.0 7.4 11.2#




Abundance Ion 43.00 (42.70 to 43.70): VU0
Ion 60.90 (60.60 to 61.60): VU0
Ion 70.00 (69.70 to 70.70): VU0

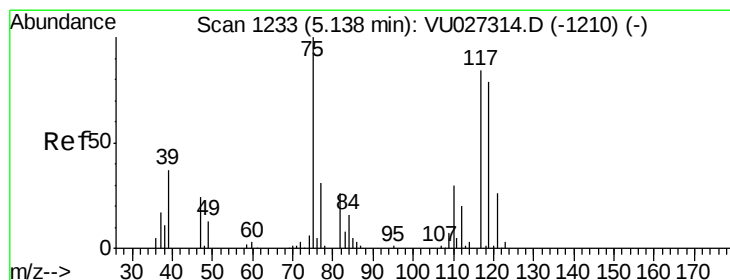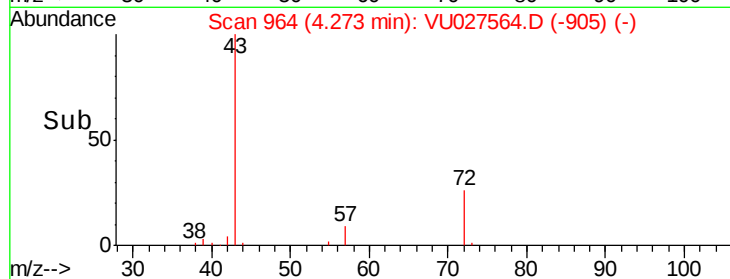
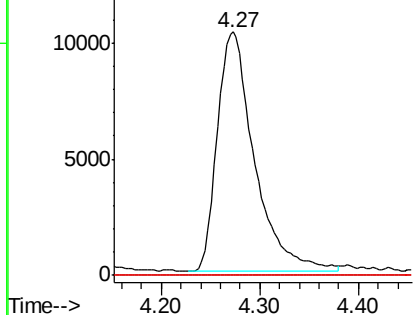



#38
Carbon Tetrachloride
Concen: 6.139 ug/l
RT: 4.99 min Scan# 1186
Delta R.T. -0.15 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Tgt Ion: 117 Resp: 12776
Ion Ratio Lower Upper
117 100
119 4.7 74.5 111.7#
121 0.0 24.6 37.0#

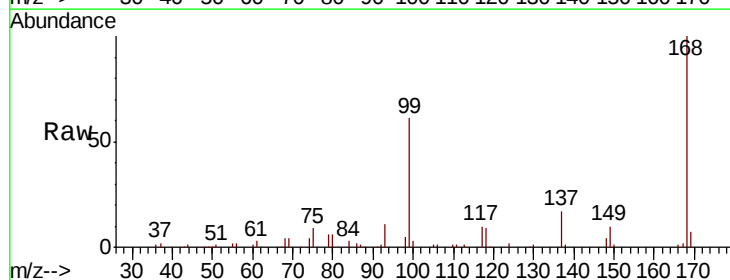

Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

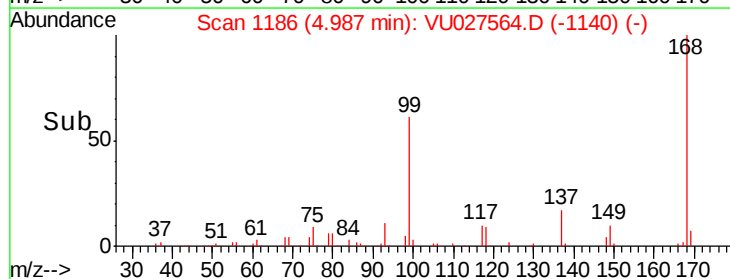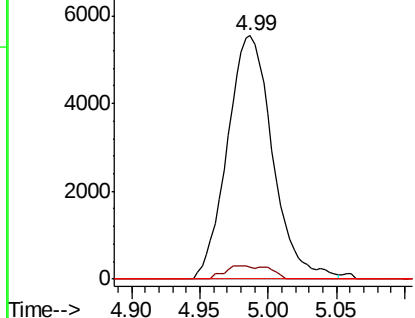



#40

Benzene

Concen: 0.220 ug/l

RT: 5.40 min Scan# 1313

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion: 78 Resp: 1475

Ion Ratio Lower Upper




78 100

77 34.3 19.3 28.9#

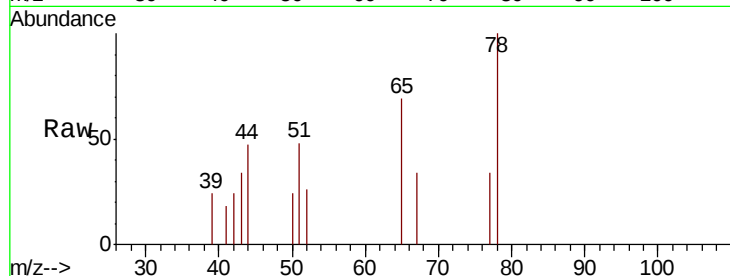

Abundance Ion 78.00 (77.70 to 78.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

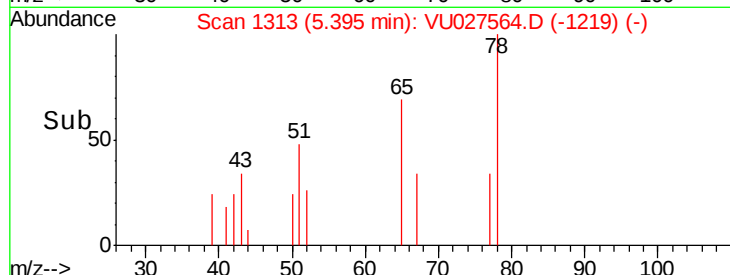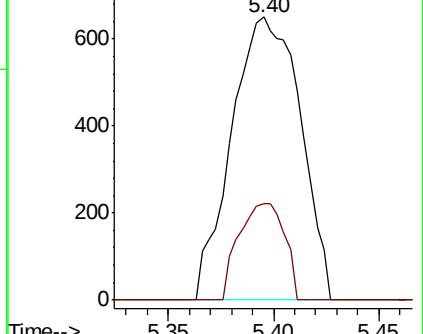

#48

Methyl methacrylate

Concen: 2.980 ug/l

RT: 6.53 min Scan# 1667

Delta R.T. -0.09 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 41 Resp: 6852

Ion Ratio Lower Upper

41 100

69 0.0 61.0 91.4#



39 51.2 39.9 59.9




Abundance Ion 41.00 (40.70 to 41.70): VU0

Ion 69.00 (68.70 to 69.70): VU0

Ion 39.00 (38.70 to 39.70): VU0

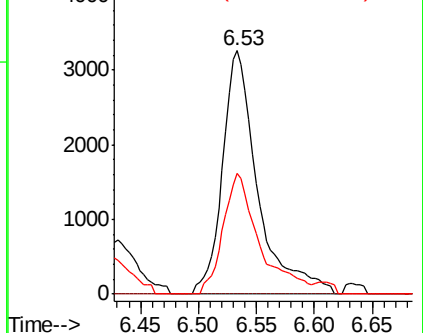

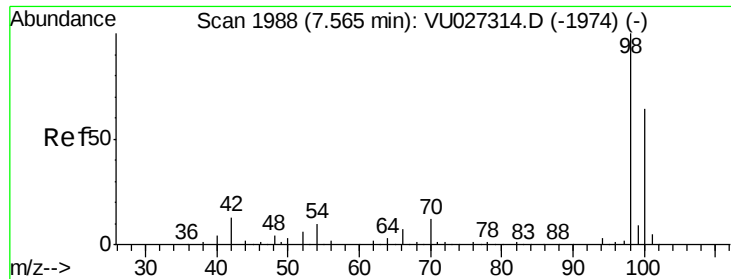

#50

Toluene-d8

Concen: 49.217 ug/l

RT: 7.57 min Scan# 1988

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :


OILY-WATER

Tgt Ion: 98 Resp: 267860

Ion Ratio Lower Upper

98 100

100 64.6 52.1 78.1

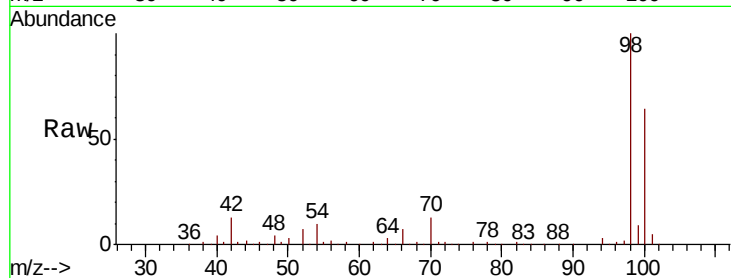

Abundance Ion 98.00 (97.70 to 98.70): VU027314.D (-1974) (-)

Ion 100.00 (99.70 to 100.70): VU027314.D (-1974) (-)

7.57

150000



100000

50000

0

7.50 7.55 7.60 7.65

Time-->

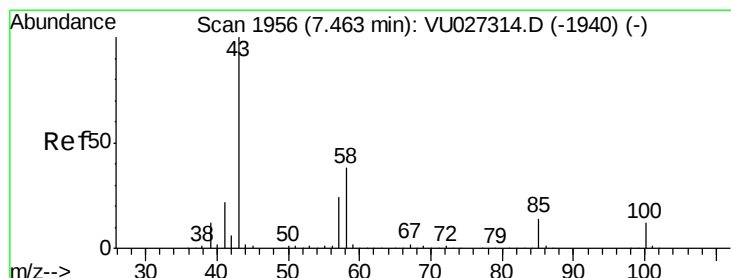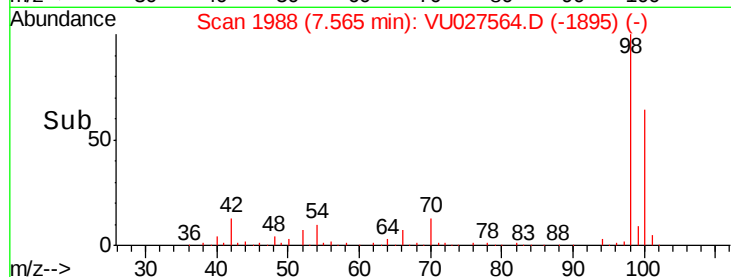

#51

4-Methyl-2-Pentanone

Concen: 1.483 ug/l

RT: 7.47 min Scan# 1958

Delta R.T. 0.01 min

Lab File: VU027564.D


Acq: 10 Oct 2018 12:53

Tgt Ion: 43 Resp: 4455

Ion Ratio Lower Upper

43 100

58 32.2 29.8 44.8

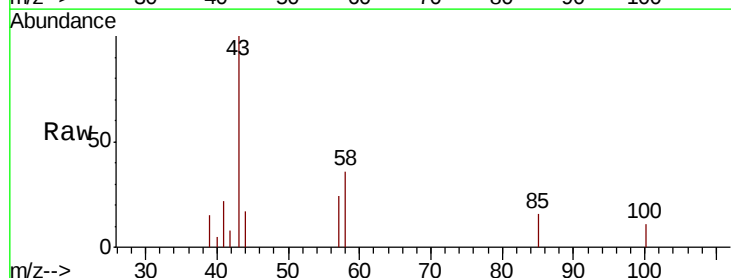

Abundance Ion 43.00 (42.70 to 43.70): VU027314.D (-1940) (-)

Ion 58.00 (57.70 to 58.70): VU027314.D (-1940) (-)

7.47

2500

2000

1500


1000


500

0

7.40 7.45 7.50

Time-->

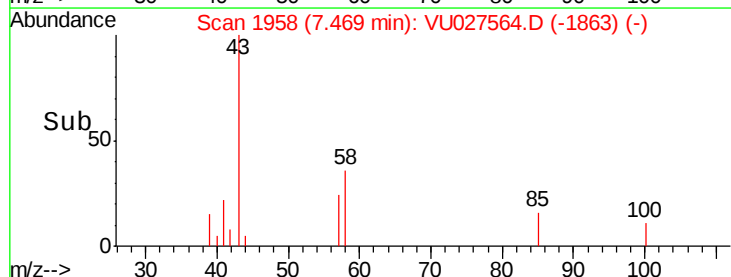

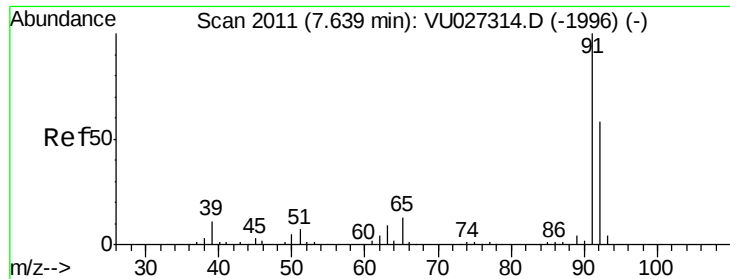

#52

Toluene

Concen: 0.250 ug/l

RT: 7.64 min Scan# 2011

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampled :


OILY-WATER

Tgt Ion: 92 Resp: 993

Ion Ratio Lower Upper




92 100

91 172.6 138.6 208.0

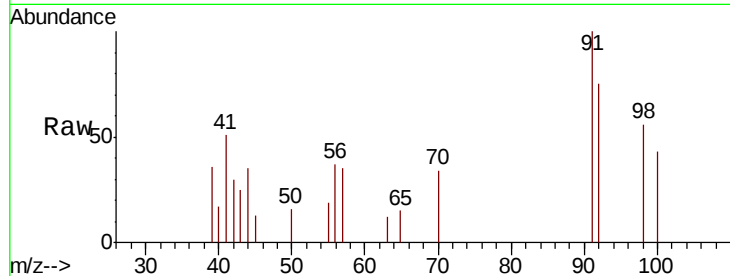

Abundance Ion 92.00 (91.70 to 92.70): VU0

Ion 91.00 (90.70 to 91.70): VU0

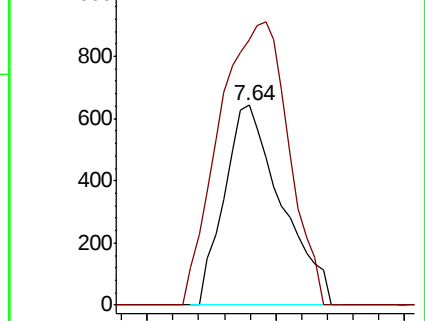

#56

Ethyl methacrylate

Concen: 2.298 ug/l

RT: 7.92 min Scan# 2099

Delta R.T. -0.10 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 69 Resp: 82

Ion Ratio Lower Upper

69 100

41 392.7 60.0 90.0#



39 236.6 29.5 44.3#




Abundance Ion 69.00 (68.70 to 69.70): VU0

Ion 41.00 (40.70 to 41.70): VU0

Ion 39.00 (38.70 to 39.70): VU0




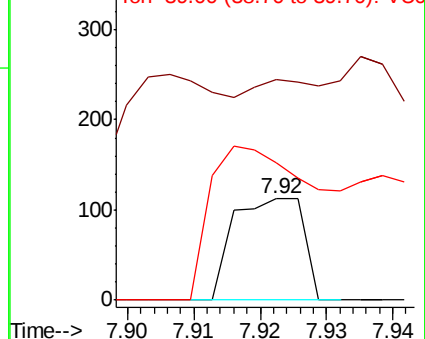


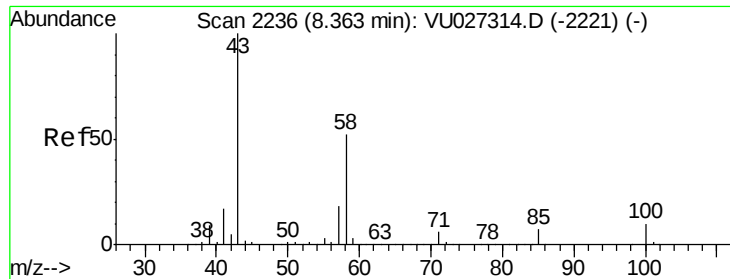

#59
2-Hexanone
Concen: 2.490 ug/l
RT: 8.37 min Scan# 2238
Delta R.T. 0.01 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53




Instrument :
MSVOA_U
ClientSampleId :
OILY-WATER


Tgt Ion: 43 Resp: 5804
Ion Ratio Lower Upper
43 100
58 50.5 26.1 78.3

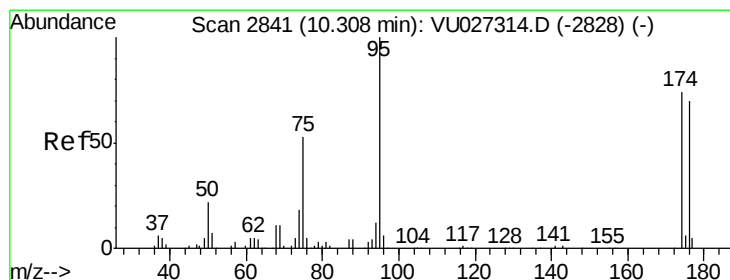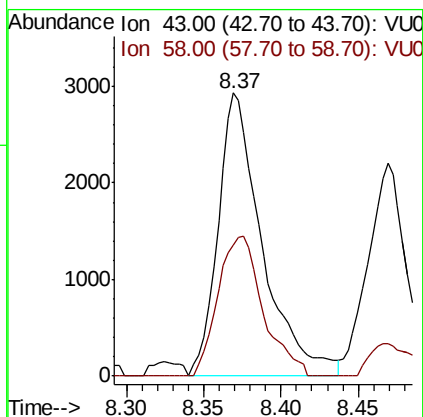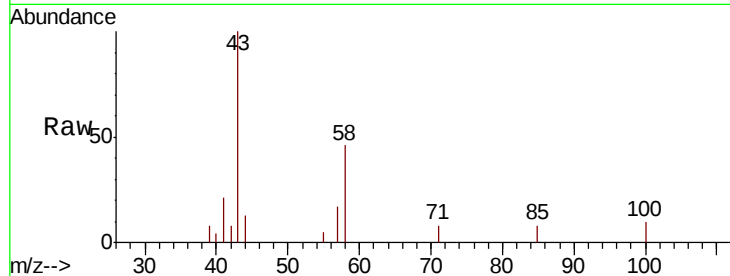

#62
4-Bromofluorobenzene
Concen: 44.416 ug/l
RT: 10.31 min Scan# 2841
Delta R.T. 0.00 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Tgt Ion: 95 Resp: 89838
Ion Ratio Lower Upper
95 100
174 74.7 0.0 147.8
176 71.7 0.0 140.8

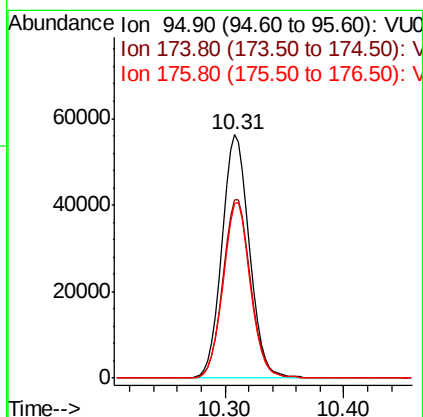


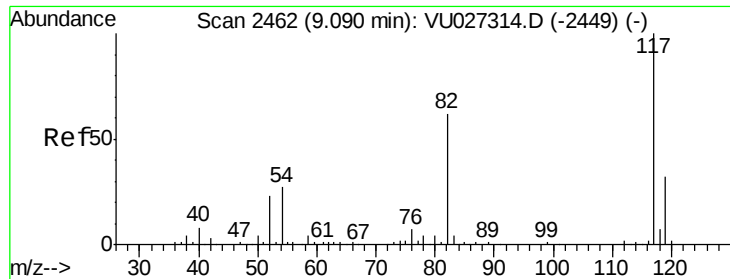




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2463
Delta R.T. 0.00 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Instrument :
MSVOA_U
ClientSampleId :
OILY-WATER

Tgt Ion:117 Resp: 185061
Ion Ratio Lower Upper
117 100
82 62.1 49.2 73.8
119 32.4 25.7 38.5

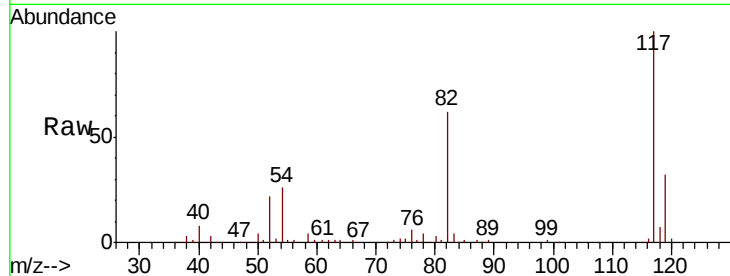


Abundance Ion 116.90 (116.60 to 117.60): V
150000 Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V


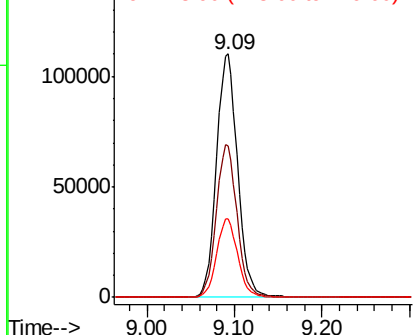



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3207
Delta R.T. 0.00 min
Lab File: VU027564.D
Acq: 10 Oct 2018 12:53

Tgt Ion:152 Resp: 85643
Ion Ratio Lower Upper
152 100
115 61.0 43.4 130.2
150 158.9 0.0 349.2



Abundance Ion 151.90 (151.60 to 152.60): V
120000 Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V




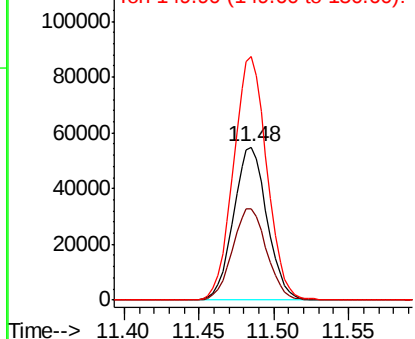


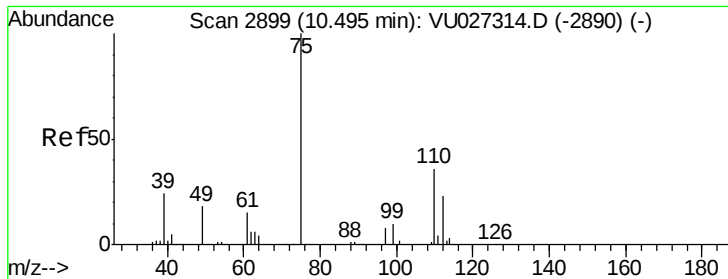

#76
 1,2,3-Trichloropropane
 Concen: 21.542 ug/l
 RT: 10.31 min Scan# 2841
 Delta R.T. -0.19 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53




Instrument :
 MSVOA_U
 ClientSampleId :
 OILY-WATER


Tgt Ion: 75 Resp: 47825
 Ion Ratio Lower Upper
 75 100
 77 1.2 20.3 60.9#

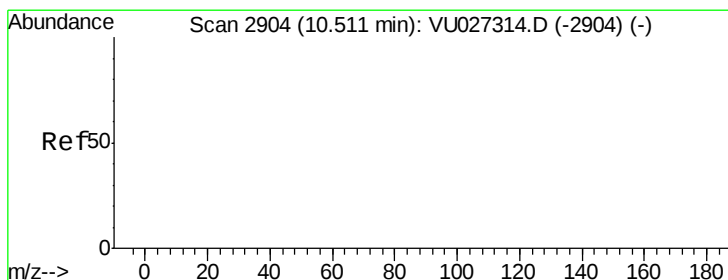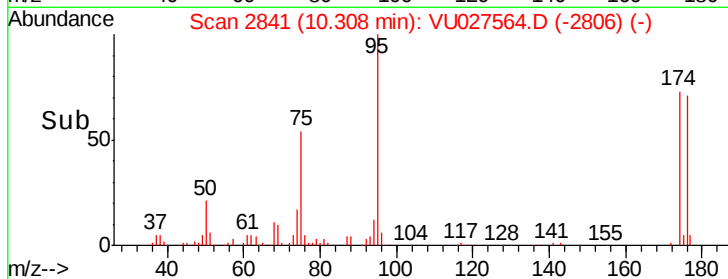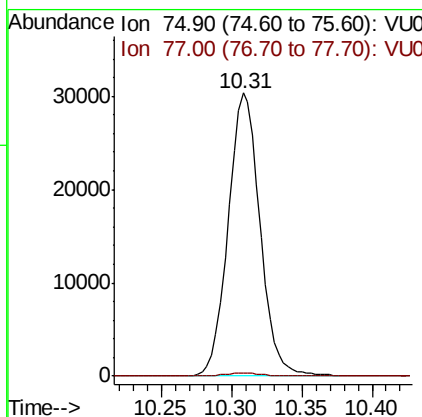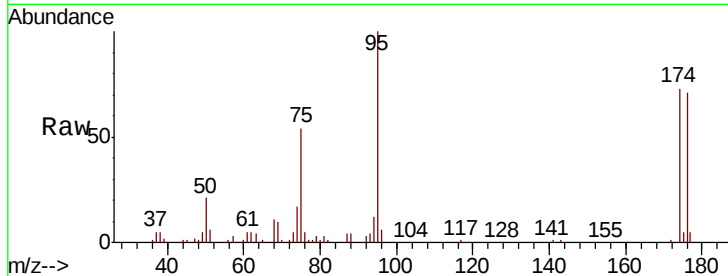

#81
 trans-1,4-Dichloro-2-butene
 Concen: 56.378 ug/l
 RT: 10.31 min Scan# 2841
 Delta R.T. -0.20 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53

Tgt Ion: 75 Resp: 47825
 Ion Ratio Lower Upper
 75 100
 53 0.0 0.0 0.0
 89 0.0 0.0 0.0


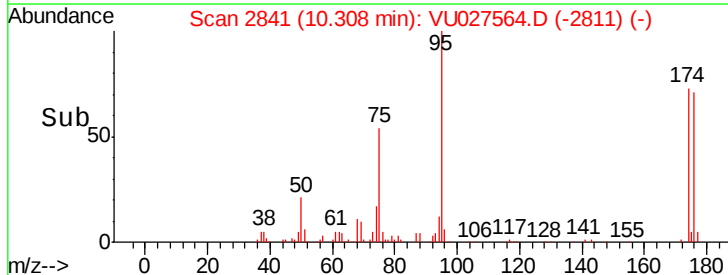
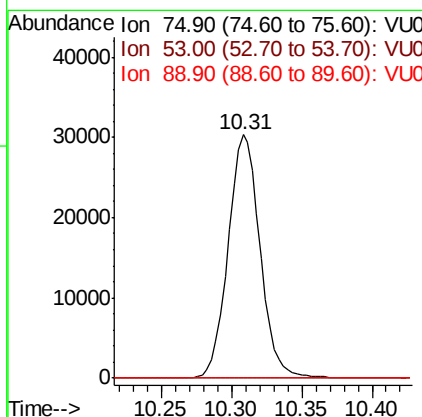
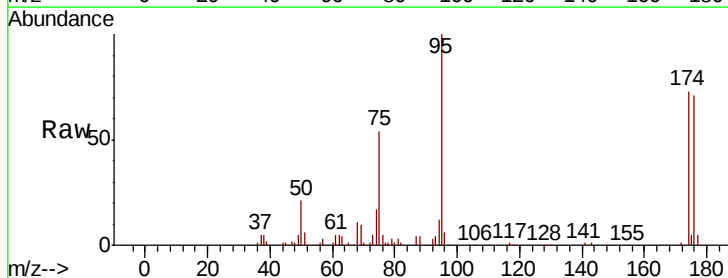


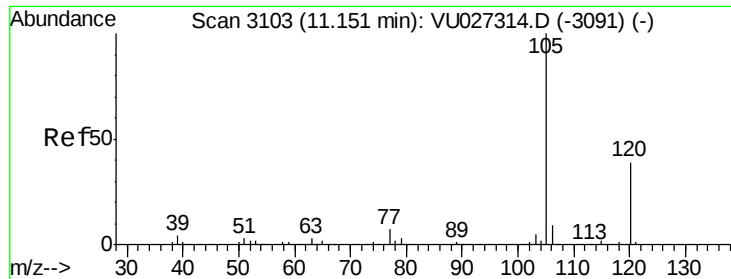

#84
 1,2,4-Trimethylbenzene
 Concen: 0.276 ug/l
 RT: 11.15 min Scan# 3103
 Delta R.T. 0.00 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53




Instrument :
 MSVOA_U
 ClientSampleId :
 OILY-WATER


Tgt Ion:105 Resp: 1426
 Ion Ratio Lower Upper
 105 100
 120 32.1 22.1 66.5

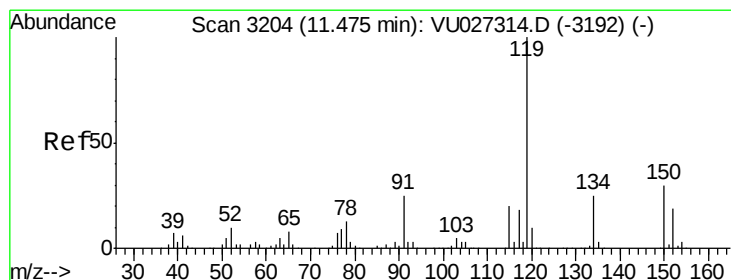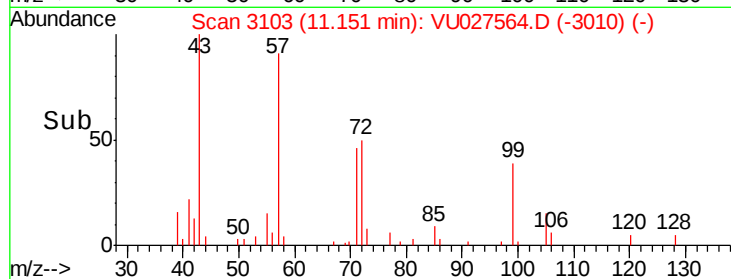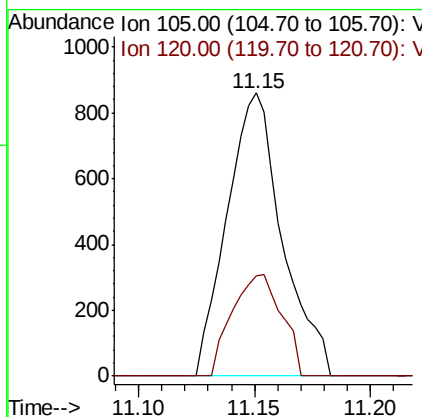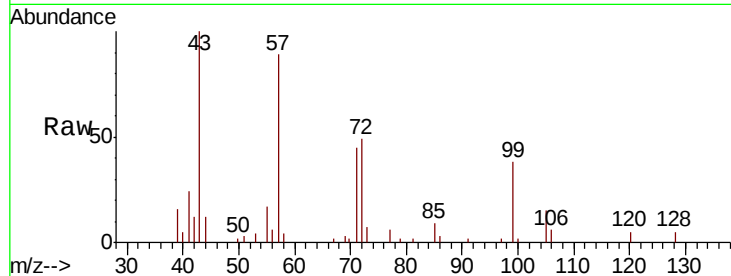

#86
 p-Isopropyltoluene
 Concen: 1.084 ug/l
 RT: 11.48 min Scan# 3204
 Delta R.T. 0.00 min
 Lab File: VU027564.D
 Acq: 10 Oct 2018 12:53

Tgt Ion:119 Resp: 5727
 Ion Ratio Lower Upper
 119 100
 134 25.0 12.7 38.1
 91 29.0 12.2 36.4

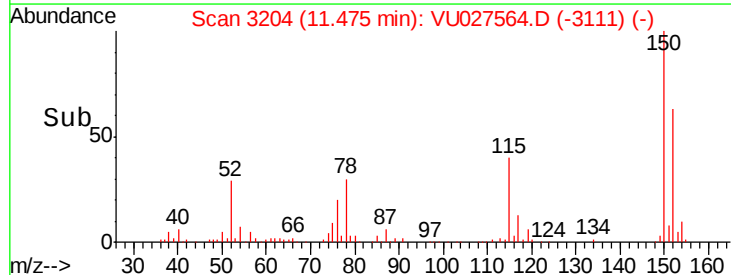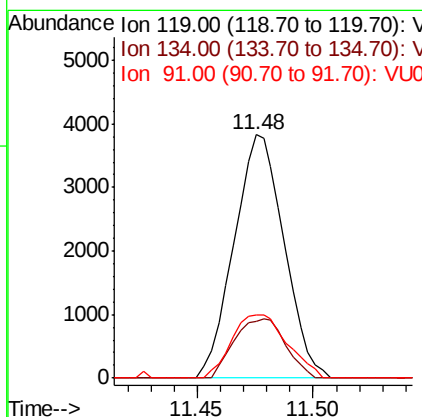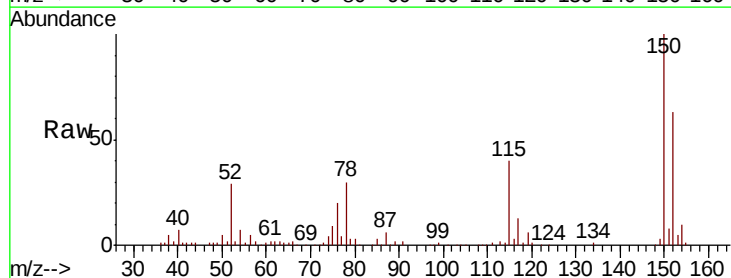

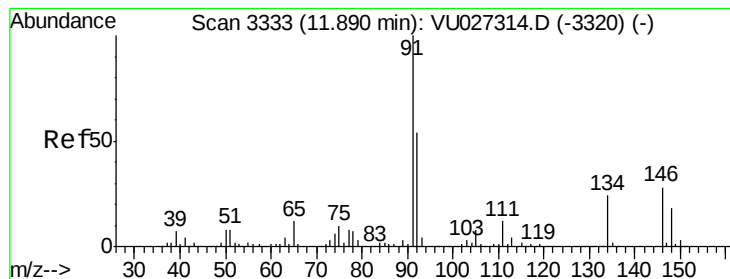

#89

n-Butylbenzene

Concen: 2.039 ug/l

RT: 11.89 min Scan# 3334

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53

Instrument :

MSVOA_U

ClientSampleId :

OILY-WATER


Tgt Ion: 91 Resp: 520

Ion Ratio Lower Upper

91 100

92 35.8 27.0 81.0

134 8.3 11.7 35.1#






Abundance Ion 91.00 (90.70 to 91.70): VU027314.D (-3320) (-)

Ion 92.00 (91.70 to 92.70): VU027314.D (-3320) (-)

Ion 134.00 (133.70 to 134.70): VU027314.D (-3320) (-)

Time-->

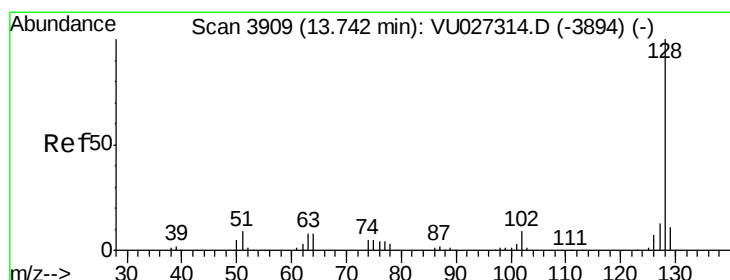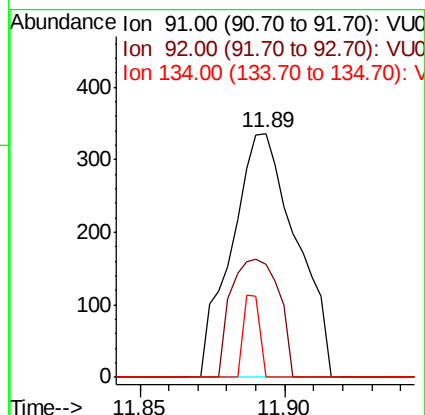

#95

Naphthalene

Concen: 2.050 ug/l

RT: 13.75 min Scan# 3910

Delta R.T. 0.00 min

Lab File: VU027564.D

Acq: 10 Oct 2018 12:53


Tgt Ion: 128 Resp: 2612

Ion Ratio Lower Upper

128 100

127 17.2 10.5 15.7#

129 8.7 8.6 12.8



Abundance Ion 128.00 (127.70 to 128.70): VU027314.D (-3894) (-)

Ion 127.00 (126.70 to 127.70): VU027314.D (-3894) (-)

Ion 129.00 (128.70 to 129.70): VU027314.D (-3894) (-)

Time-->

