

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101018\  
Data File : VU027536.D  
Acq On : 09 Oct 2018 21:08  
Operator : MD/SY  
Sample : J5303-23  
Misc : 5.0mL/MSVOA U/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
EB07-20181004

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U100118W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.328       | 348           | 359         | 374          | rBV      | 5451           | 8262          | 1.18%           | 0.232%        |
| 2         | 2.450       | 386           | 397         | 418          | rBV      | 29331          | 54031         | 7.71%           | 1.515%        |
| 3         | 4.205       | 928           | 943         | 959          | rBV2     | 6738           | 19541         | 2.79%           | 0.548%        |
| 4         | 4.887       | 1139          | 1155        | 1171         | rBV2     | 100758         | 227108        | 32.39%          | 6.368%        |
| 5         | 4.987       | 1172          | 1186        | 1209         | rVV      | 159648         | 353338        | 50.39%          | 9.907%        |
| 6         | 5.315       | 1270          | 1288        | 1316         | rBV      | 128240         | 275641        | 39.31%          | 7.729%        |
| 7         | 5.890       | 1452          | 1467        | 1495         | rBV      | 247775         | 503059        | 71.75%          | 14.105%       |
| 8         | 7.569       | 1974          | 1989        | 2025         | rBV      | 392558         | 701140        | 100.00%         | 19.659%       |
| 9         | 9.093       | 2448          | 2463        | 2490         | rBV      | 339597         | 570646        | 81.39%          | 16.000%       |
| 10        | 10.311      | 2829          | 2842        | 2864         | rBV      | 240454         | 385711        | 55.01%          | 10.815%       |
| 11        | 11.485      | 3195          | 3207        | 3224         | rBV      | 294870         | 467976        | 66.75%          | 13.122%       |


Sum of corrected areas: 3566453

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101018\  
Data File : VU027536.D  
Acq On : 09 Oct 2018 21:08  
Operator : MD/SY  
Sample : J5303-23  
Misc : 5.0mL/MSVOA U/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
EB07-20181004

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\82U100118W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

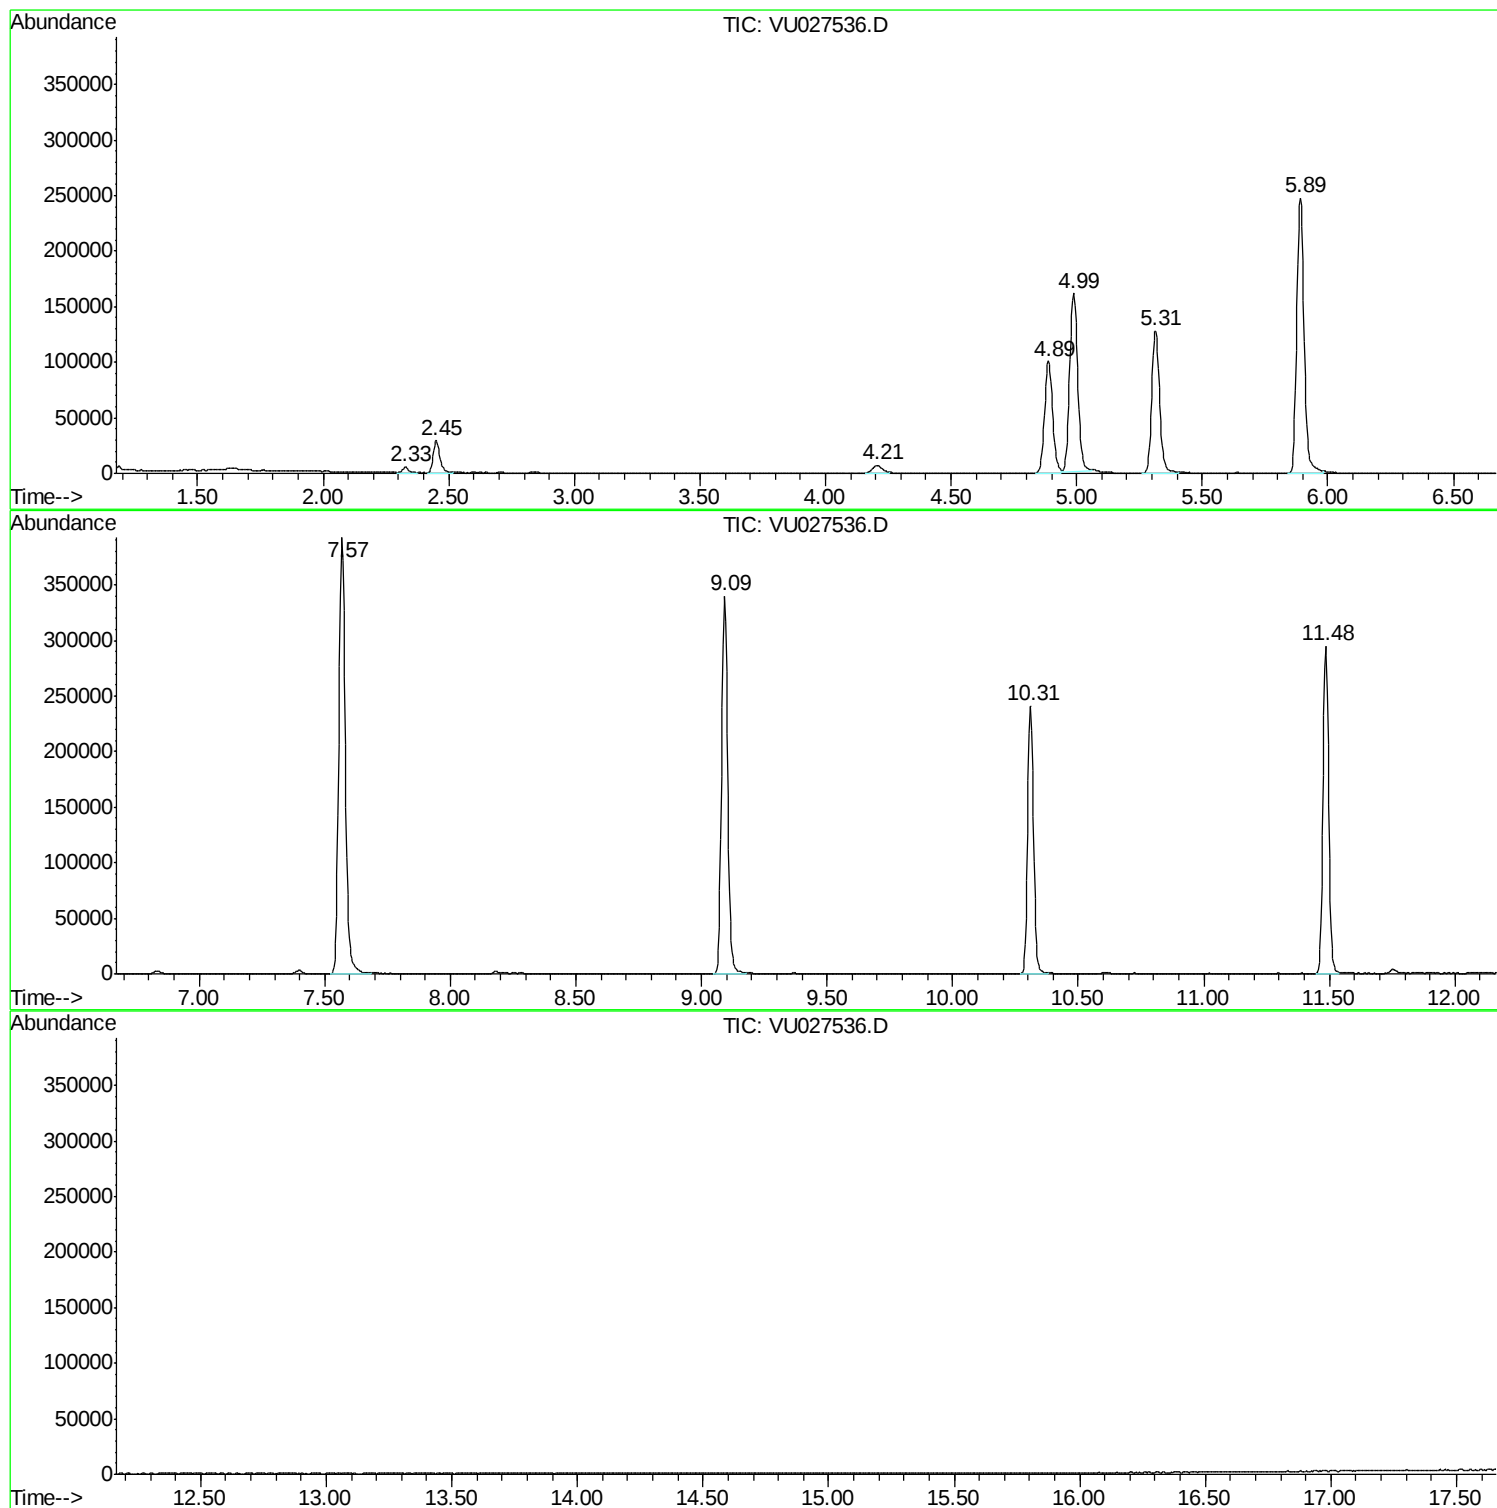

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_U\DATA\VU101018\  
Data File : VU027536.D  
Acq On : 09 Oct 2018 21:08  
Operator : MD/SY  
Sample : J5303-23  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
EB07-20181004

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\82U100118W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_U\DATA\VU101018\  
Data File : VU027536.D  
Acq On : 09 Oct 2018 21:08  
Operator : MD/SY  
Sample : J5303-23  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
EB07-20181004

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\82U100118W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |