


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101018\
Data File : VU027525.D
Acq On : 09 Oct 2018 16:39
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U100118W.M
Title : SW846 8260
Last Update : Tue Oct 02 02:04:34 2018

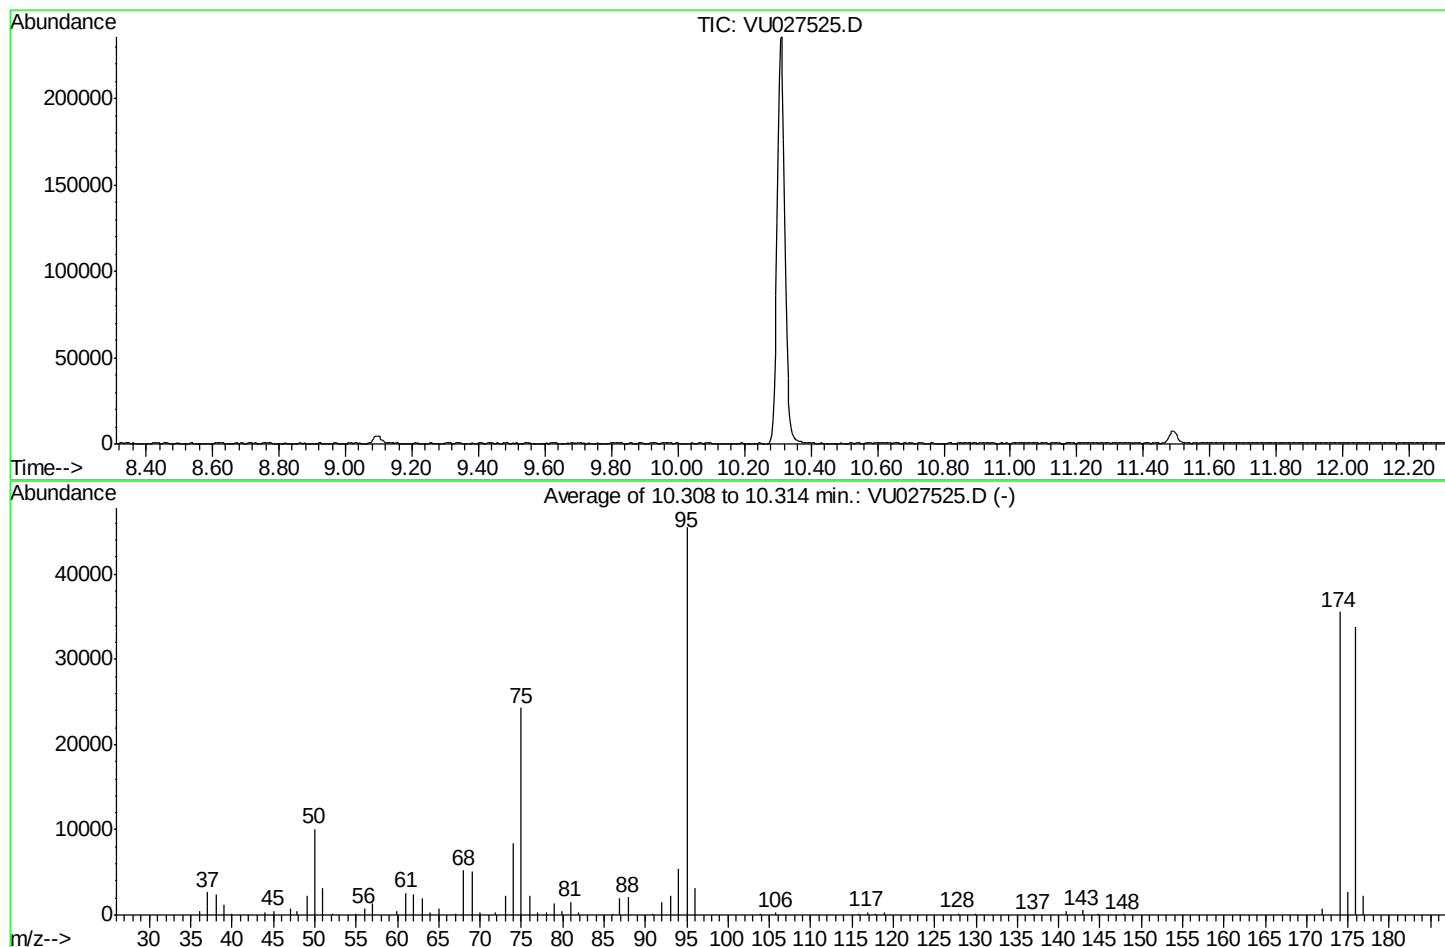

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	10104	PASS
75	95	30	60	53.4	24317	PASS
95	95	100	100	100.0	45496	PASS
96	95	5	9	7.1	3213	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.2	35581	PASS
175	174	5	9	7.8	2776	PASS
176	174	95	101	95.2	33866	PASS
177	176	5	9	6.6	2220	PASS