
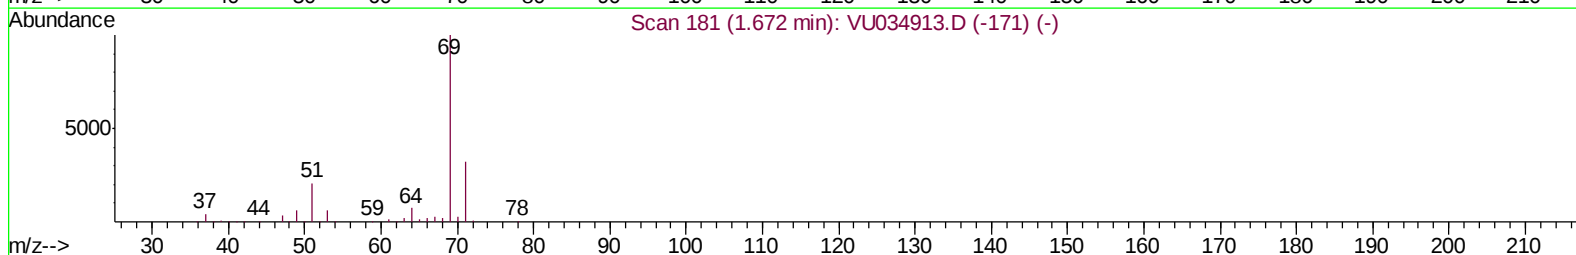
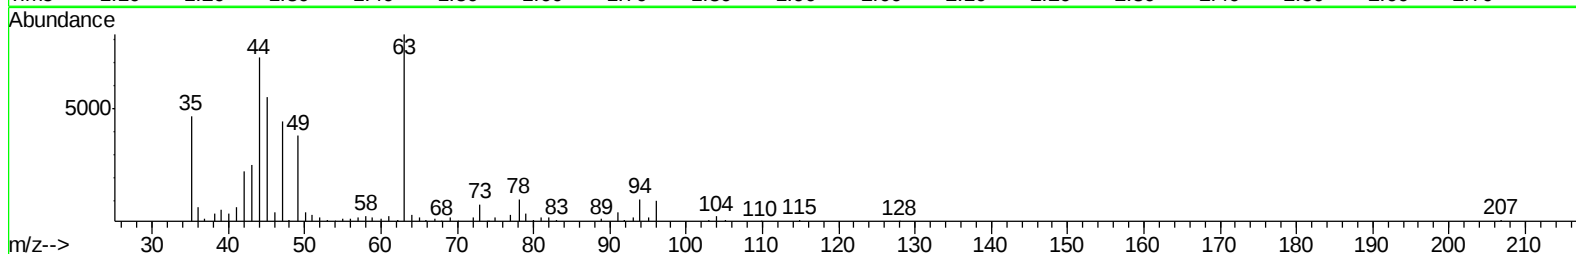


Data File : VU035019.D
Acq On : 09 Oct 2019 19:52
Operator : JC/SP
Sample : K5267-08
Misc : 6.34g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 10 04:50:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 04:46:10 2019
Response via : Initial Calibration

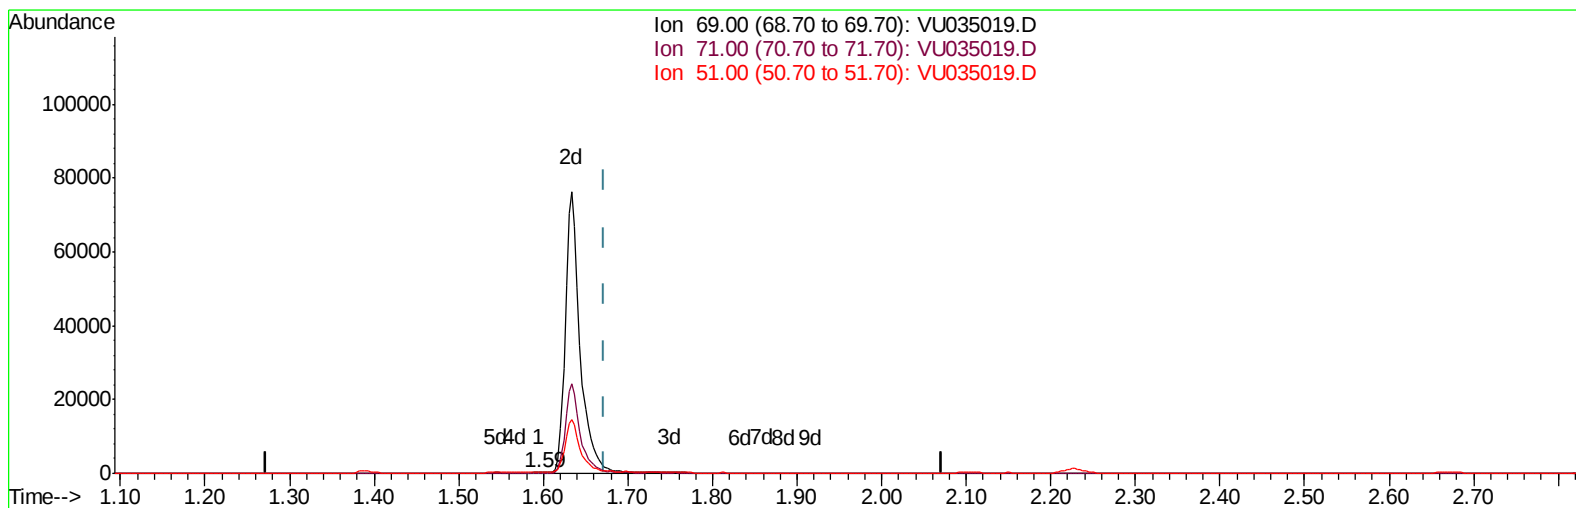

TIC: VU035019.D

(7) Chloroethane-d5 (S)

1.595min (-0.077) 0.09ug/L

response 207

Ion	Exp%	Act%
69.00	100	100
71.00	32.20	30.92
51.00	27.80	29.47
0.00	0.00	0.00