
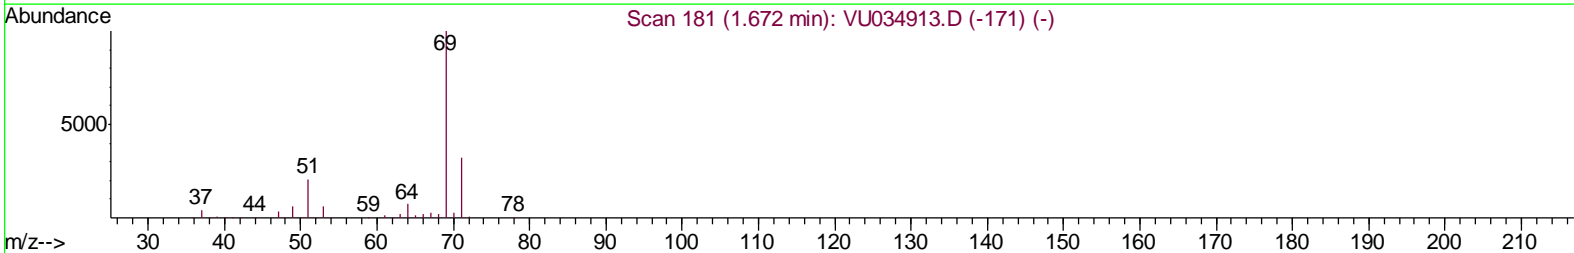
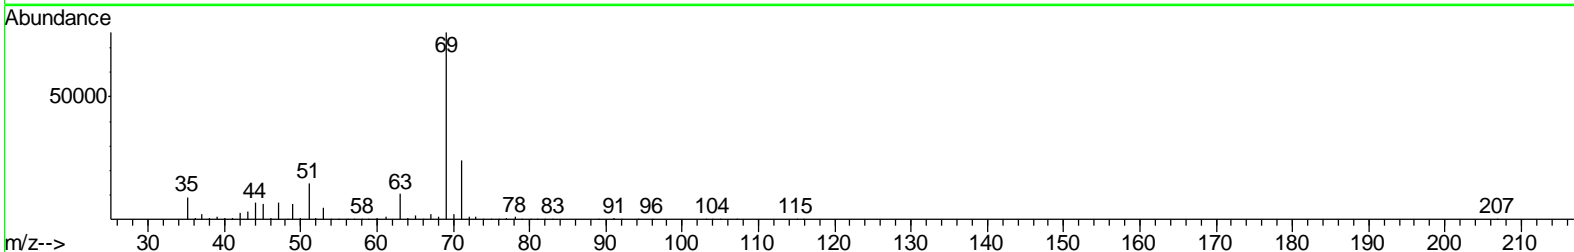


Data File : VU035019.D  
Acq On : 09 Oct 2019 19:52  
Operator : JC/SP  
Sample : K5267-08  
Misc : 6.34g/5mL/100uL/5.0mL/MSVOA\_U/MEOH  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 10 04:50:16 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM100319WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Oct 10 04:46:10 2019  
Response via : Initial Calibration

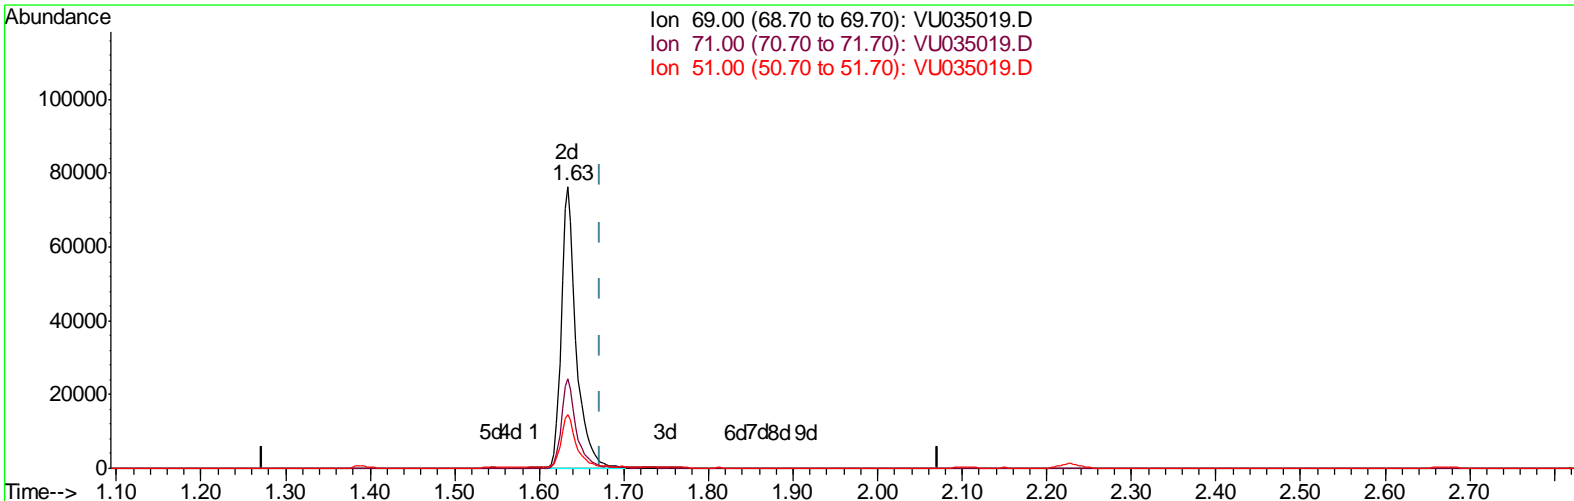

TIC: VU035019.D

(7) Chloroethane-d5 (S)  
1.634min (-0.039) 39.15ug/L m  
response 93780

Ion	Exp%	Act%
69.00	100	100
71.00	32.20	0.07#
51.00	27.80	0.07#
0.00	0.00	0.00