
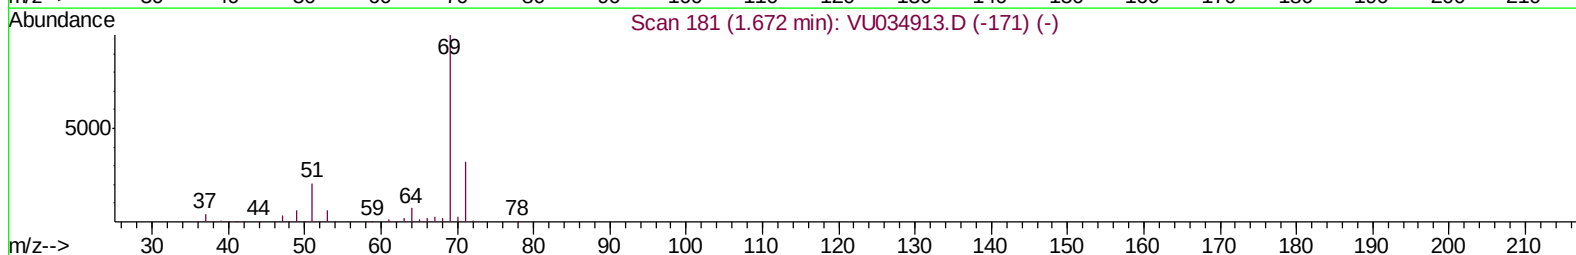
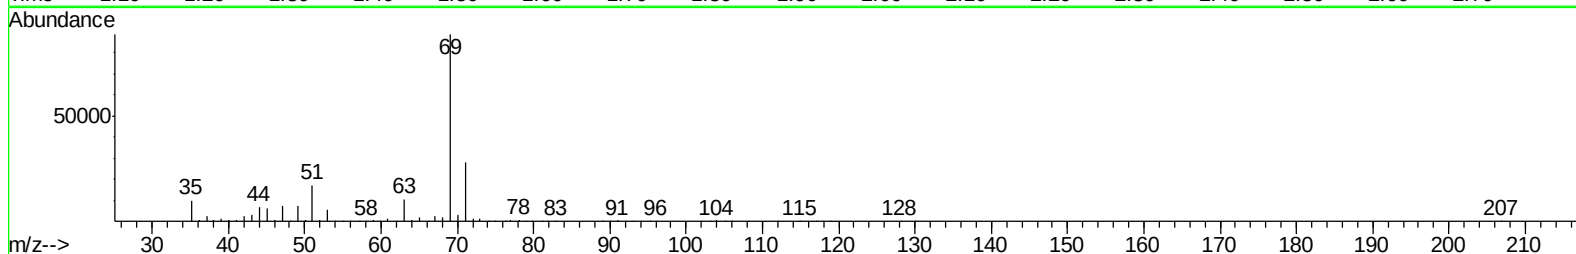


Data File : VU035024.D
Acq On : 09 Oct 2019 21:48
Operator : JC/SP
Sample : K5265-06
Misc : 6.94g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 10 04:51:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 04:46:10 2019
Response via : Initial Calibration

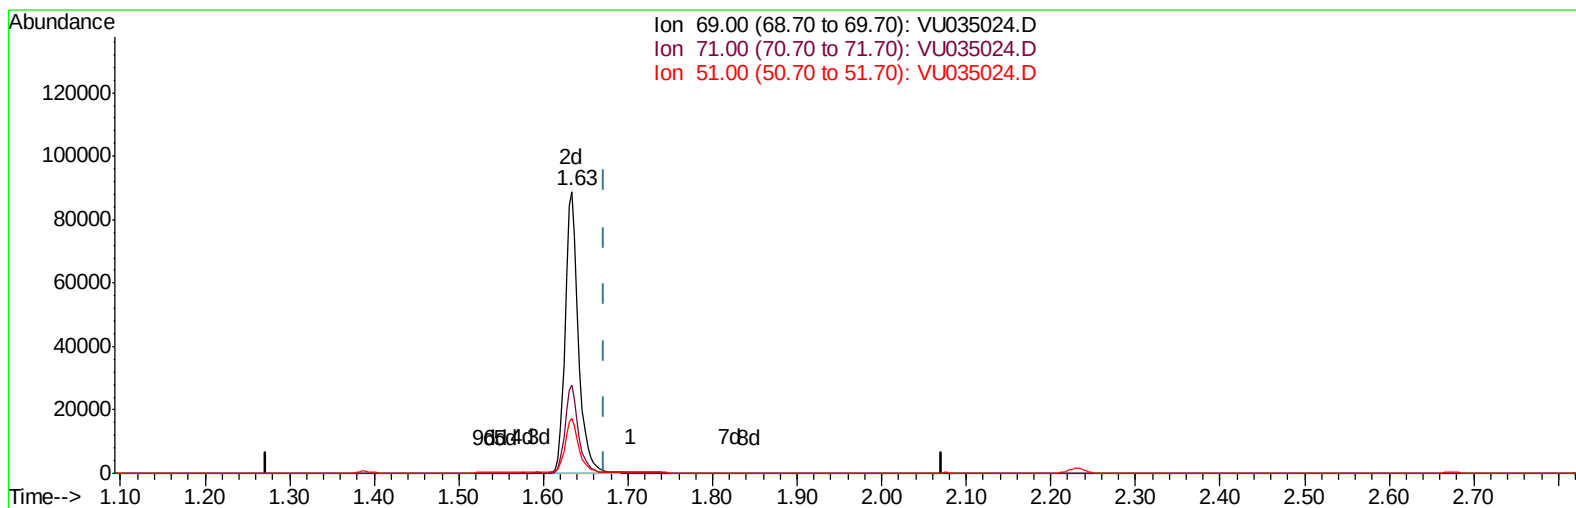

TIC: VU035024.D

(7) Chloroethane-d5 (S)

1.633min (-0.039) 38.74ug/L m

response 97588

Ion	Exp%	Act%
69.00	100	100
71.00	32.20	0.00#
51.00	27.80	0.15#
0.00	0.00	0.00