

Data File : VU035027.D
Acq On : 09 Oct 2019 22:59
Operator : JC/SP
Sample : K5265-12
Misc : 7.10g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBAS3

Quant Time: Oct 10 04:51:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 04:46:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	423736	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	416947	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	166586	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	125602	36.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.76%
7) Chloroethane-d5	1.63	69	93844	36.56	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	73.12%
11) 1,1-Dichloroethene-d2	2.23	63	179717	29.87	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.74%#
21) 2-Butanone-d5	4.17	46	205726	82.00	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.00%
24) Chloroform-d	4.62	84	217160	39.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.44%
26) 1,2-Dichloroethane-d4	5.28	65	158820	42.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.48%
32) Benzene-d6	5.31	84	490483	41.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.66%
36) 1,2-Dichloropropane-d6	6.31	67	162359	41.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.90%
41) Toluene-d8	7.54	98	441657	40.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.32%
43) trans-1,3-Dichloropropene-	7.83	79	62453	36.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.06%
47) 2-Hexanone-d5	8.31	63	152457	83.07	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.07%
57) 1,1,2,2-Tetrachloroethane-	10.42	84	232990	42.39	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.78%
64) 1,2-Dichlorobenzene-d4	11.84	152	147281	43.06	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.12%

Target Compounds


					Qvalue
25) Chloroform	4.65	83	9403	1.678 ug/L	86
37) 1,2-Dichloropropane	6.31	63	18386	5.417 ug/L #	89
39) cis-1,3-Dichloropropene	7.21	75	4038	0.785 ug/L #	61
48) 2-Hexanone	8.31	43	18091	4.515 ug/L #	71
59) 1,2,3-Trichloropropane	11.47	75	22155	5.049 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU035027.D
Acq On : 09 Oct 2019 22:59
Operator : JC/SP
Sample : K5265-12
Misc : 7.10g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBAS3

Quant Time: Oct 10 04:51:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 04:46:10 2019
Response via : Initial Calibration




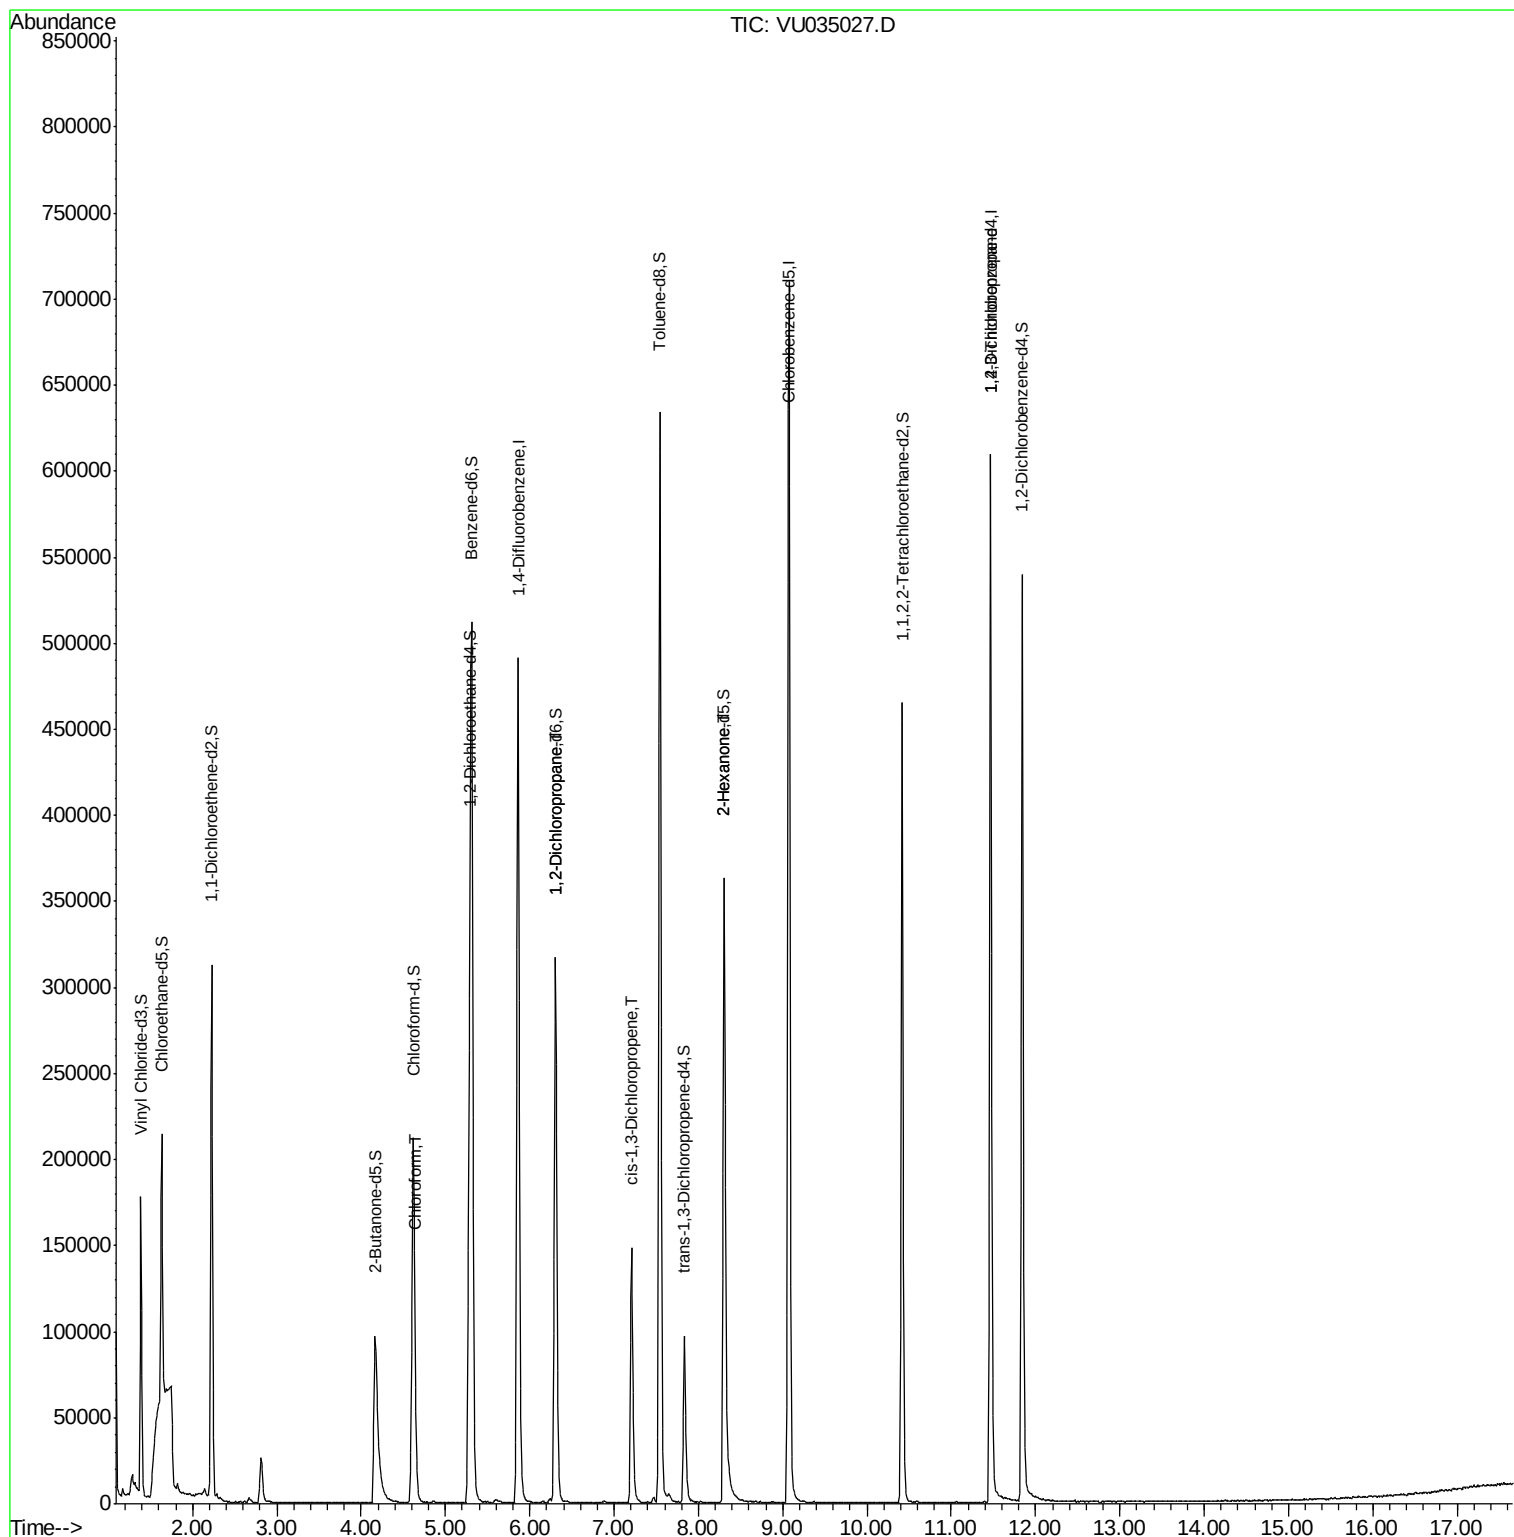


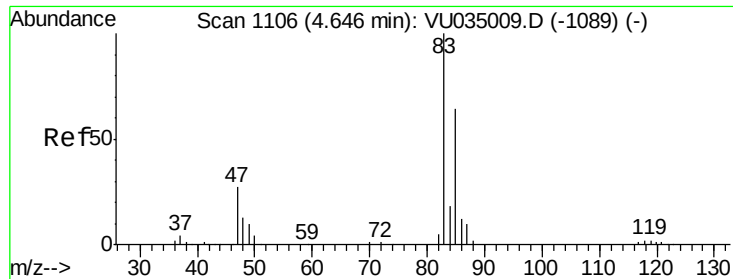

#25
Chloroform
Concen: 1.678 ug/L
RT: 4.65 min Scan# 1106
Delta R.T. 0.00 min
Lab File: VU035027.D
Acq: 09 Oct 2019 22:59




Instrument :
MSVOA_U
ClientSampleId :
DBAS3


Tgt Ion: 83 Resp: 9403
Ion Ratio Lower Upper
83 100
85 74.0 44.2 82.2

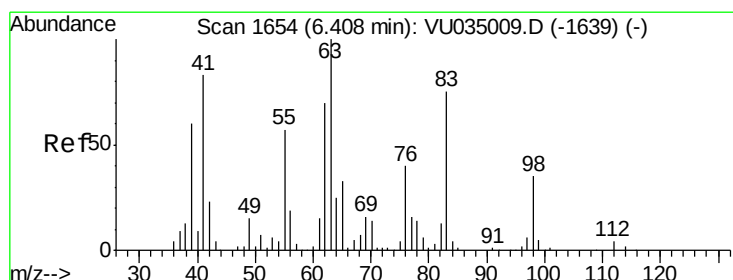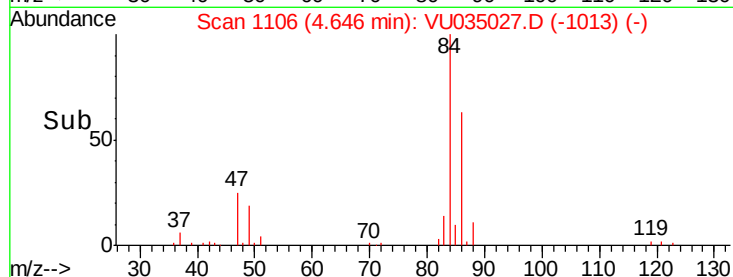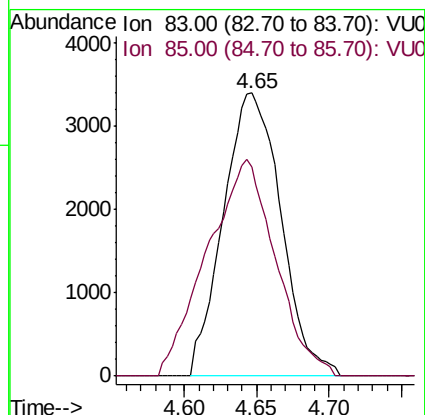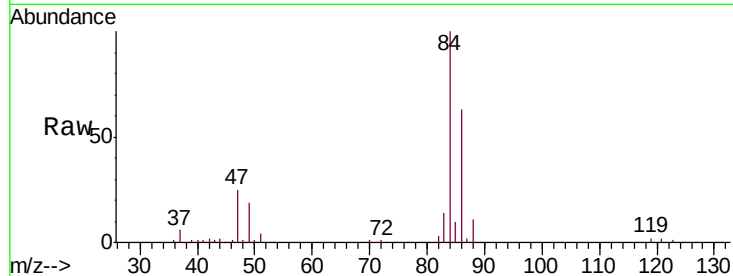

#37
1,2-Dichloropropane
Concen: 5.417 ug/L
RT: 6.31 min Scan# 1622
Delta R.T. -0.10 min
Lab File: VU035027.D
Acq: 09 Oct 2019 22:59

Tgt Ion: 63 Resp: 18386
Ion Ratio Lower Upper
63 100
112 0.0 2.9 4.3#


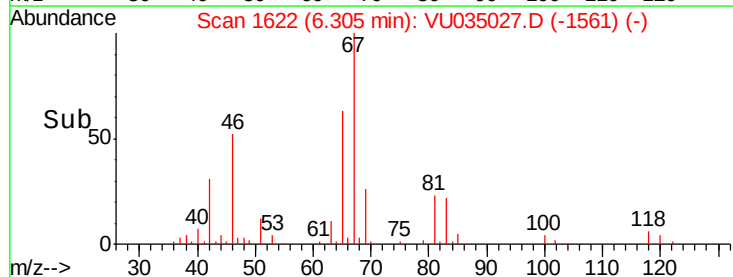
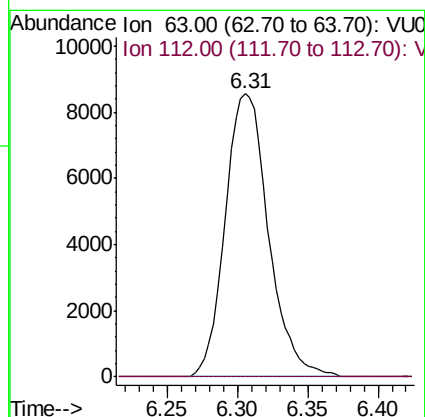
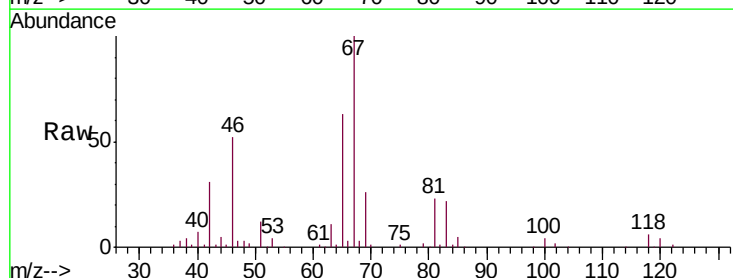


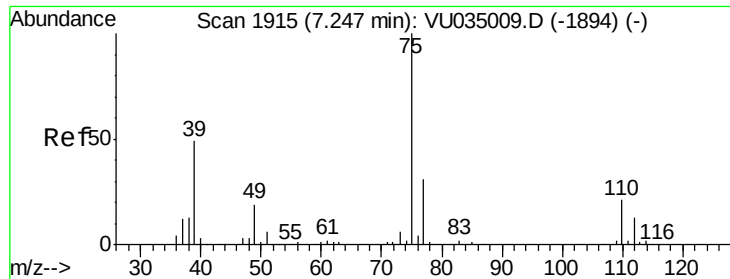

#39
 cis-1,3-Dichloropropene
 Concen: 0.785 ug/L
 RT: 7.21 min Scan# 1903
 Delta R.T. -0.04 min
 Lab File: VU035027.D
 Acq: 09 Oct 2019 22:59




Instrument :
 MSVOA_U
 ClientSampleId :
 DBAS3


Tgt Ion: 75 Resp: 4038
 Ion Ratio Lower Upper
 75 100
 77 53.1 22.0 40.8#

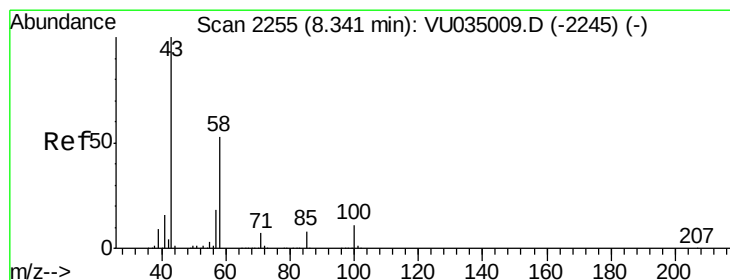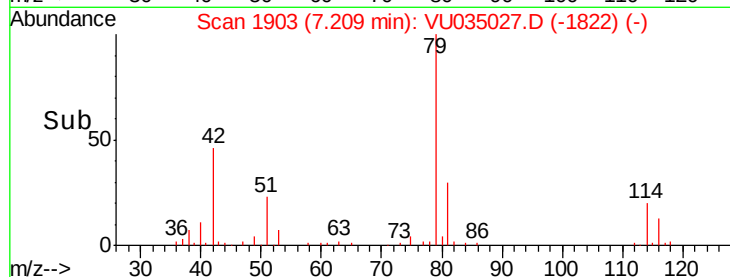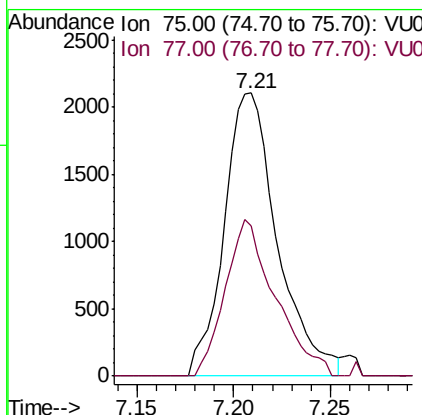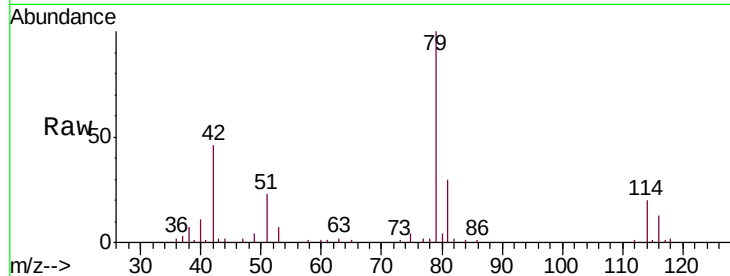

#48
 2-Hexanone
 Concen: 4.515 ug/L
 RT: 8.31 min Scan# 2244
 Delta R.T. -0.04 min
 Lab File: VU035027.D
 Acq: 09 Oct 2019 22:59

Tgt Ion: 43 Resp: 18091
 Ion Ratio Lower Upper
 43 100
 58 27.7 40.8 61.2#
 57 25.1 14.0 21.0#
 100 0.0 8.0 12.0#

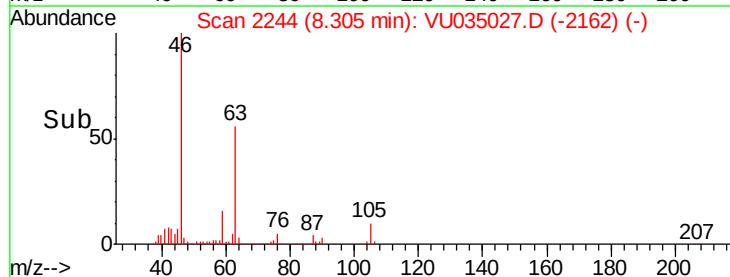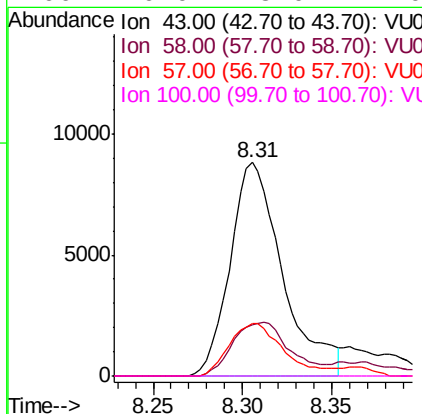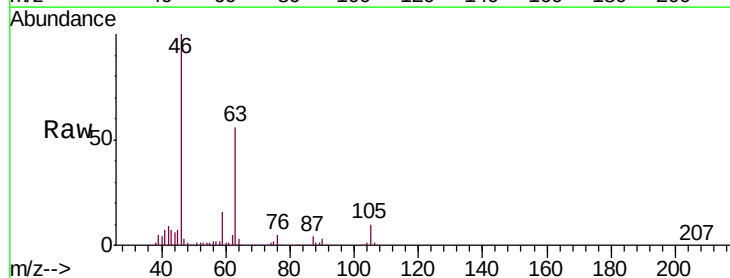

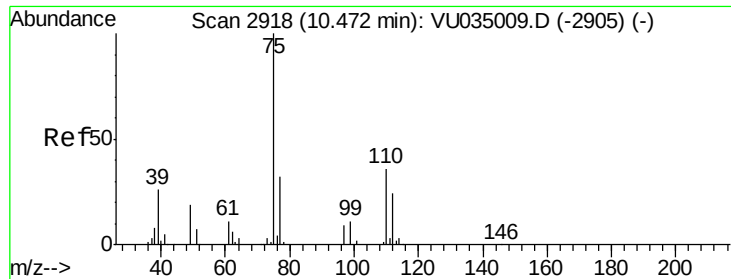

#59

1,2,3-Trichloropropane

Concen: 5.049 ug/L

RT: 11.47 min Scan# 3227

Delta R.T. 0.99 min

Lab File: VU035027.D

Acq: 09 Oct 2019 22:59

Instrument :

MSVOA_U

ClientSampleId :

DBAS3

Tgt Ion: 75 Resp: 22155

Ion Ratio Lower Upper

75 100

77 34.8 25.7 38.5

