


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101019\
Data File : VU035008.D
Acq On : 09 Oct 2019 15:26
Operator : JC/SP
Sample : BFB43
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100319WMA.M
Title : VOC Analysis
Last Update : Thu Oct 10 05:07:06 2019

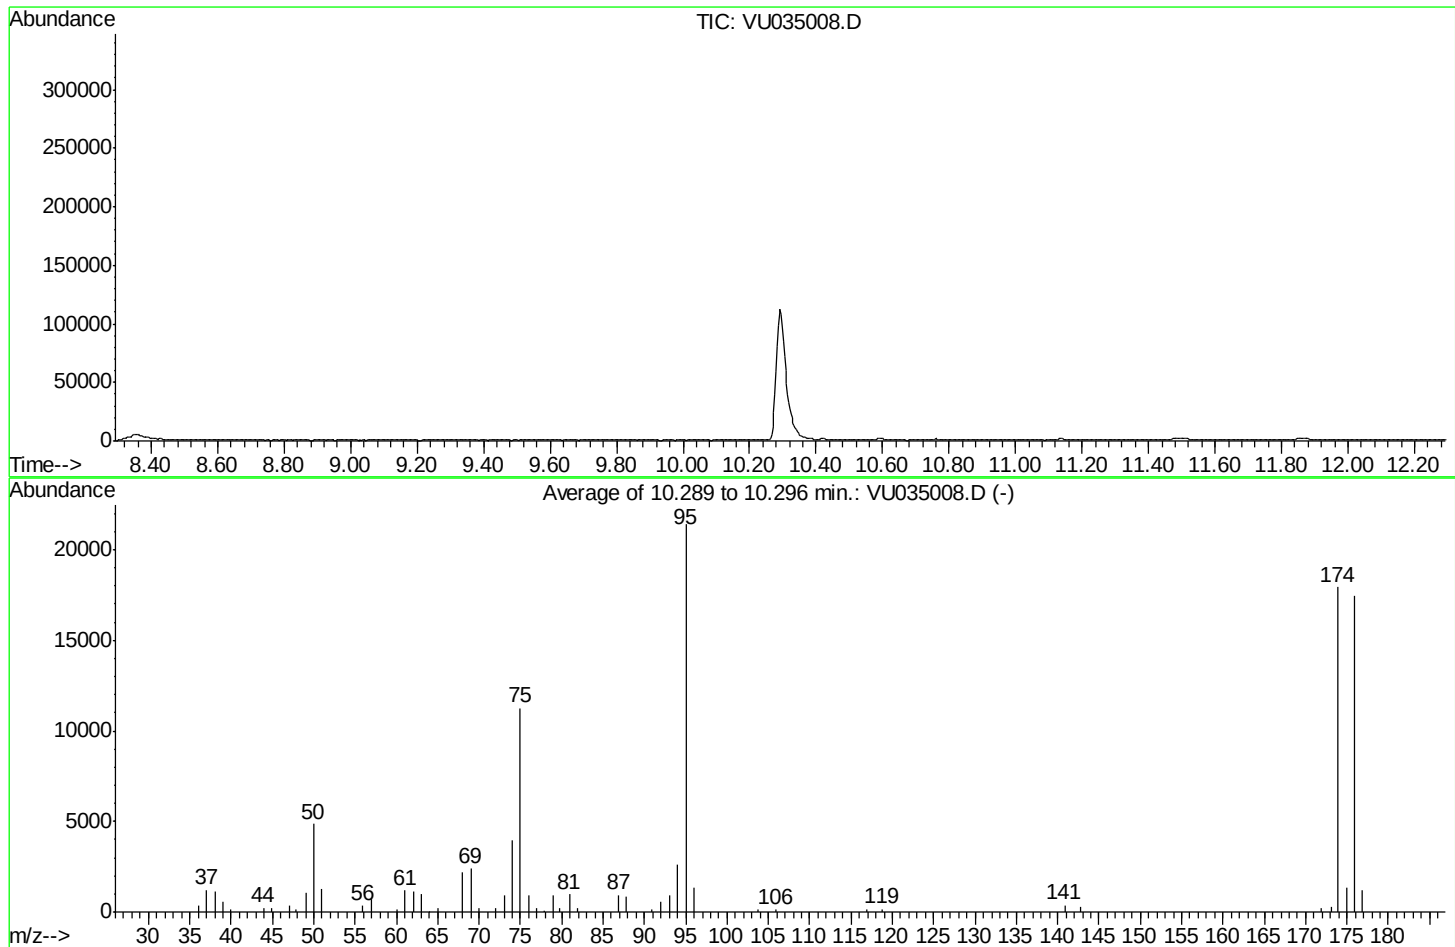

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4859	PASS
75	95	30	80	52.6	11252	PASS
95	95	100	100	100.0	21402	PASS
96	95	5	9	6.4	1375	PASS
173	174	0.00	2	1.6	287	PASS
174	95	50	120	83.8	17936	PASS
175	174	5	9	7.3	1312	PASS
176	174	95	101	97.1	17424	PASS
177	176	5	9	7.0	1221	PASS

m/z	Abundance
36.00	308.0
37.00	1323.0
38.00	1017.0
39.00	531.0
39.90	297.0
44.00	843.0
44.80	228.0
47.00	360.0
47.90	162.0
49.00	1049.0
50.00	4893.0
51.00	1403.0
55.90	376.0
57.00	759.0
60.00	180.0
61.00	1207.0
62.00	1027.0
63.00	1016.0
65.00	182.0
68.00	2128.0
69.00	2410.0
70.00	216.0
72.00	181.0
73.00	914.0
74.00	3890.0
75.00	11637.0
76.00	967.0
77.00	315.0
77.90	116.0
78.90	942.0
79.80	277.0
81.00	904.0
81.90	190.0
86.90	945.0
87.80	785.0
90.80	136.0
91.90	652.0
93.00	981.0
94.00	2764.0
95.00	21048.0
96.00	1417.0
103.80	107.0
106.00	129.0
116.90	203.0
118.80	152.0
140.90	358.0
142.80	311.0
171.90	211.0
173.10	252.0
173.90	17496.0
175.00	1292.0
175.90	17024.0
176.90	1161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	348.0
37.00	1225.0
38.00	1181.0
39.00	551.0
39.90	320.0
44.00	796.0
44.90	217.0
47.00	348.0
47.90	160.0
49.00	1072.0
50.00	5036.0
51.00	1293.0
55.90	368.0
57.00	774.0
60.00	176.0
61.00	1206.0
62.00	1134.0
63.00	976.0
65.00	208.0
68.00	2251.0
69.00	2437.0
70.00	217.0
71.90	198.0
73.00	945.0
74.00	4023.0
75.00	11456.0
76.00	925.0
77.00	234.0
78.90	993.0
79.80	210.0
80.90	1003.0
81.80	186.0
86.90	952.0
87.80	836.0
90.90	102.0
91.90	597.0
93.00	899.0
94.00	2674.0
95.00	21920.0
96.00	1397.0
103.80	126.0
106.00	122.0
116.90	164.0
118.80	192.0
140.90	374.0
142.80	331.0
171.90	213.0
173.10	287.0
173.90	18232.0
174.90	1331.0
175.90	17768.0
176.90	1215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	342.0
37.00	1097.0
38.00	1308.0
39.00	575.0
39.90	279.0
43.90	757.0
44.90	189.0
47.00	267.0
47.90	152.0
49.00	961.0
50.00	4650.0
51.00	1116.0
55.90	313.0
57.00	697.0
60.00	158.0
61.00	1109.0
62.10	1145.0
63.00	919.0
64.00	106.0
65.00	206.0
68.00	2126.0
69.00	2314.0
70.00	194.0
71.90	192.0
73.00	963.0
74.00	3914.0
75.00	10664.0
76.00	891.0
76.90	141.0
78.90	908.0
79.80	150.0
80.90	992.0
81.90	180.0
86.90	898.0
87.90	849.0
90.90	100.0
92.00	535.0
93.00	877.0
94.00	2412.0
95.00	21240.0
96.00	1313.0
103.80	113.0
105.90	104.0
116.90	123.0
118.80	179.0
140.90	361.0
142.80	289.0
171.90	233.0
173.10	322.0
173.90	18080.0
174.90	1315.0
175.90	17480.0
176.90	1288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

Scan 2850 (10.254 min): VU035008.D
BFB43

m/z	Abundance
40.00	178.0
44.00	585.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43