


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101020\
 Data File : VU040624.D
 Acq On : 10 Oct 2020 09:58
 Operator : SY/MD
 Sample : BFB34
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB204

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 12 01:29:55 2020

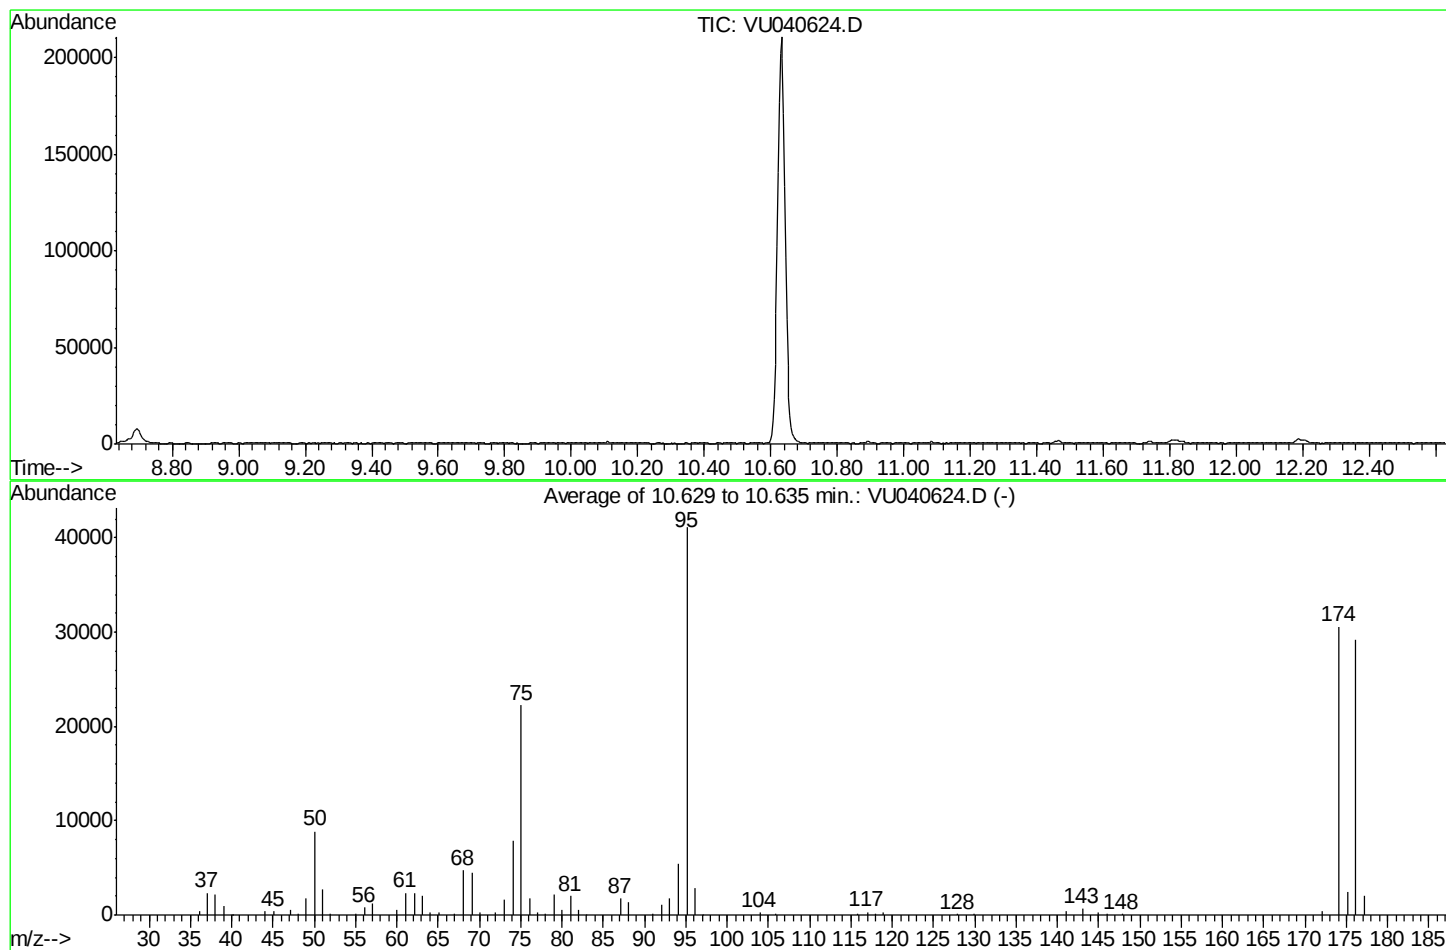

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	8886	PASS
75	95	30	80	54.1	22250	PASS
95	95	100	100	100.0	41114	PASS
96	95	5	9	6.9	2828	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.3	30554	PASS
175	174	5	9	7.9	2402	PASS
176	174	95	101	95.3	29133	PASS
177	176	5	9	7.1	2063	PASS

m/z	Abundance
36.10	537.0
37.00	2335.0
38.10	2512.0
39.00	1056.0
40.10	163.0
44.00	723.0
45.10	419.0
47.20	538.0
48.10	202.0
49.00	1887.0
50.10	9025.0
51.00	2763.0
52.00	166.0
55.10	104.0
56.10	768.0
57.00	1128.0
60.00	546.0
61.10	2319.0
62.10	2300.0
63.10	1859.0
64.00	296.0
65.10	301.0
68.00	4749.0
69.10	4393.0
70.00	337.0
72.00	321.0
73.00	1602.0
74.10	7917.0
75.10	22184.0
76.10	1974.0
77.00	299.0
78.00	142.0
79.00	2087.0
80.00	547.0
81.00	1921.0
82.00	474.0
87.10	1735.0
88.00	1379.0
90.90	133.0
92.00	1082.0
93.10	1879.0
94.10	5415.0
95.10	40928.0
96.10	2873.0
97.00	109.0
103.90	251.0
106.00	172.0
115.80	175.0
117.00	299.0
118.00	174.0
119.00	331.0
141.10	421.0
143.00	575.0
145.00	205.0
145.90	123.0
147.90	143.0
172.00	461.0
174.10	29616.0
175.10	2465.0
176.10	28328.0
177.10	1992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB204

m/z	Abundance
36.10	453.0
37.00	2406.0
38.10	2349.0
39.00	1000.0
39.90	153.0
44.00	752.0
45.00	410.0
47.20	587.0
48.00	201.0
49.00	1878.0
50.10	9107.0
51.10	2870.0
52.00	202.0
55.10	183.0
56.10	780.0
57.00	1264.0
60.00	546.0
61.00	2383.0
62.10	2389.0
63.10	2043.0
64.00	356.0
65.10	335.0
66.90	156.0
68.00	4844.0
69.10	4581.0
70.00	337.0
72.00	300.0
73.00	1673.0
74.10	8265.0
75.10	22920.0
76.10	1866.0
77.00	330.0
77.90	126.0
79.00	2250.0
80.00	573.0
81.00	2052.0
82.00	559.0
87.00	1823.0
88.00	1373.0
91.00	154.0
92.00	1145.0
93.00	1787.0
94.10	5577.0
95.10	42536.0
96.10	2971.0
104.00	275.0
106.00	203.0
115.80	193.0
117.00	335.0
118.00	165.0
118.90	319.0
127.90	120.0
129.90	102.0
141.00	432.0
143.00	674.0
145.00	246.0
146.00	104.0
147.80	131.0
172.10	383.0
174.10	31472.0
175.10	2490.0
176.10	30128.0
177.10	2132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB204

m/z	Abundance
36.00	345.0
37.00	2368.0
38.00	1836.0
39.10	851.0
39.90	125.0
40.20	114.0
44.00	627.0
45.00	359.0
47.10	527.0
47.90	191.0
49.00	1689.0
50.10	8528.0
51.10	2676.0
52.00	186.0
55.10	209.0
56.00	739.0
57.00	1288.0
59.90	512.0
61.00	2330.0
62.10	2226.0
63.10	2079.0
64.00	308.0
65.10	352.0
66.90	196.0
68.00	4474.0
69.10	4450.0
70.00	282.0
72.00	257.0
73.10	1743.0
74.10	7468.0
75.10	21648.0
76.10	1651.0
77.00	296.0
77.90	160.0
79.00	2202.0
80.00	540.0
81.00	1956.0
82.00	535.0
82.90	101.0
87.00	1736.0
88.10	1330.0
91.00	148.0
92.00	1156.0
93.10	1737.0
94.10	5116.0
95.10	39880.0
96.10	2641.0
104.00	274.0
105.90	222.0
115.80	181.0
117.00	387.0
118.00	143.0
118.90	269.0
127.90	123.0
129.90	125.0
141.00	448.0
143.00	746.0
145.00	246.0
147.80	120.0
172.10	364.0
174.10	30576.0
175.10	2253.0
176.10	28944.0
177.10	2065.0

Instrument :
MSVOA_U
ClientSampleId :
BFB204

Scan 2877 (10.590 min): VU040624.D
BFB34

m/z	Abundance
40.00	124.0
44.00	353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB204