

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051318.D
 Acq On : 10 Oct 2022 11:34
 Operator : JC/MD
 Sample : N4922-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB8W0

Quant Time: Oct 11 00:59:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	190734	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	208891	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	79430	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	56212	3.654	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.000%	
7) Chloroethane-d5	1.912	69	56839	4.300	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.000%	
11) 1,1-Dichloroethene-d2	2.562	65	24047	3.954	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.000%	
20) 2-Butanone-d5	4.639	46	179754	53.066	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.140%	
24) Chloroform-d	5.060	84	140216	4.888	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.700	65	76777	5.190	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.800%	
32) Benzene-d6	5.726	84	248369	4.322	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.400%	
36) 1,2-Dichloropropane-d6	6.690	67	91865	4.707	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.200%	
41) Toluene-d8	7.896	98	190523	3.706	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.200%	
43) trans-1,3-Dichloroprop...	8.179	79	29097	4.538	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.800%	
46) 2-Hexanone-d5	8.632	63	94946	43.936	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.880%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	74537	4.781	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.600%	
66) 1,2-Dichlorobenzene-d4	12.192	152	69463	5.031	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.600%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.517	50	8149	0.373	ug/L	96
13) Acetone	2.649	43	14954	5.886	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051318.D
Acq On : 10 Oct 2022 11:34
Operator : JC/MD
Sample : N4922-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB8W0

Quant Time: Oct 11 00:59:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration




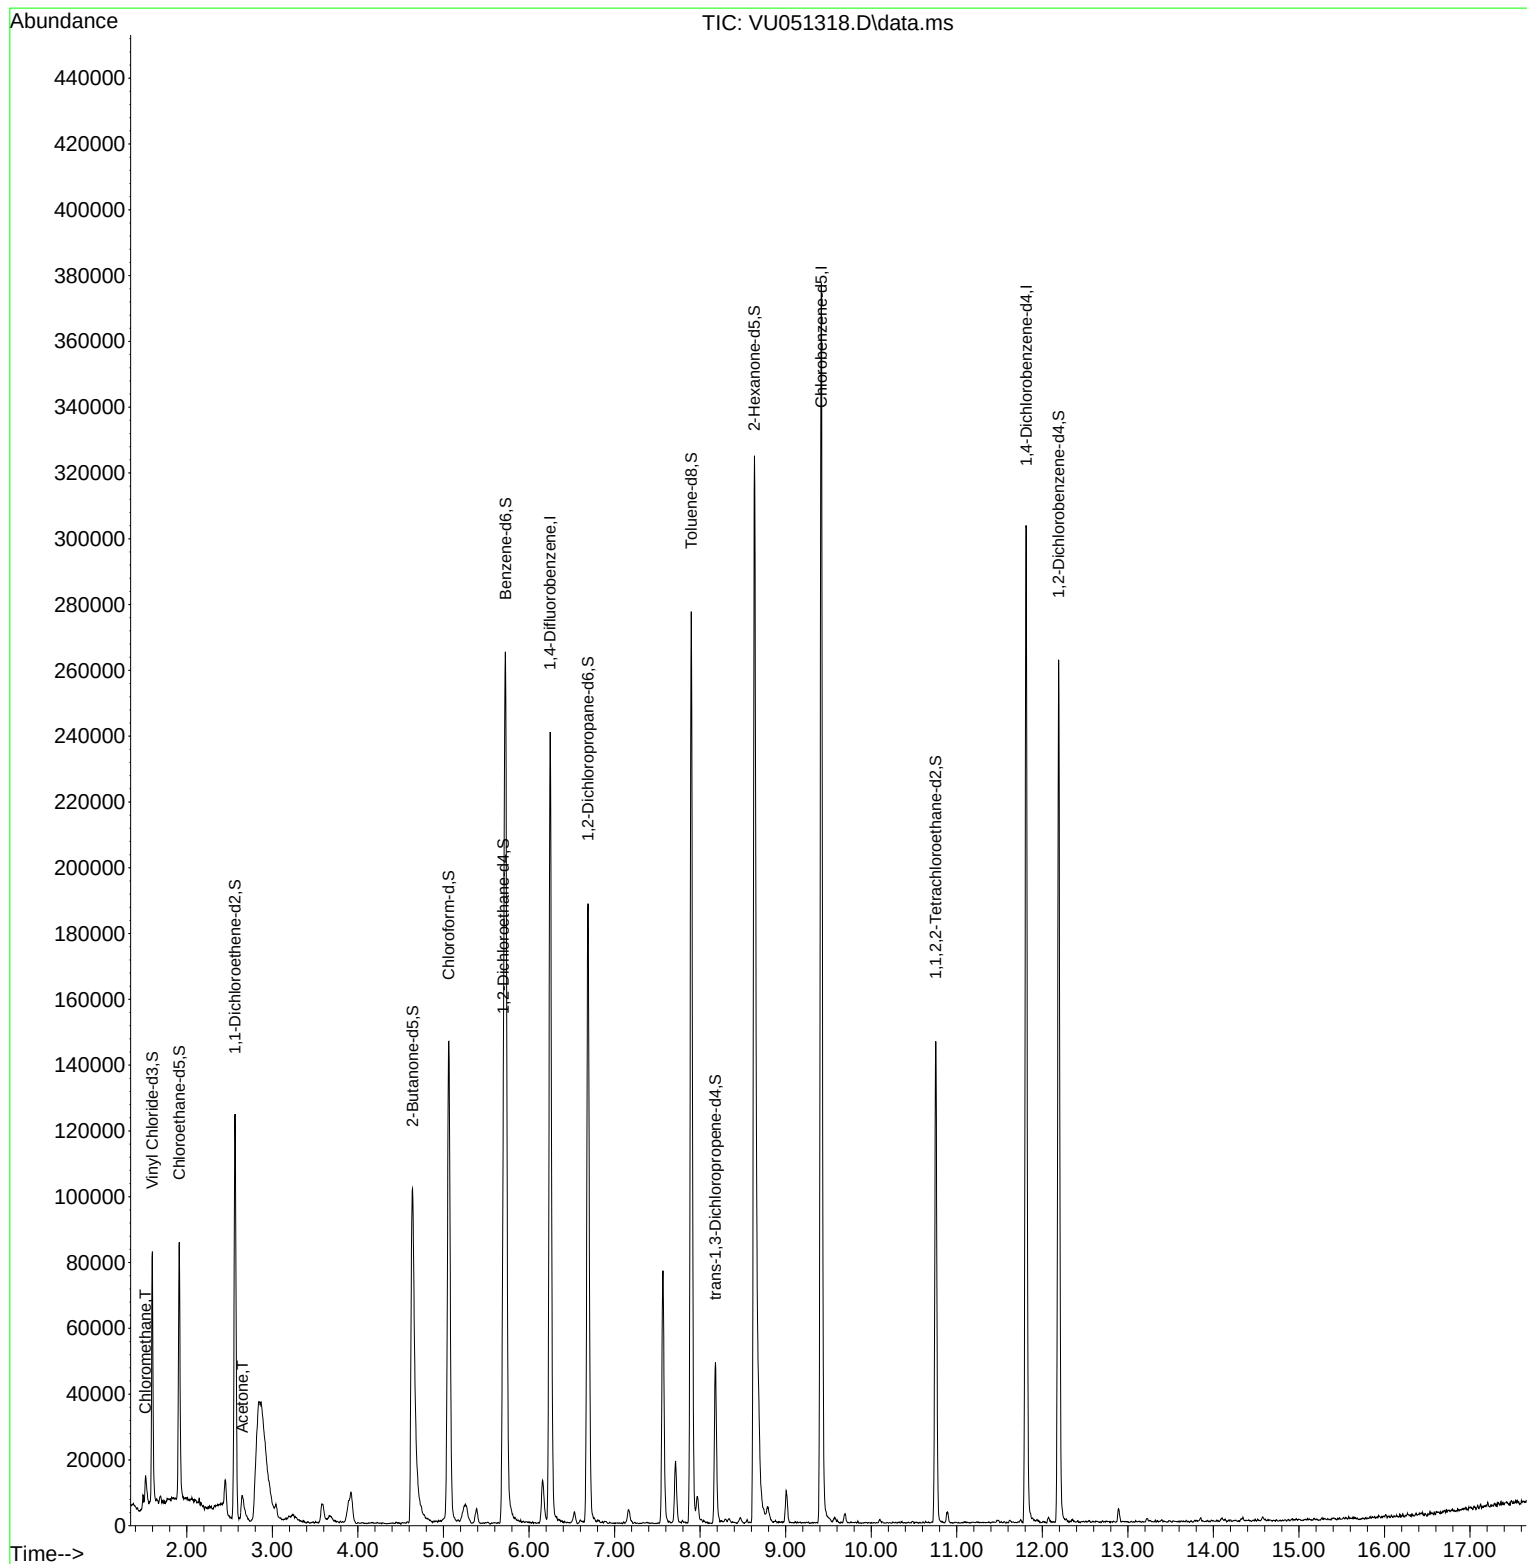


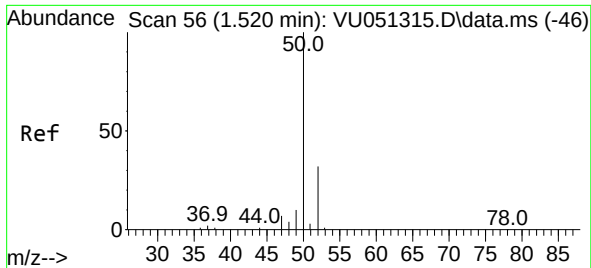

#3
Chloromethane
Concen: 0.373 ug/L
RT: 1.517 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU051318.D
Acq: 10 Oct 2022 11:34

Instrument :
MSVOA_U
ClientSampleId :
CB8W0

Tgt Ion: 50 Resp: 8149
Ion Ratio Lower Upper
50 100
52 34.7 22.9 42.5

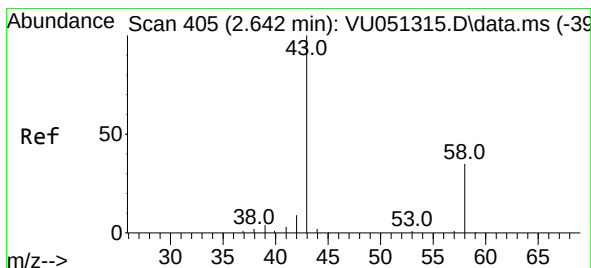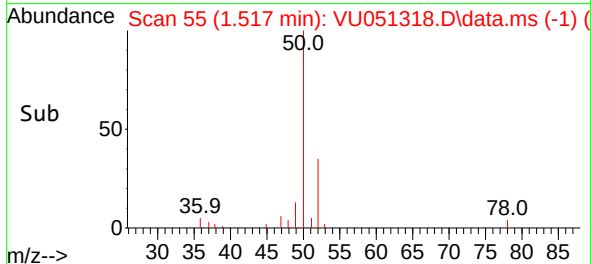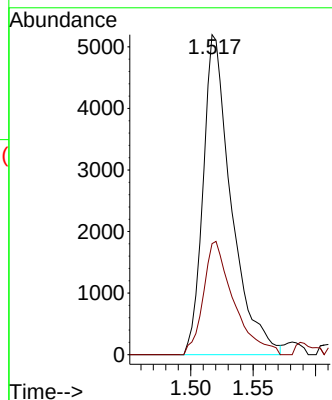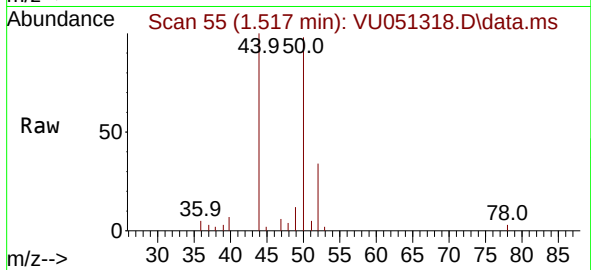

#13
Acetone
Concen: 5.886 ug/L
RT: 2.649 min Scan# 407
Delta R.T. 0.006 min
Lab File: VU051318.D
Acq: 10 Oct 2022 11:34

Tgt Ion: 43 Resp: 14954
Ion Ratio Lower Upper
43 100
58 32.5 0.0 68.8

