

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051325.D
 Acq On : 10 Oct 2022 14:25
 Operator : JC/MD
 Sample : N5049-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT4

Quant Time: Oct 11 01:01:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	189740	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	212009	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	83049	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	54467	3.559	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.200%
7) Chloroethane-d5	1.909	69	54727	4.162	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.200%
11) 1,1-Dichloroethene-d2	2.562	65	23151	3.827	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.600%
20) 2-Butanone-d5	4.620	46	188584	55.964	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.920%
24) Chloroform-d	5.060	84	135124	4.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.700	65	73672	5.006	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.200%
32) Benzene-d6	5.726	84	238597	4.091	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	6.690	67	88547	4.470	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.896	98	177670	3.405	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	8.179	79	27237	4.185	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.800%
46) 2-Hexanone-d5	8.632	63	105180	47.956	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.920%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	77645	4.907	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	69566	4.819	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						Qvalue
13) Acetone	2.629	43	8470	3.351	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051325.D
Acq On : 10 Oct 2022 14:25
Operator : JC/MD
Sample : N5049-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT4

Quant Time: Oct 11 01:01:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration

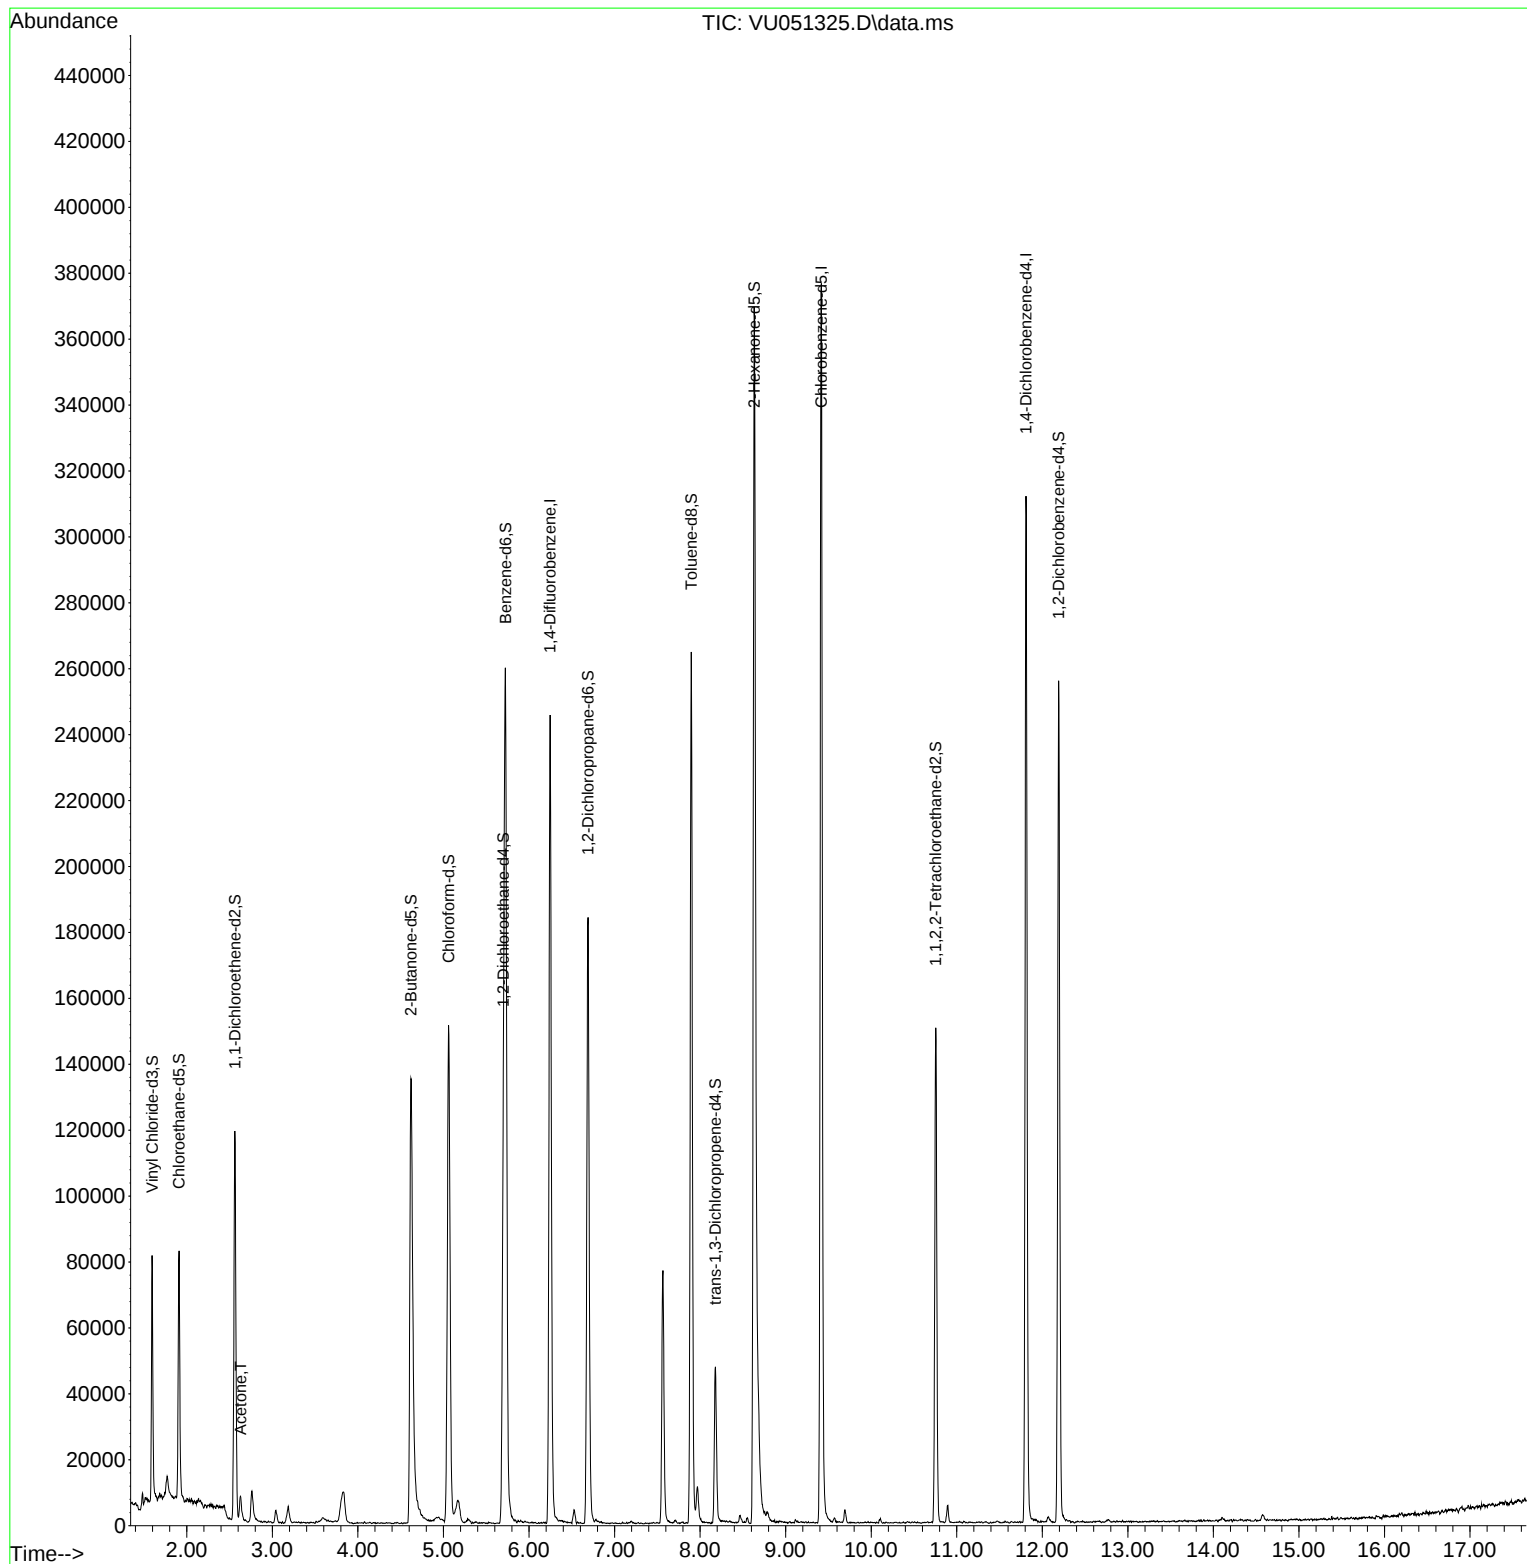

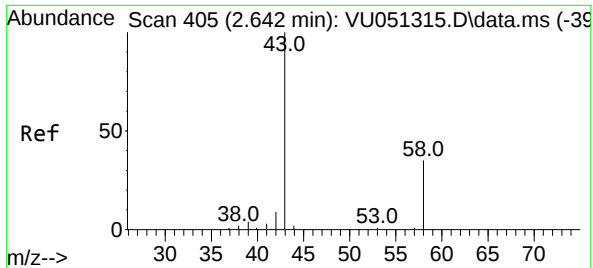

#13
 Acetone
 Concen: 3.351 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. -0.013 min
 Lab File: VU051325.D
 Acq: 10 Oct 2022 14:25

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT4

Tgt Ion: 43 Resp: 8470
 Ion Ratio Lower Upper
 43 100
 58 39.3 0.0 68.8

