

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051334.D
 Acq On : 10 Oct 2022 18:06
 Operator : JC/MD
 Sample : N5026-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX8

Quant Time: Oct 11 01:03:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	177405	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	199741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	76517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50378	3.520	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.400%
7) Chloroethane-d5	1.912	69	53757	4.372	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%
11) 1,1-Dichloroethene-d2	2.565	65	21935	3.878	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%
20) 2-Butanone-d5	4.620	46	157083	49.857	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.720%
24) Chloroform-d	5.063	84	131179	4.917	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.700	65	69883	5.079	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.726	84	228190	4.153	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.690	67	85616	4.588	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.800%
41) Toluene-d8	7.896	98	170180	3.462	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.200%#
43) trans-1,3-Dichloroprop...	8.179	79	24500	3.996	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.632	63	85385	41.322	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.640%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	72047	4.833	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	64468	4.847	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
13) Acetone	2.623	43	12296	5.203	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051334.D
Acq On : 10 Oct 2022 18:06
Operator : JC/MD
Sample : N5026-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX8

Quant Time: Oct 11 01:03:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration

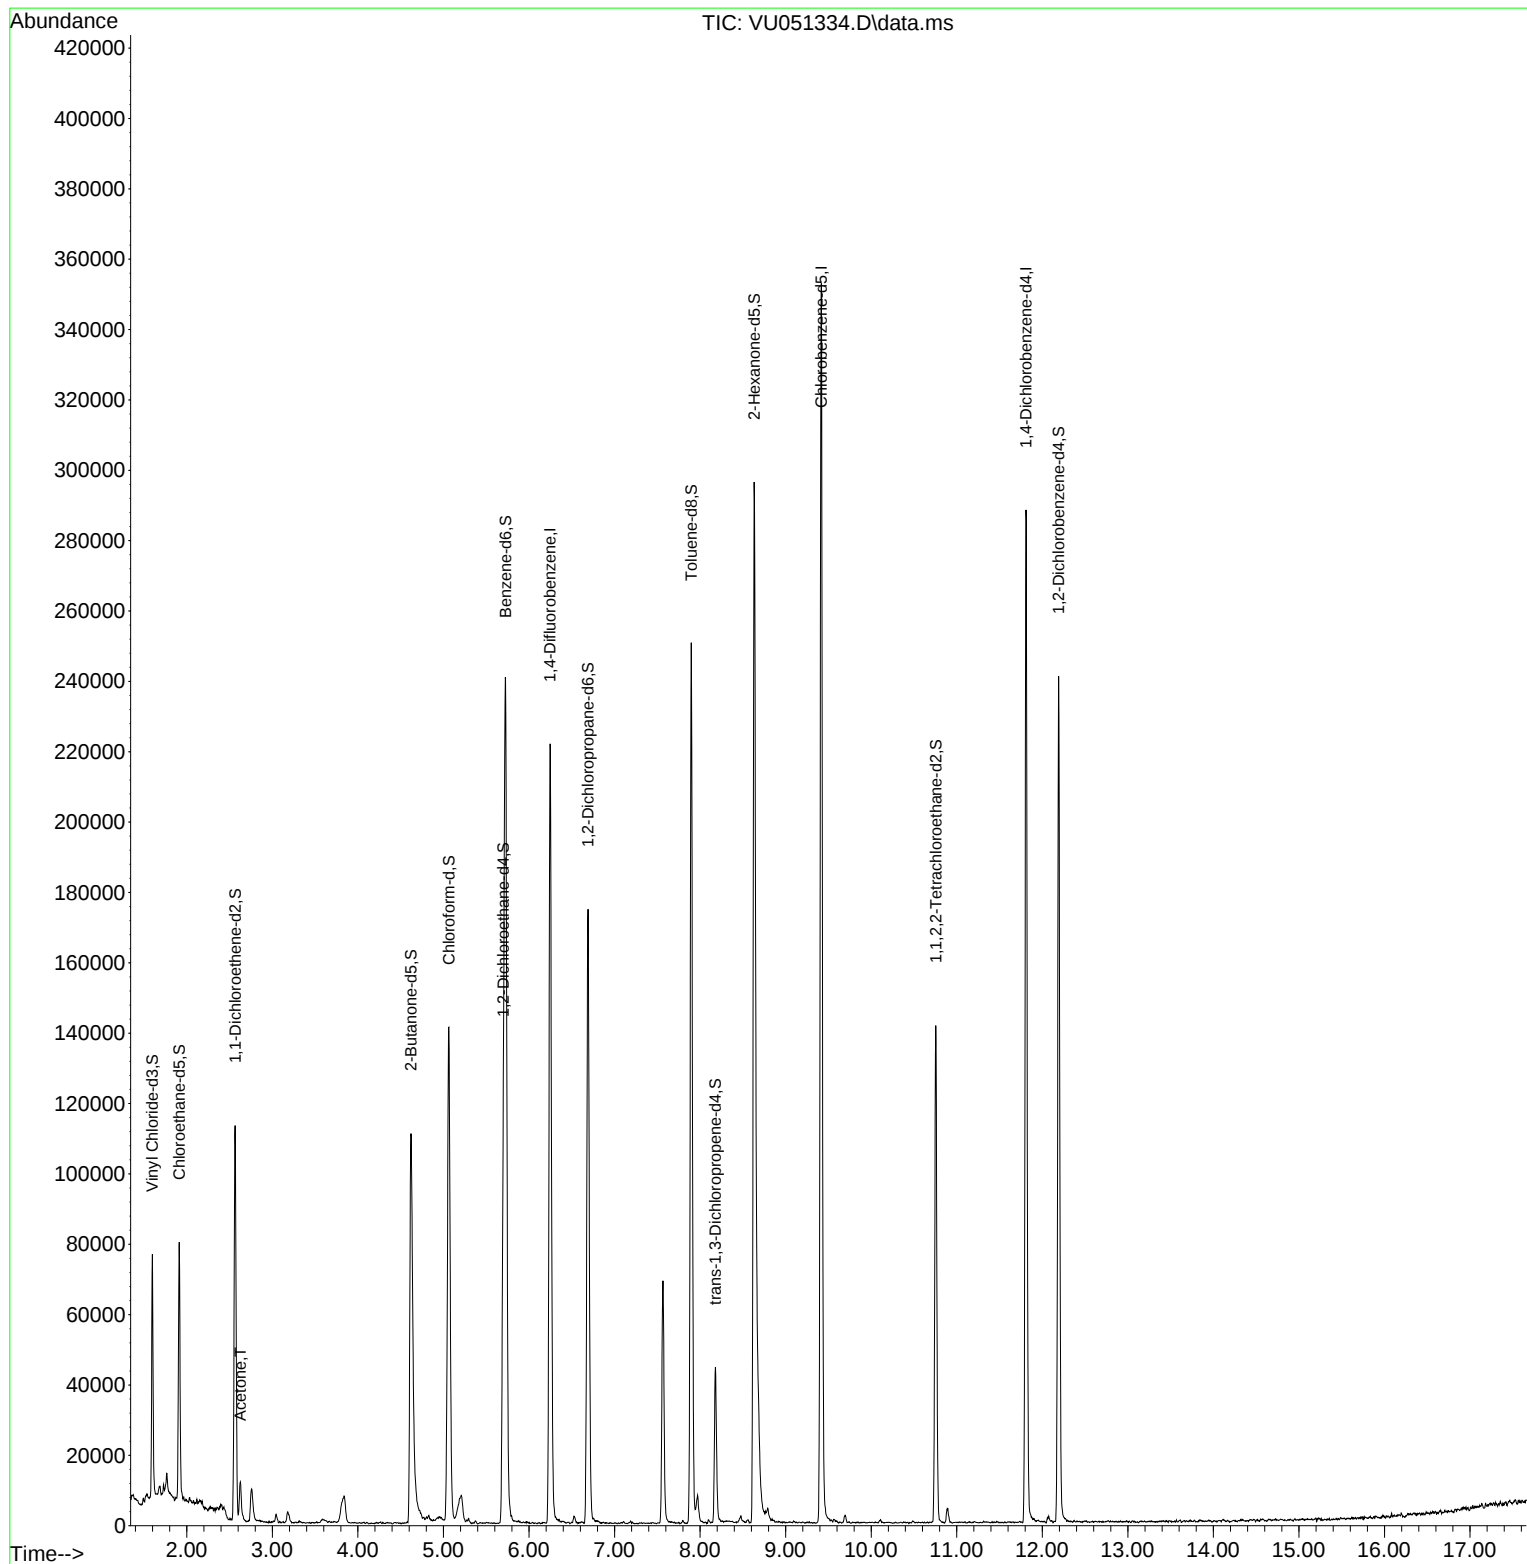

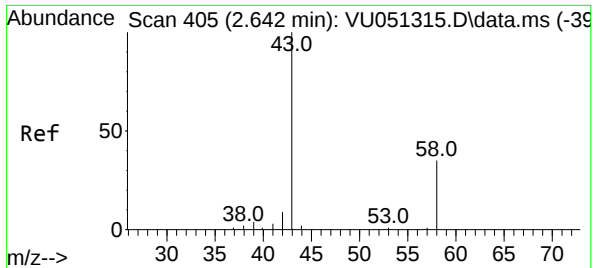

#13
 Acetone
 Concen: 5.203 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. -0.019 min
 Lab File: VU051334.D
 Acq: 10 Oct 2022 18:06

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX8

Tgt Ion: 43 Resp: 12296
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 68.8

