

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051337.D
 Acq On : 10 Oct 2022 19:20
 Operator : JC/MD
 Sample : N5026-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX4

Quant Time: Oct 11 01:03:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	171547	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	198370	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	74085	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51914	3.752	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.912	69	54998	4.626	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.562	65	22513	4.116	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.400%
20) 2-Butanone-d5	4.620	46	161662	53.063	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.120%
24) Chloroform-d	5.060	84	139626	5.412	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.200%
26) 1,2-Dichloroethane-d4	5.700	65	74263	5.582	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.600%
32) Benzene-d6	5.726	84	235772	4.320	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	6.690	67	89532	4.831	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.896	98	176584	3.617	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
43) trans-1,3-Dichloroprop...	8.179	79	25560	4.198	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.629	63	87225	42.504	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.000%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	73668	4.976	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	65434	5.082	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	11385	4.982	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051337.D
Acq On : 10 Oct 2022 19:20
Operator : JC/MD
Sample : N5026-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX4

Quant Time: Oct 11 01:03:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration

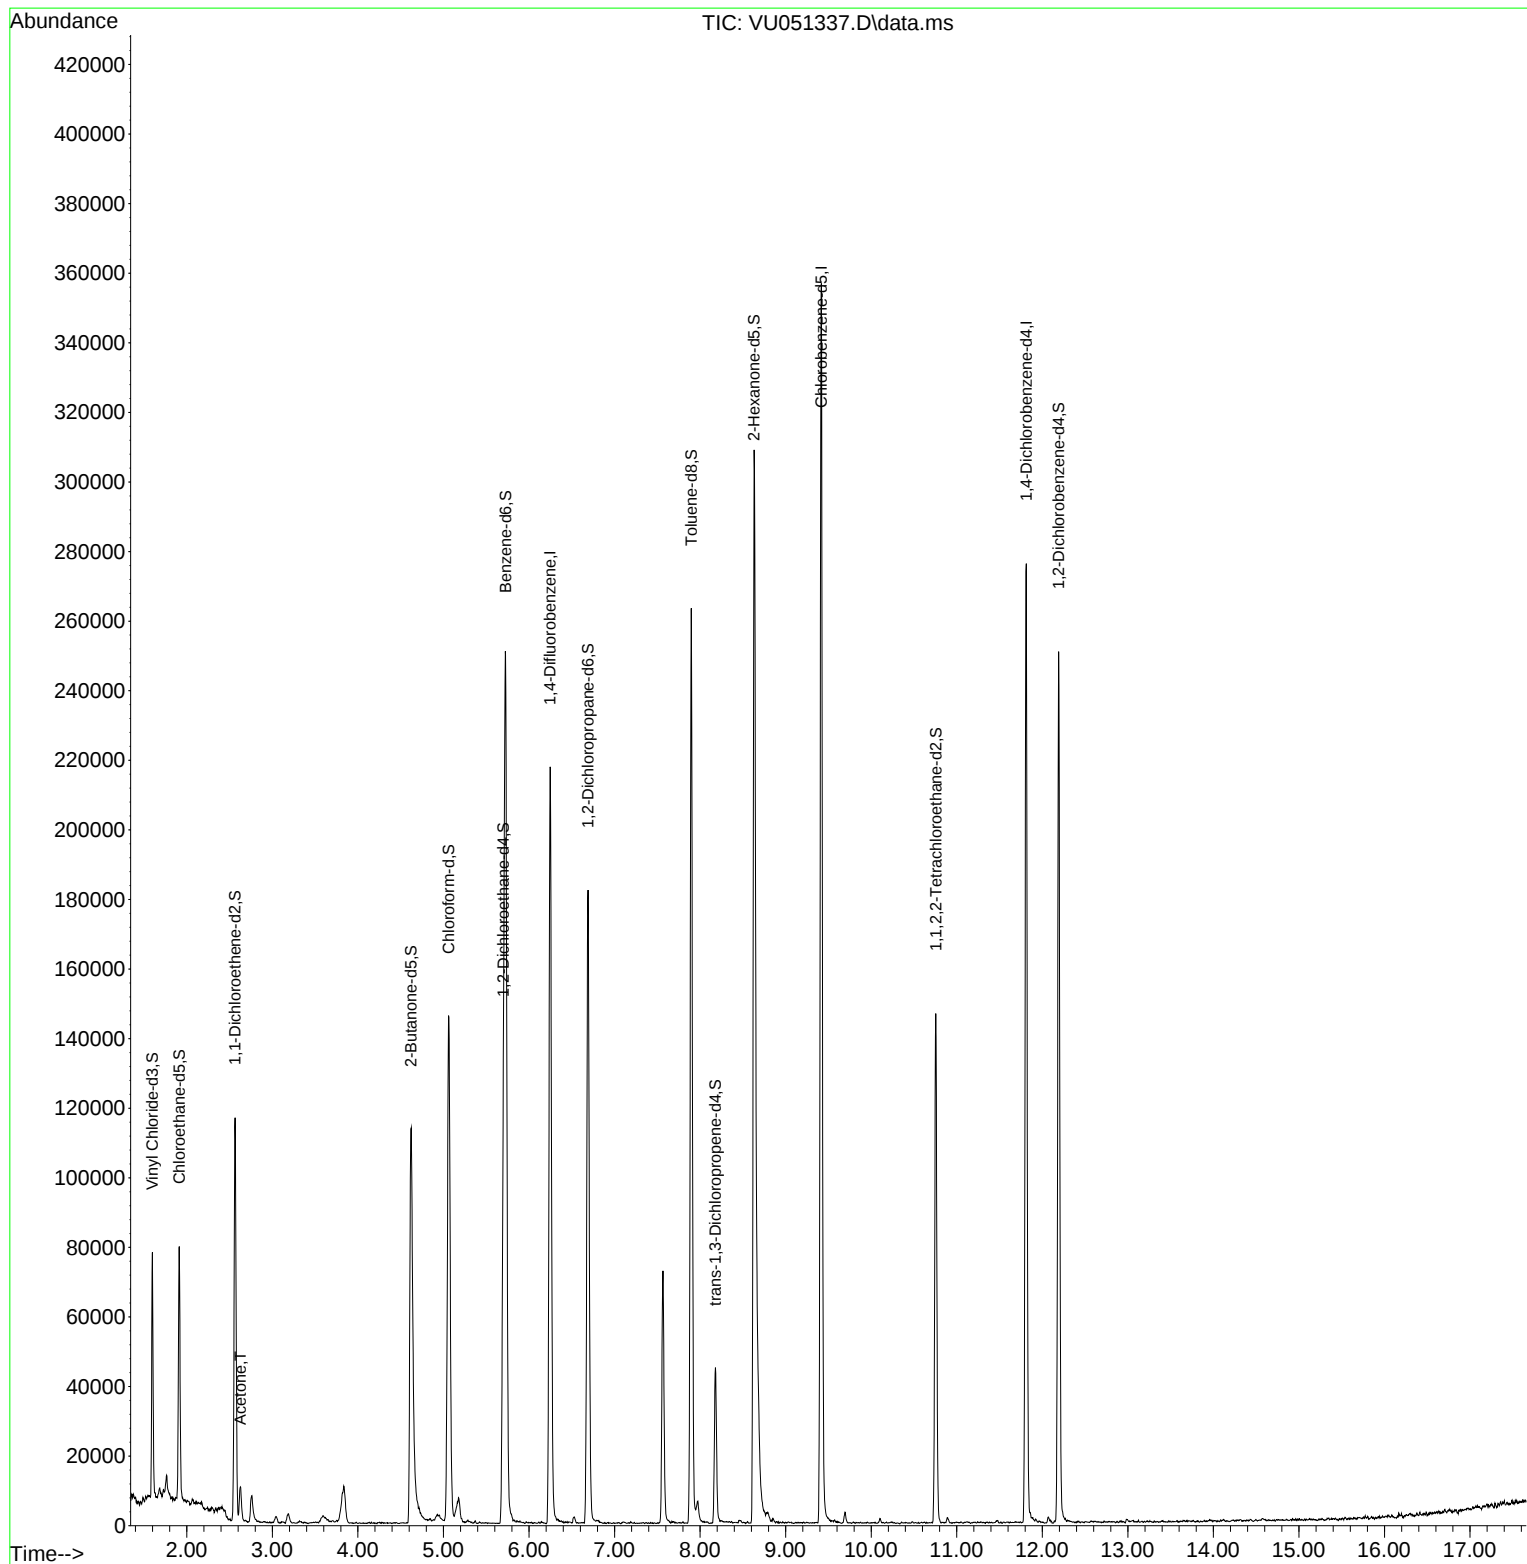

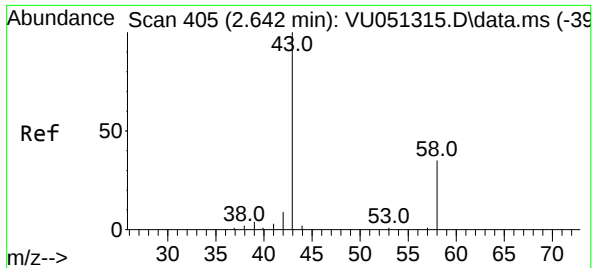

#13
 Acetone
 Concen: 4.982 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.016 min
 Lab File: VU051337.D
 Acq: 10 Oct 2022 19:20

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX4

Tgt Ion: 43 Resp: 11385
 Ion Ratio Lower Upper
 43 100
 58 34.7 0.0 68.8

