

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051338.D
 Acq On : 10 Oct 2022 19:45
 Operator : JC/MD
 Sample : N5026-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX5

Quant Time: Oct 11 01:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	175481	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	196761	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	74409	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	52325	3.697	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.000%
7) Chloroethane-d5	1.912	69	55031	4.525	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.400%
11) 1,1-Dichloroethene-d2	2.565	65	21959	3.924	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	4.620	46	157261	50.461	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.920%
24) Chloroform-d	5.060	84	138180	5.236	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
26) 1,2-Dichloroethane-d4	5.700	65	71867	5.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%
32) Benzene-d6	5.726	84	233670	4.317	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	6.690	67	88378	4.808	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.896	98	176738	3.650	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	8.179	79	26762	4.431	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.600%
46) 2-Hexanone-d5	8.632	63	86919	42.701	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.400%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	74265	5.057	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	66105	5.111	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%
Target Compounds					Qvalue	
13) Acetone	2.626	43	12035	5.149	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051338.D
Acq On : 10 Oct 2022 19:45
Operator : JC/MD
Sample : N5026-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX5

Quant Time: Oct 11 01:04:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration

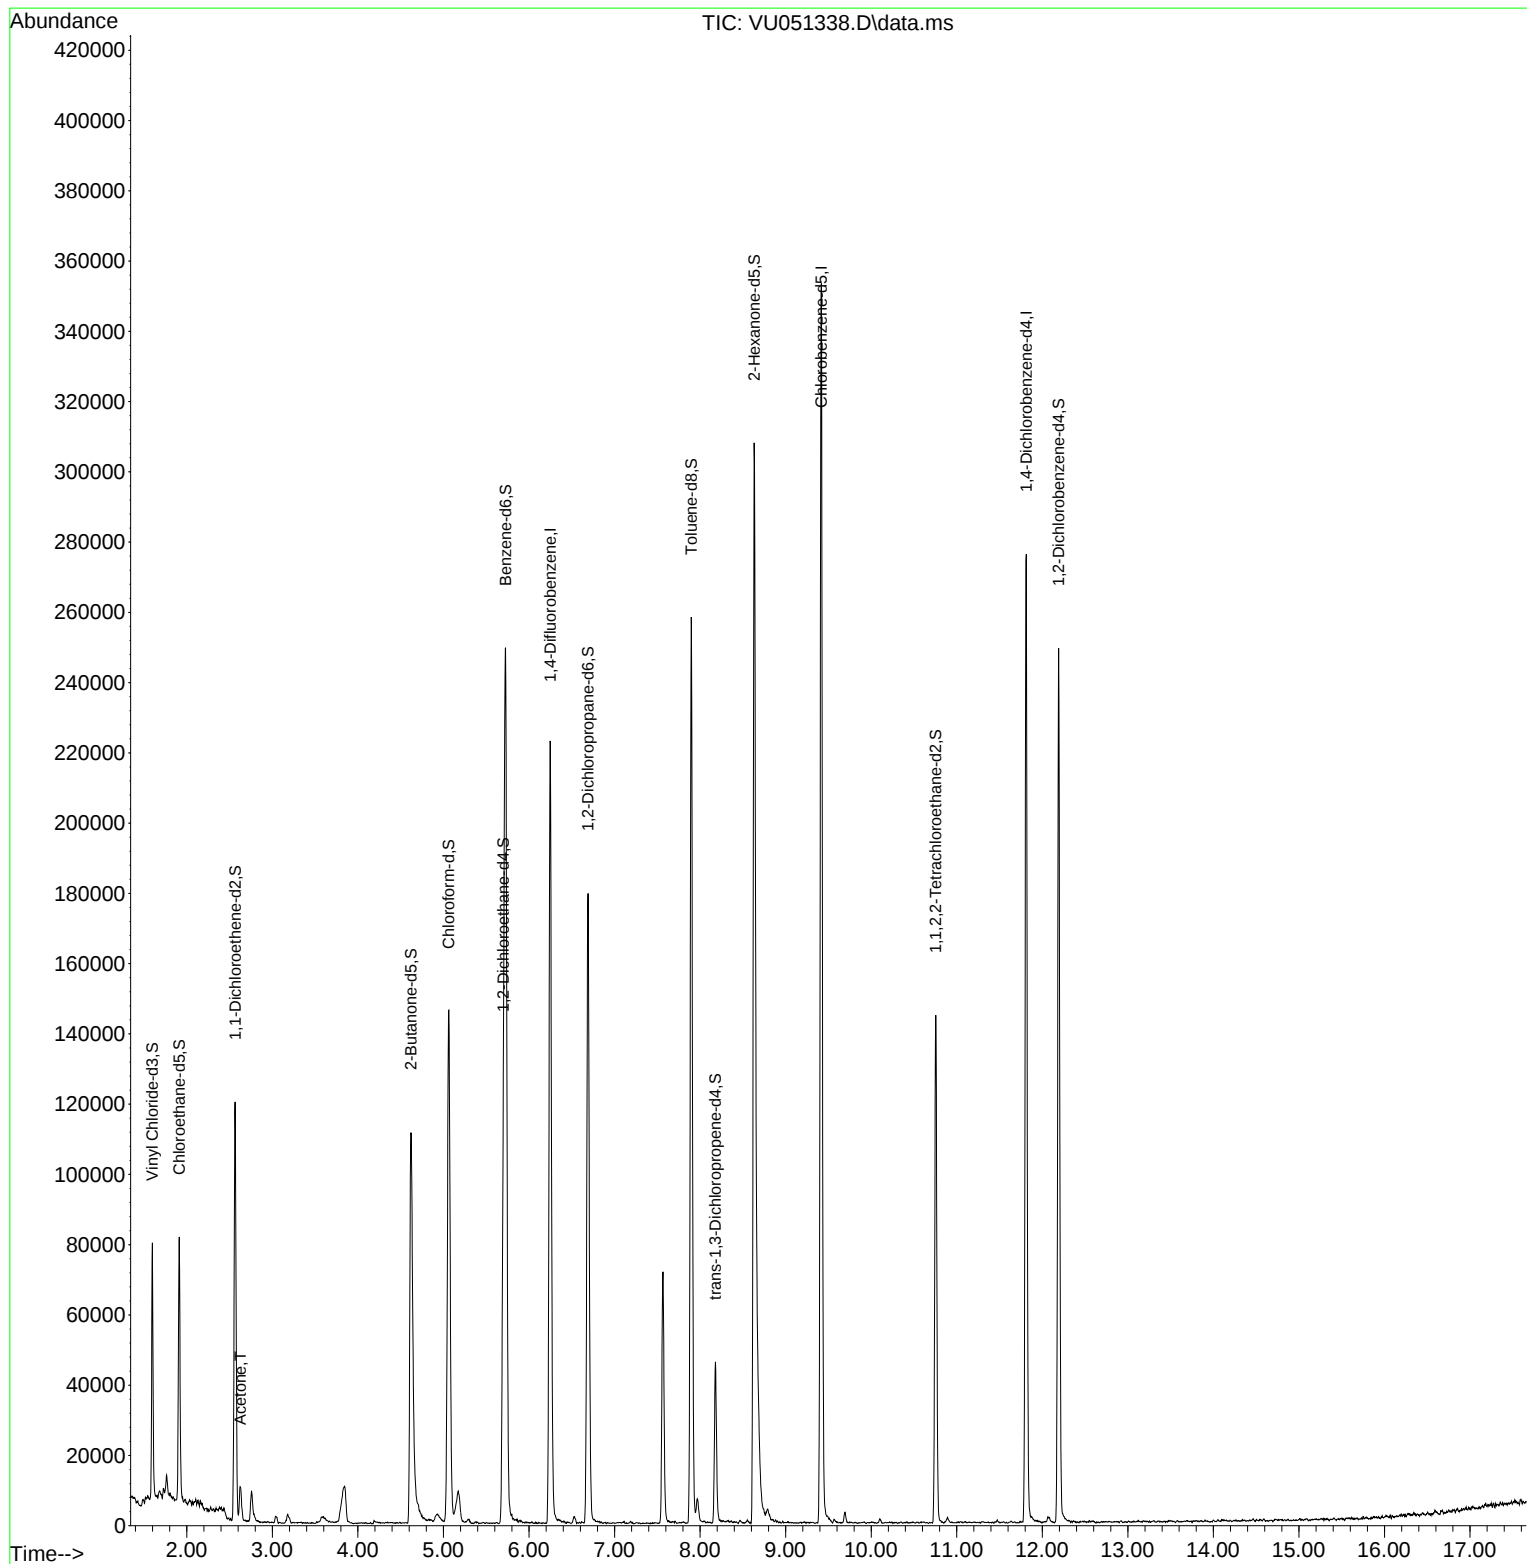

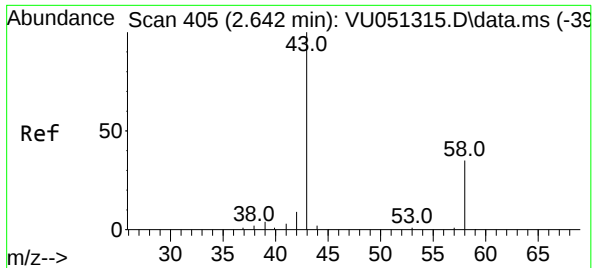

#13
 Acetone
 Concen: 5.149 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.016 min
 Lab File: VU051338.D
 Acq: 10 Oct 2022 19:45

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX5

Tgt Ion: 43 Resp: 12035
 Ion Ratio Lower Upper
 43 100
 58 32.0 0.0 68.8

