

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051339.D
 Acq On : 10 Oct 2022 20:10
 Operator : JC/MD
 Sample : N5026-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX6

Quant Time: Oct 11 01:04:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 00:58:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	172463	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	198468	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	74824	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51428	3.697	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.000%
7) Chloroethane-d5	1.912	69	55071	4.607	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.565	65	21913	3.985	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%
20) 2-Butanone-d5	4.620	46	157497	51.421	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.840%
24) Chloroform-d	5.060	84	134056	5.169	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
26) 1,2-Dichloroethane-d4	5.700	65	71346	5.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.726	84	226853	4.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.690	67	85406	4.606	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%
41) Toluene-d8	7.896	98	169774	3.476	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.600%#
43) trans-1,3-Dichloroprop...	8.179	79	25516	4.188	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.800%
46) 2-Hexanone-d5	8.632	63	82902	40.378	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.760%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	72662	4.906	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	64376	4.950	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds						
13) Acetone	2.626	43	9780	4.257	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051339.D
Acq On : 10 Oct 2022 20:10
Operator : JC/MD
Sample : N5026-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX6

Quant Time: Oct 11 01:04:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 00:58:34 2022
Response via : Initial Calibration

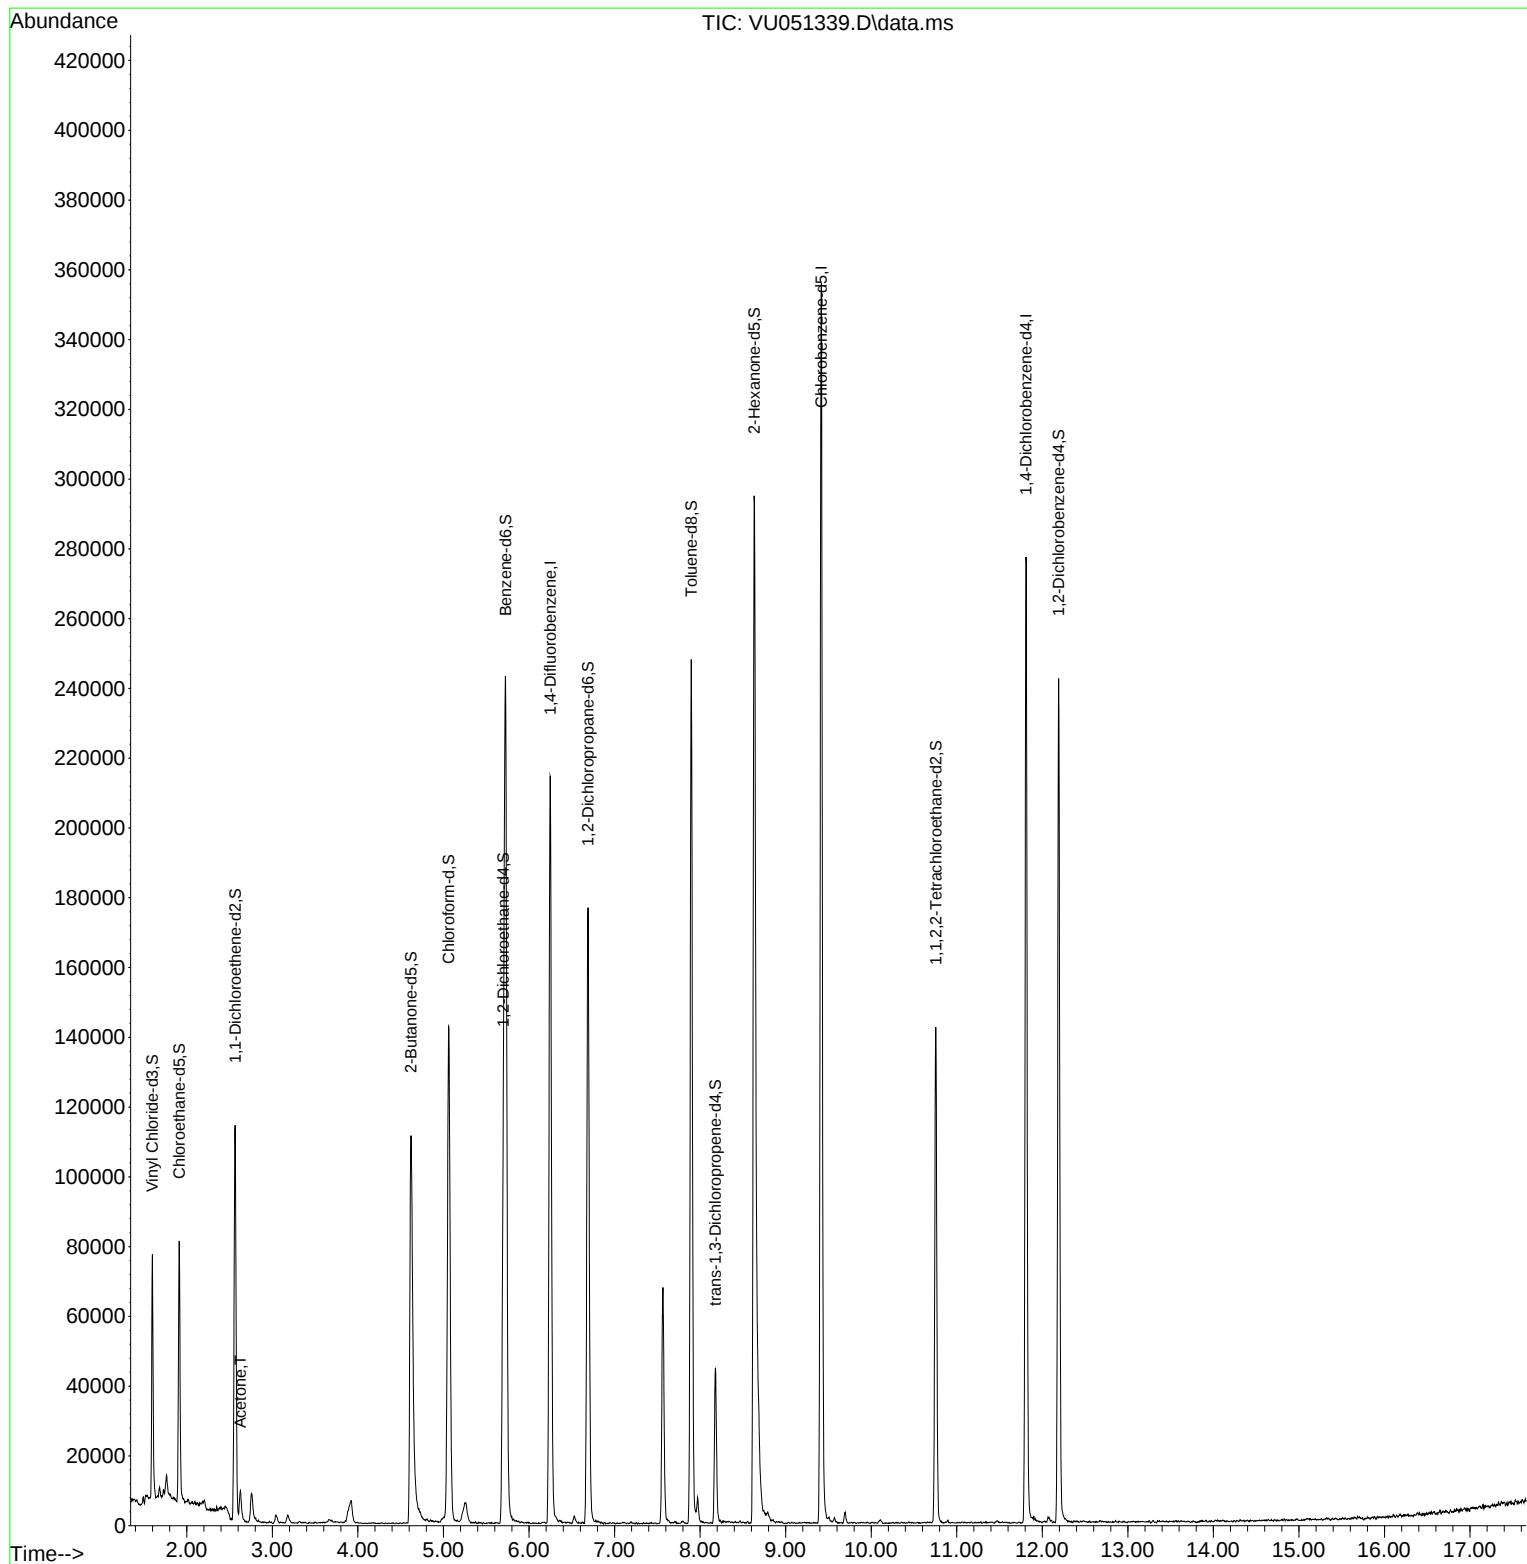

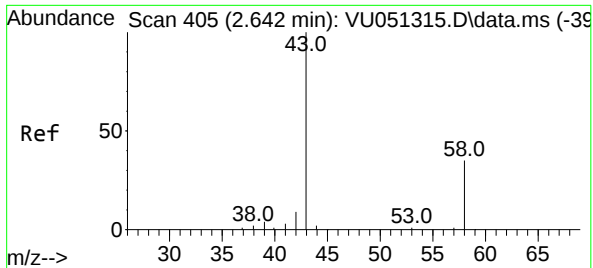

#13
 Acetone
 Concen: 4.257 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.016 min
 Lab File: VU051339.D
 Acq: 10 Oct 2022 20:10

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX6

Tgt Ion: 43 Resp: 9780
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 68.8

