

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051351.D
 Acq On : 11 Oct 2022 01:40
 Operator : JC/MD
 Sample : N5071-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB7

Quant Time: Oct 11 05:57:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	178176	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	210890	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	80658	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	52044	3.621	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.400%
7) Chloroethane-d5	1.909	69	54107	4.381	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.600%
11) 1,1-Dichloroethene-d2	2.562	65	22340	3.932	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.600%
20) 2-Butanone-d5	4.620	46	193798	61.244	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.480%
24) Chloroform-d	5.064	84	137285	5.123	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	5.700	65	76062	5.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.000%
32) Benzene-d6	5.726	84	234607	4.044	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.800%
36) 1,2-Dichloropropane-d6	6.691	67	90780	4.607	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%
41) Toluene-d8	7.896	98	174027	3.353	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.000%#
43) trans-1,3-Dichloroprop...	8.179	79	26546	4.101	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.633	63	102918	47.174	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.340%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	82460	5.239	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	69813	4.980	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds					Qvalue	
13) Acetone	2.623	43	10850	4.572	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051351.D
Acq On : 11 Oct 2022 01:40
Operator : JC/MD
Sample : N5071-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB7

Quant Time: Oct 11 05:57:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

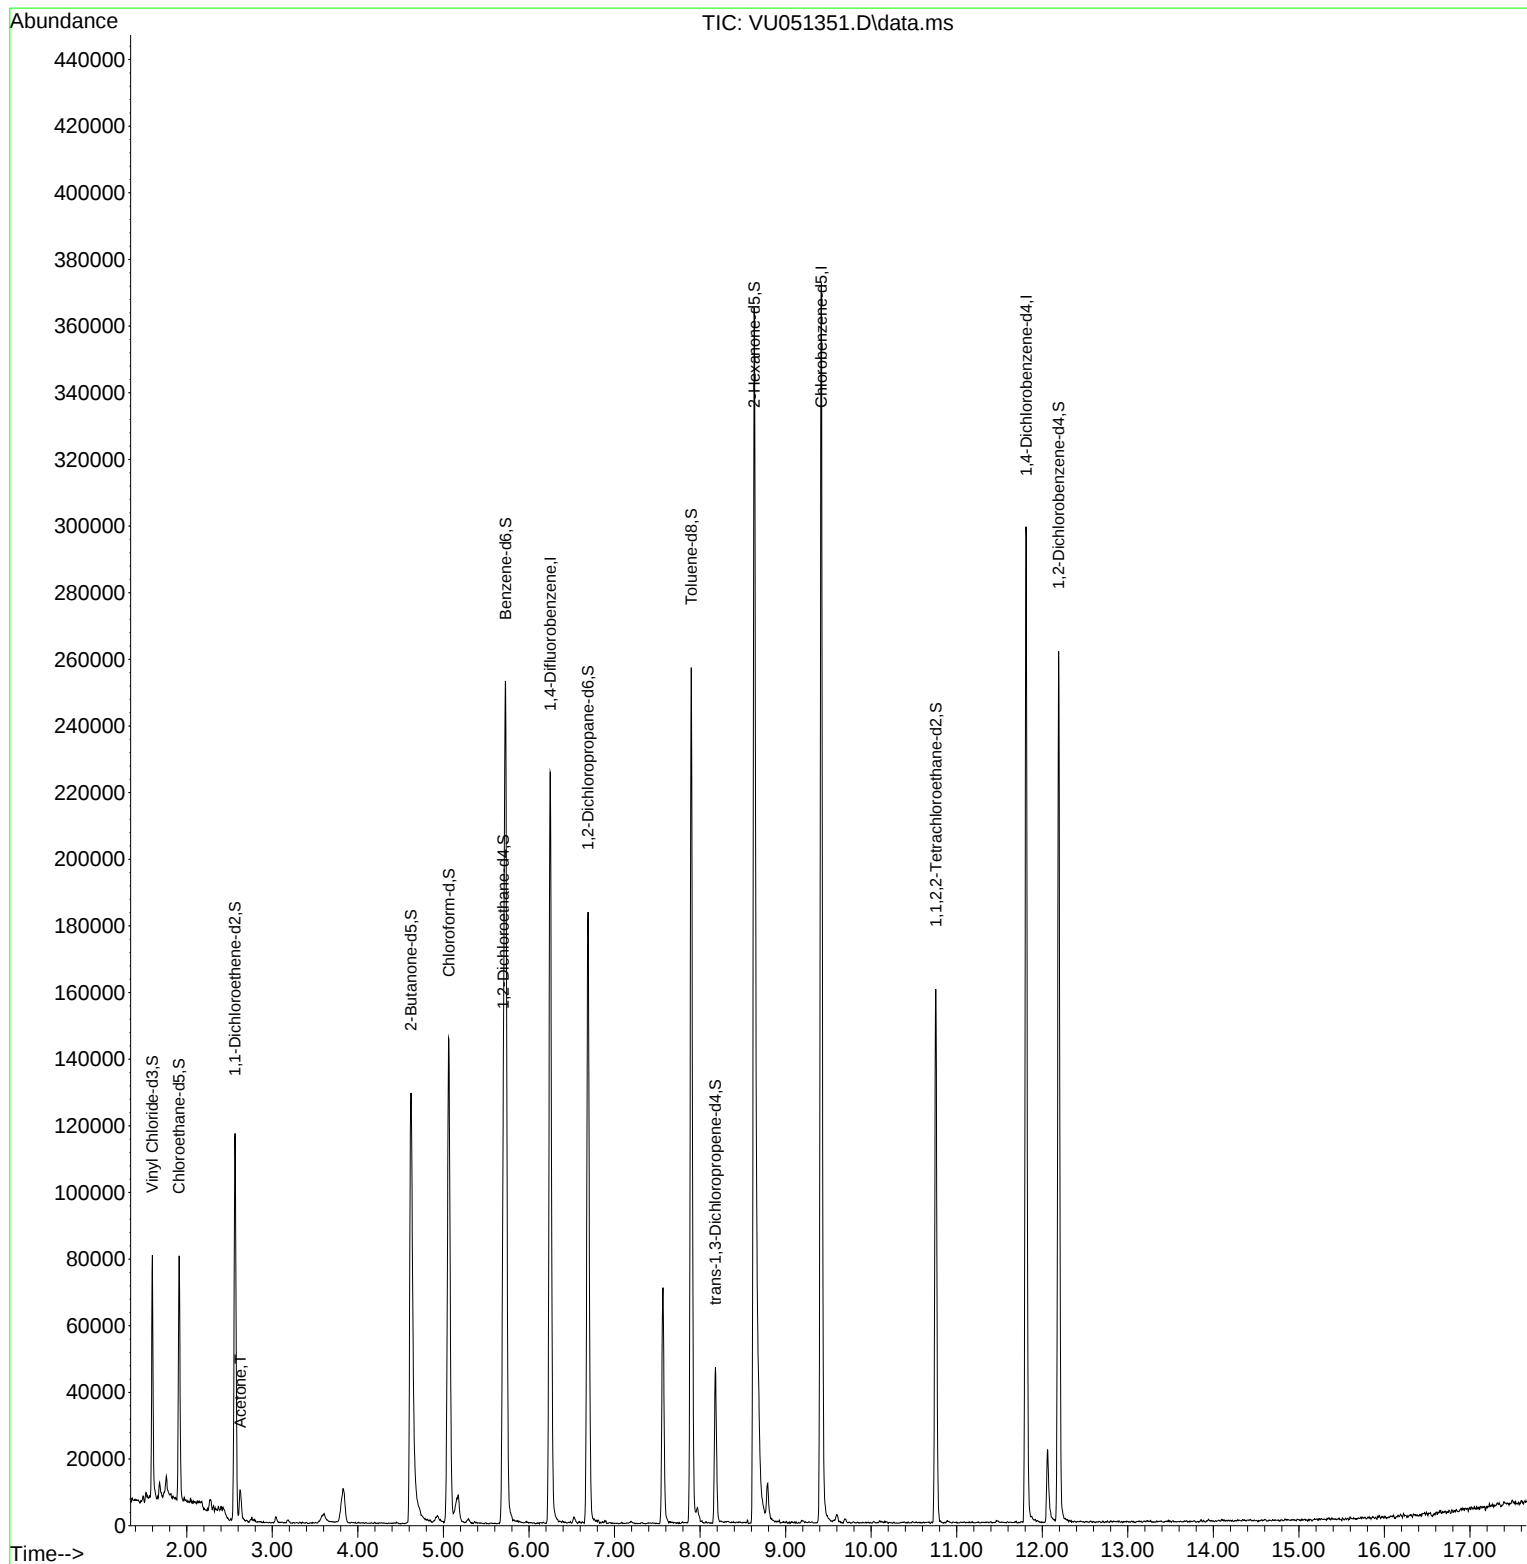

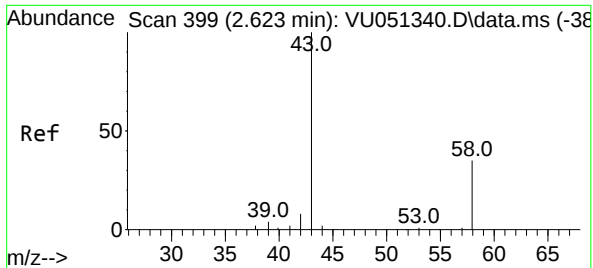

#13
 Acetone
 Concen: 4.572 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. 0.000 min
 Lab File: VU051351.D
 Acq: 11 Oct 2022 01:40

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB7

Tgt Ion: 43 Resp: 10850
 Ion Ratio Lower Upper
 43 100
 58 35.3 0.0 68.8

