

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051352.D
 Acq On : 11 Oct 2022 02:05
 Operator : JC/MD
 Sample : N5071-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB8

Quant Time: Oct 11 05:58:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	173622	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	204000	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	75921	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	49590	3.541	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.800%
7) Chloroethane-d5	1.912	69	51479	4.278	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.562	65	20982	3.790	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.800%
20) 2-Butanone-d5	4.620	46	154083	49.971	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.940%
24) Chloroform-d	5.063	84	130495	4.998	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.700	65	69942	5.194	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.726	84	222569	3.966	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.400%
36) 1,2-Dichloropropane-d6	6.690	67	84719	4.445	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.800%
41) Toluene-d8	7.896	98	162906	3.245	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.800%#
43) trans-1,3-Dichloroprop...	8.179	79	23559	3.762	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.200%
46) 2-Hexanone-d5	8.632	63	78582	37.236	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.480%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	71216	4.678	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	65571	4.969	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.400%
Target Compounds						Qvalue
13) Acetone	2.626	43	10904	4.715	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051352.D
Acq On : 11 Oct 2022 02:05
Operator : JC/MD
Sample : N5071-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB8

Quant Time: Oct 11 05:58:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

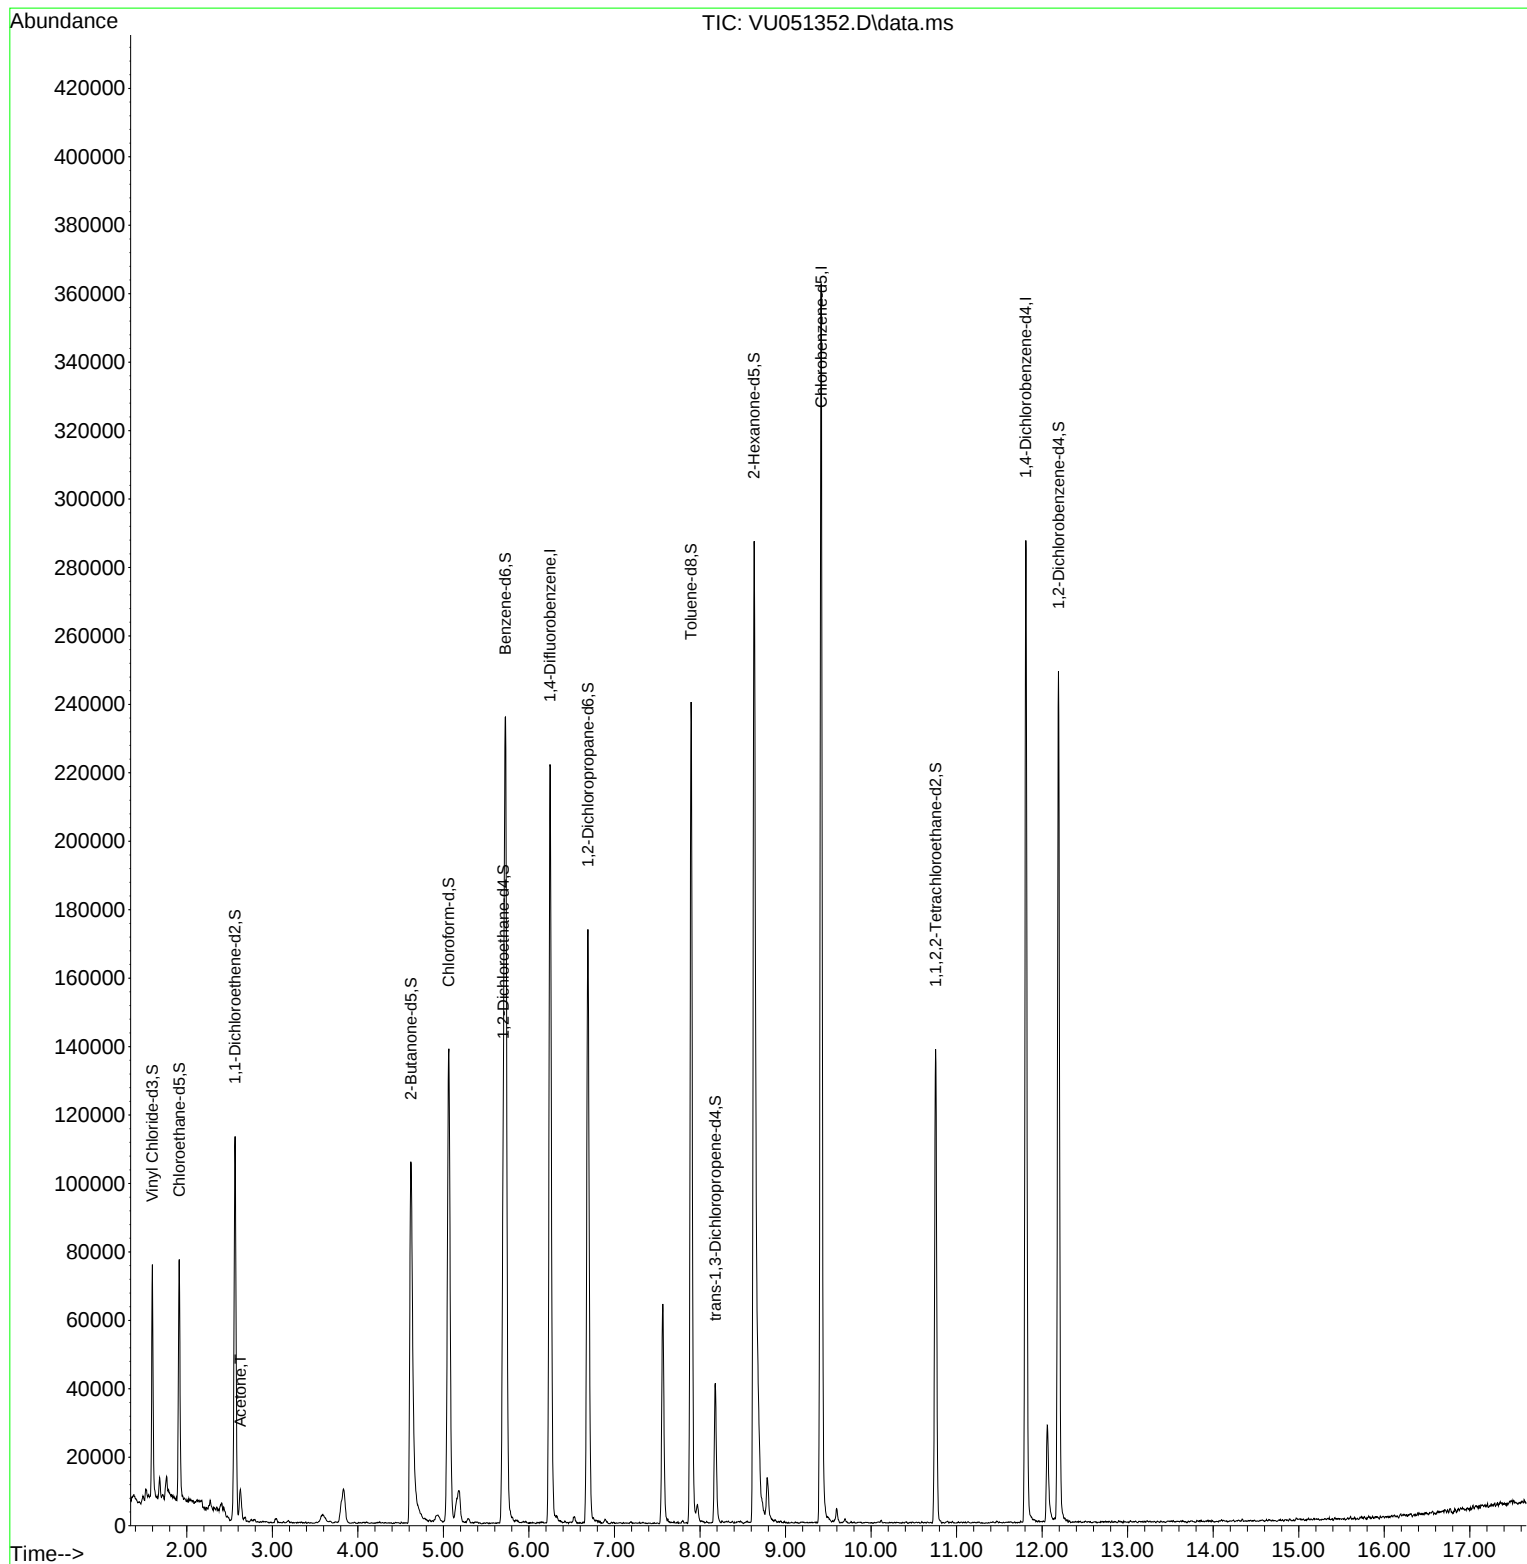

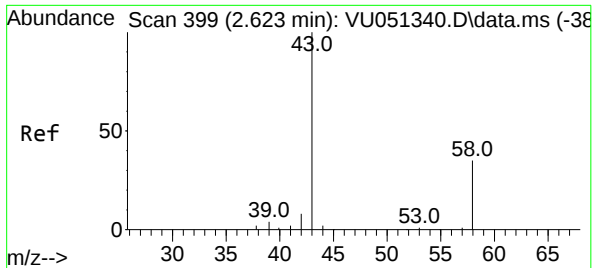

#13
 Acetone
 Concen: 4.715 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051352.D
 Acq: 11 Oct 2022 02:05

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB8

Tgt Ion:	43	Resp:	10904
Ion Ratio	Lower	Upper	
43	100		
58	32.4	0.0	68.8

