

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051356.D
 Acq On : 11 Oct 2022 03:44
 Operator : JC/MD
 Sample : N5071-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BC4

Quant Time: Oct 11 05:58:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	181561	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	212570	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	79885	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50819	3.470	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.400%
7) Chloroethane-d5	1.912	69	52973	4.210	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.200%
11) 1,1-Dichloroethene-d2	2.565	65	21998	3.800	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.000%
20) 2-Butanone-d5	4.620	46	167218	51.859	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.720%
24) Chloroform-d	5.060	84	133141	4.876	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.700	65	71817	5.100	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%
32) Benzene-d6	5.726	84	228887	3.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%
36) 1,2-Dichloropropane-d6	6.690	67	87548	4.408	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.896	98	167965	3.210	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.200%#
43) trans-1,3-Dichloroprop...	8.179	79	24285	3.722	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.632	63	88293	40.150	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.300%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	73983	4.663	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	65344	4.706	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.200%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	10544	4.360	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051356.D
Acq On : 11 Oct 2022 03:44
Operator : JC/MD
Sample : N5071-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BC4

Quant Time: Oct 11 05:58:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

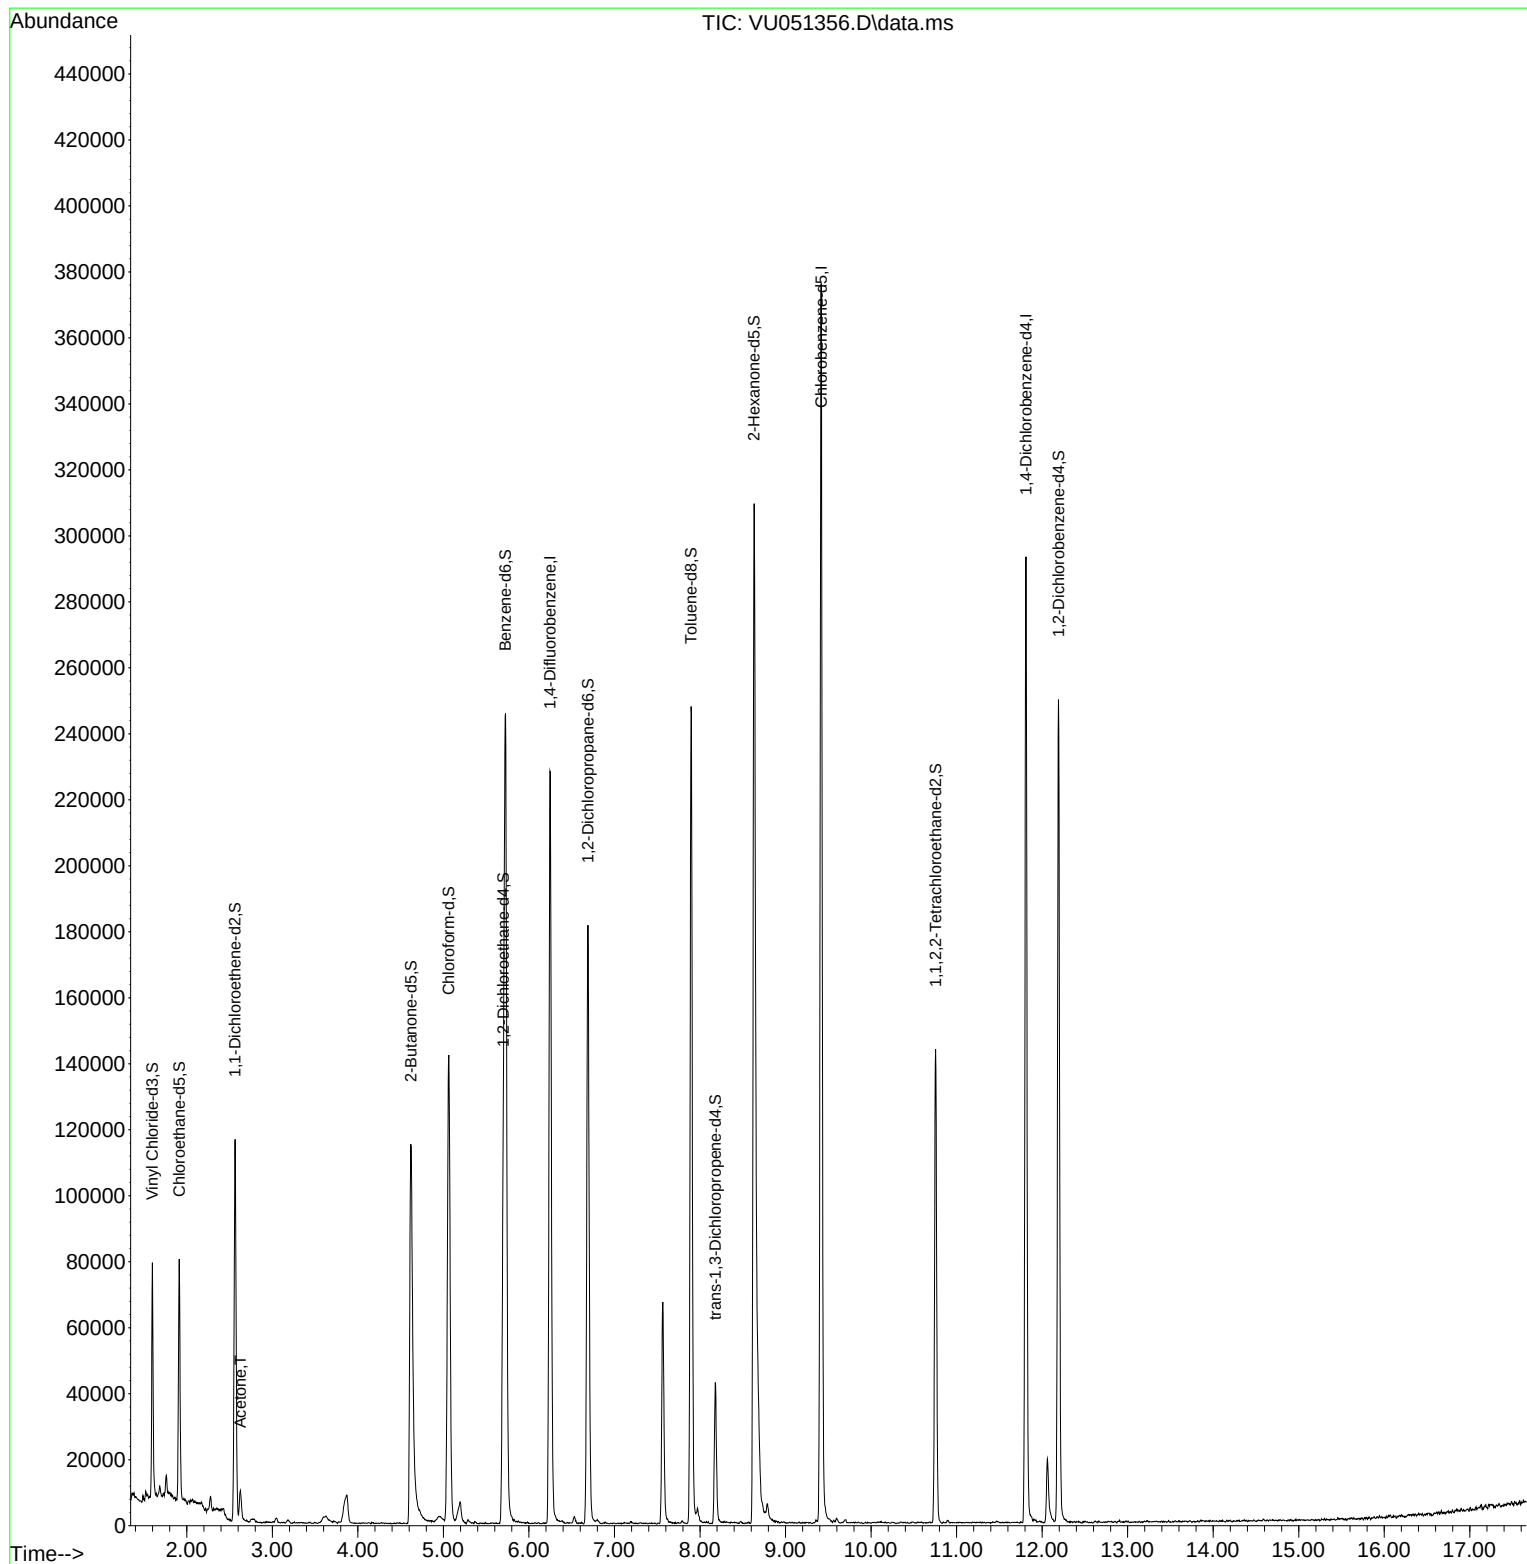

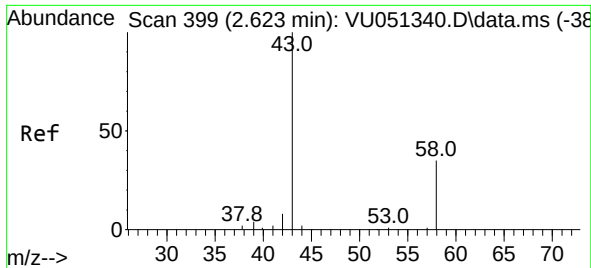

#13
 Acetone
 Concen: 4.360 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051356.D
 Acq: 11 Oct 2022 03:44

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BC4

Tgt Ion: 43 Resp: 10544
 Ion Ratio Lower Upper
 43 100
 58 35.0 0.0 68.8

