

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051357.D
 Acq On : 11 Oct 2022 04:09
 Operator : JC/MD
 Sample : N5071-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BC6

Quant Time: Oct 11 05:59:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	183621	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	212431	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	79504	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	52126	3.519	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.400%
7) Chloroethane-d5	1.913	69	54946	4.317	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.400%
11) 1,1-Dichloroethene-d2	2.565	65	22021	3.761	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.200%
20) 2-Butanone-d5	4.620	46	170160	52.180	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.360%
24) Chloroform-d	5.060	84	137214	4.969	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.700	65	73280	5.146	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
32) Benzene-d6	5.726	84	233965	4.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.000%
36) 1,2-Dichloropropane-d6	6.690	67	88208	4.444	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.800%
41) Toluene-d8	7.896	98	174980	3.347	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.000%#
43) trans-1,3-Dichloroprop...	8.179	79	25264	3.875	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.400%
46) 2-Hexanone-d5	8.633	63	85743	39.016	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.040%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	78332	4.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	66415	4.806	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds						Qvalue
13) Acetone	2.626	43	8917	3.646	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051357.D
Acq On : 11 Oct 2022 04:09
Operator : JC/MD
Sample : N5071-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BC6

Quant Time: Oct 11 05:59:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

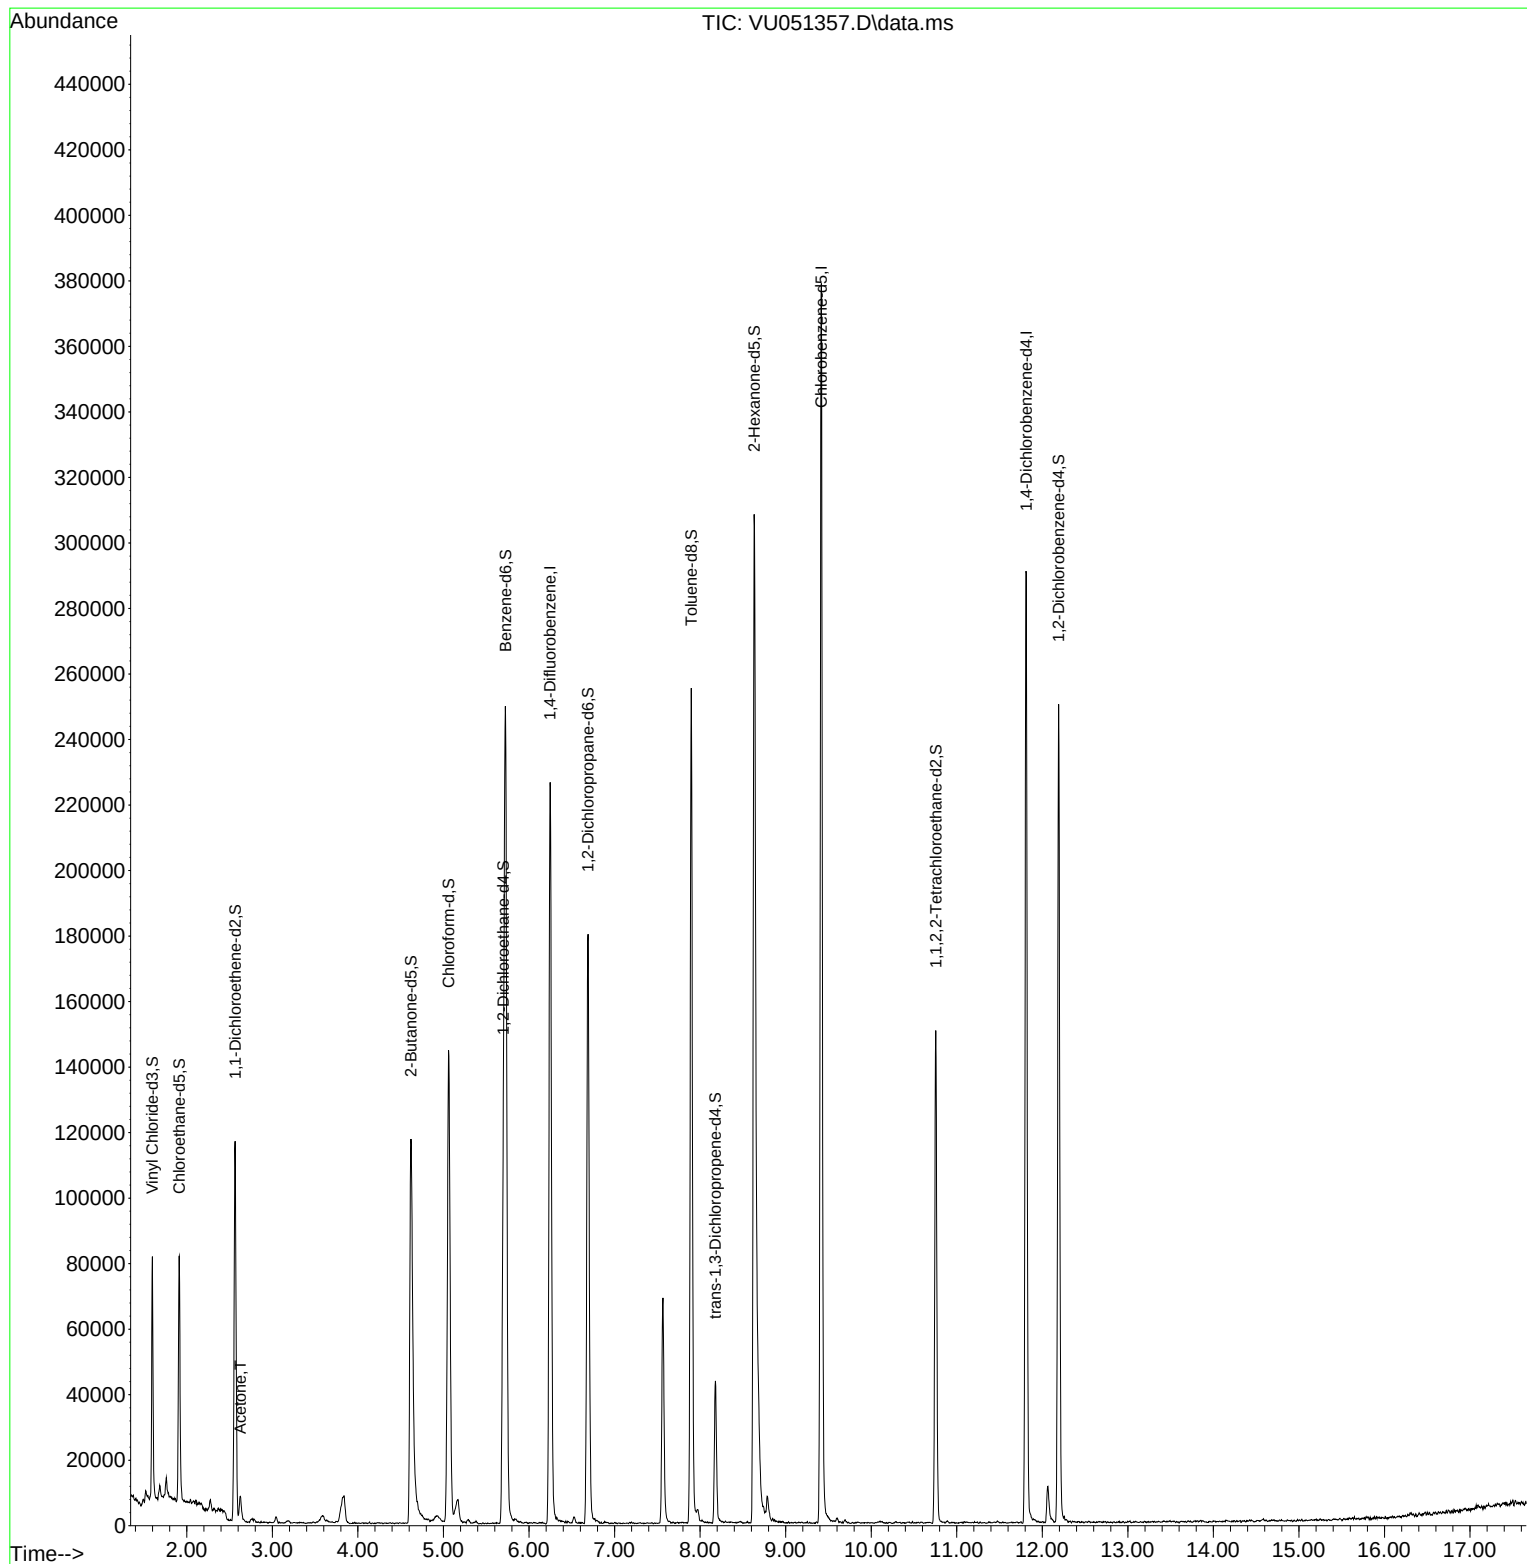

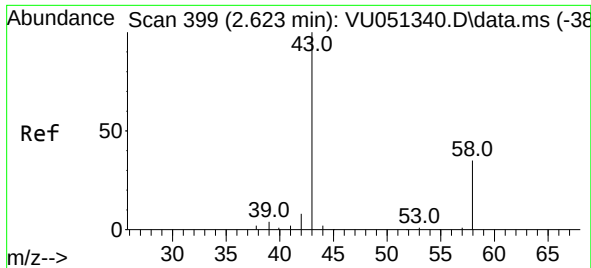

#13
 Acetone
 Concen: 3.646 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051357.D
 Acq: 11 Oct 2022 04:09

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BC6

Tgt Ion: 43 Resp: 8917
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 68.8

