

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051361.D
 Acq On : 11 Oct 2022 05:47
 Operator : JC/MD
 Sample : N5071-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD1

Quant Time: Oct 11 08:17:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	160433	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	188296	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	69426	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50653	3.914	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.912	69	54101	4.865	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.400%
11) 1,1-Dichloroethene-d2	2.565	65	21215	4.147	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.000%
20) 2-Butanone-d5	4.620	46	170022	59.673	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.340%
24) Chloroform-d	5.060	84	134311	5.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.400%
26) 1,2-Dichloroethane-d4	5.700	65	74968	6.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.600%
32) Benzene-d6	5.726	84	229673	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
36) 1,2-Dichloropropane-d6	6.690	67	86853	4.937	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.800%
41) Toluene-d8	7.896	98	169512	3.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%
43) trans-1,3-Dichloroprop...	8.182	79	24449	4.230	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.632	63	87041	44.684	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.360%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	77900	5.543	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	66972	5.550	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.000%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	9420	4.408	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051361.D
Acq On : 11 Oct 2022 05:47
Operator : JC/MD
Sample : N5071-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BD1

Quant Time: Oct 11 08:17:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

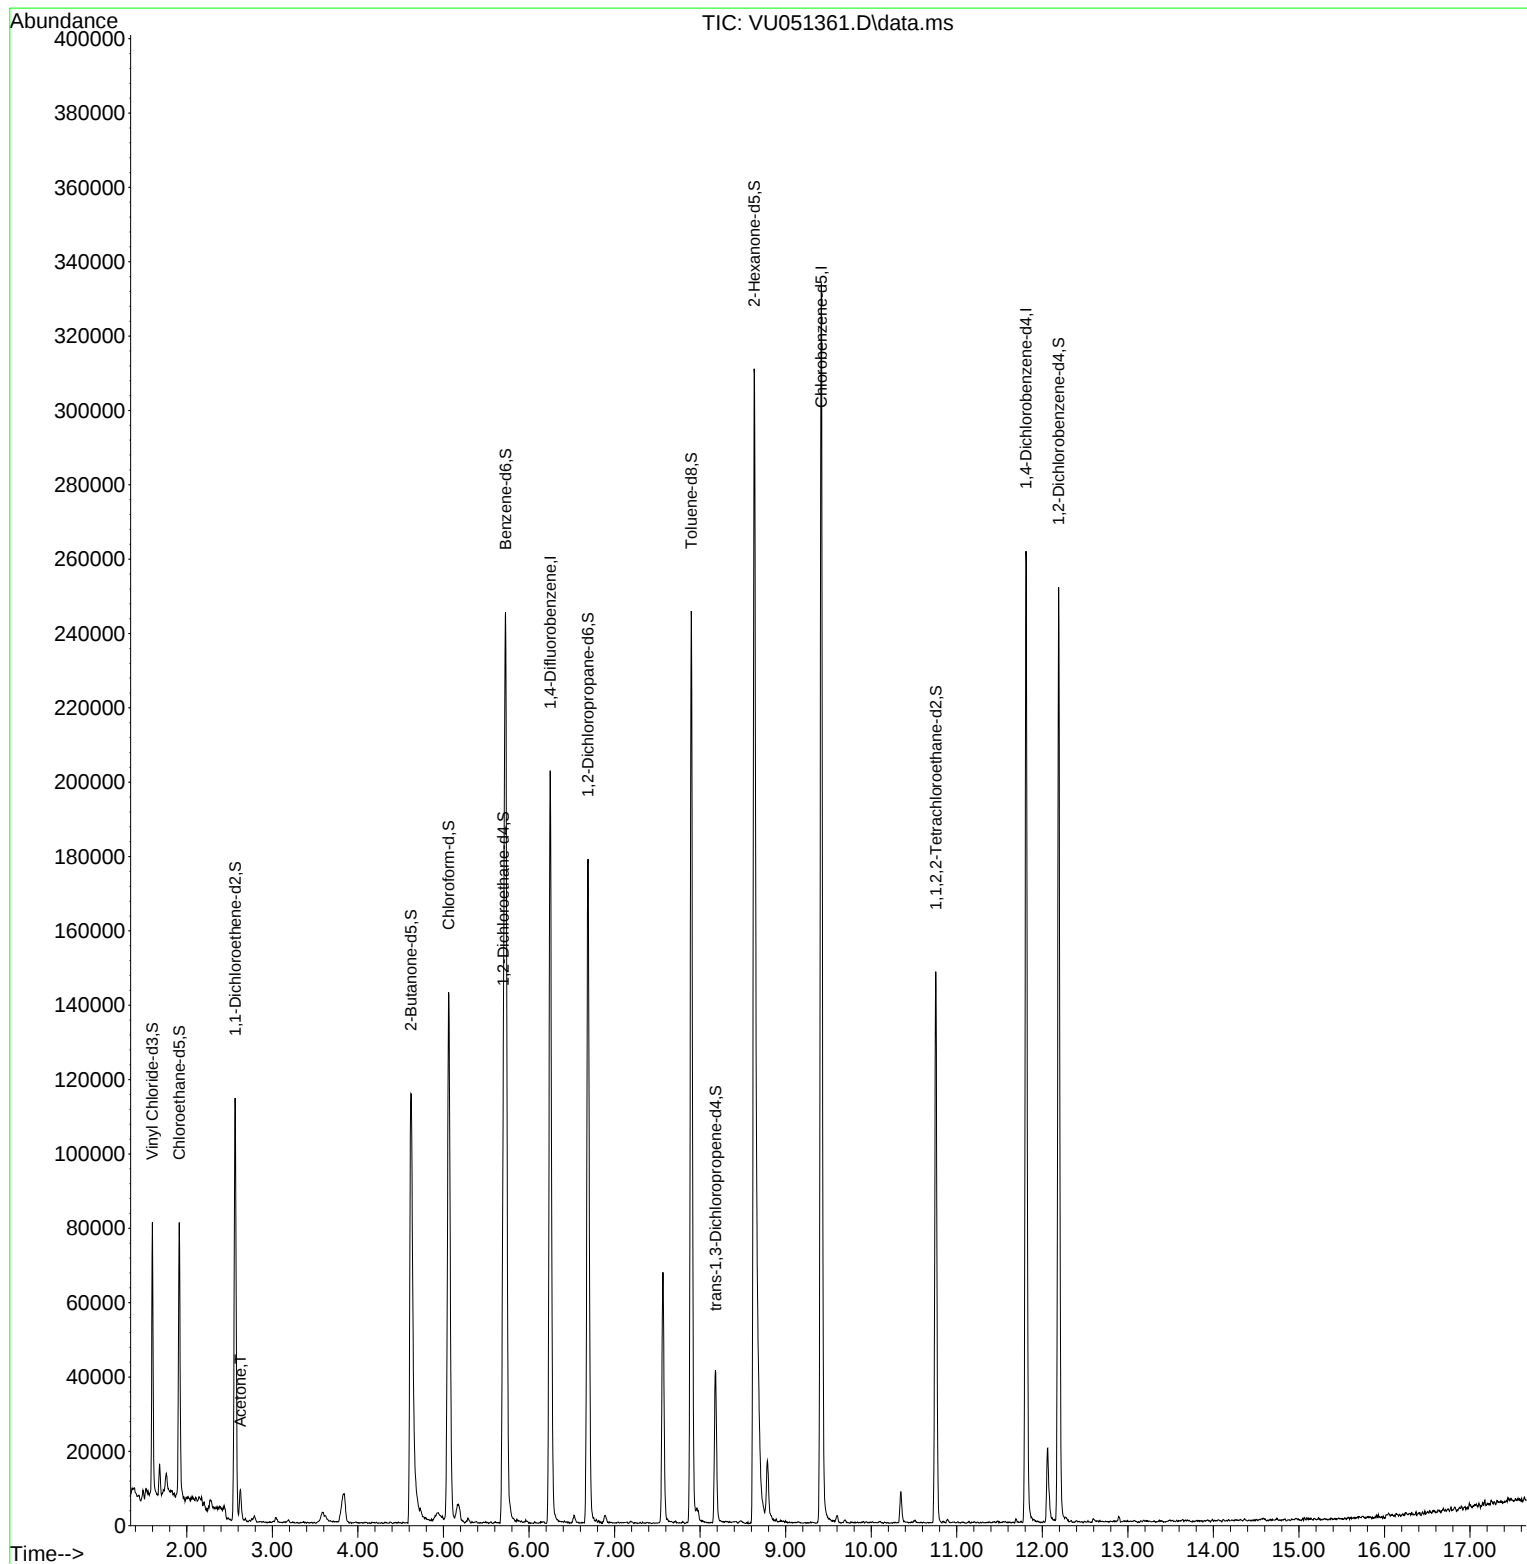

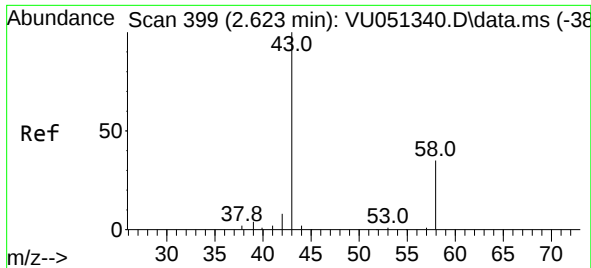

#13
 Acetone
 Concen: 4.408 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051361.D
 Acq: 11 Oct 2022 05:47

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD1

Tgt Ion: 43 Resp: 9420
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 68.8

