

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051362.D
 Acq On : 11 Oct 2022 06:12
 Operator : JC/MD
 Sample : N5071-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD2

Quant Time: Oct 11 08:18:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	170653	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	193126	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	73428	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51675	3.754	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.912	69	53383	4.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.565	65	21755	3.998	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.000%
20) 2-Butanone-d5	4.620	46	158517	52.303	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.600%
24) Chloroform-d	5.063	84	134714	5.249	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
26) 1,2-Dichloroethane-d4	5.700	65	71182	5.378	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.600%
32) Benzene-d6	5.726	84	226040	4.255	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
36) 1,2-Dichloropropane-d6	6.690	67	86752	4.808	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.896	98	170055	3.578	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	8.182	79	24002	4.049	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%
46) 2-Hexanone-d5	8.632	63	82213	41.150	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.300%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	75975	5.271	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	65141	5.104	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						
					Qvalue	
13) Acetone	2.623	43	11249	4.949	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051362.D
Acq On : 11 Oct 2022 06:12
Operator : JC/MD
Sample : N5071-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BD2

Quant Time: Oct 11 08:18:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

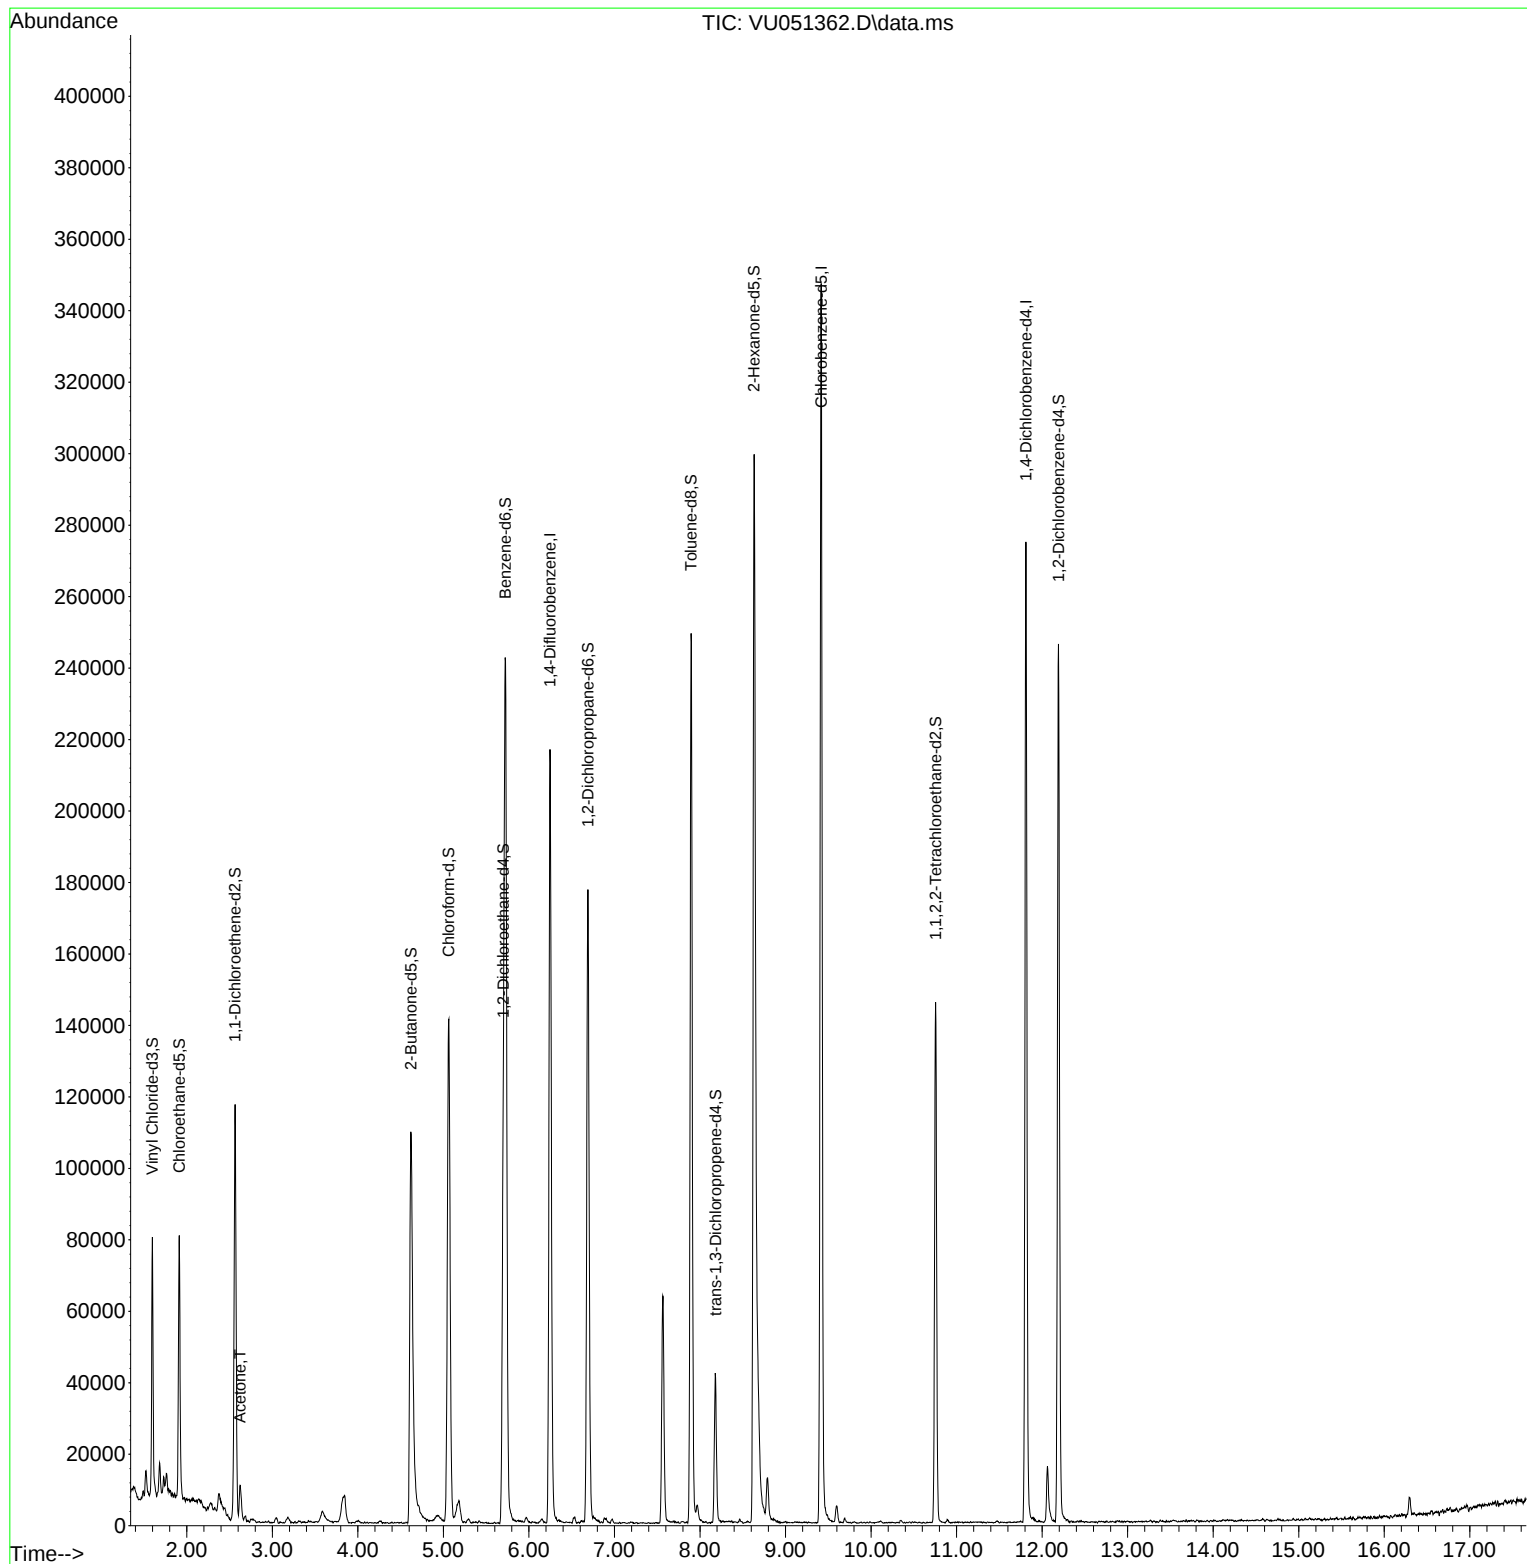

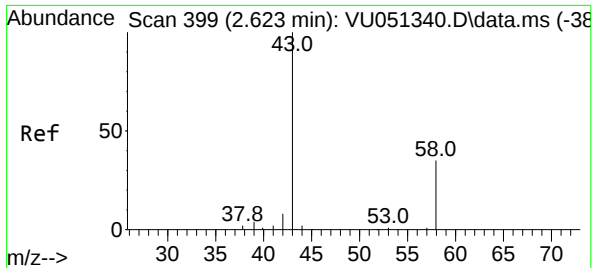

#13
 Acetone
 Concen: 4.949 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. 0.000 min
 Lab File: VU051362.D
 Acq: 11 Oct 2022 06:12

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD2

Tgt Ion: 43 Resp: 11249
 Ion Ratio Lower Upper
 43 100
 58 36.7 0.0 68.8

