

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051363.D
 Acq On : 11 Oct 2022 06:37
 Operator : JC/MD
 Sample : N5071-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD3

Quant Time: Oct 11 08:18:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 11 02:38:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	163462	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	184824	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	70051	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	48659	3.690	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.800%
7) Chloroethane-d5	1.912	69	51395	4.536	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	2.565	65	21104	4.049	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.000%
20) 2-Butanone-d5	4.620	46	156782	54.006	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.020%
24) Chloroform-d	5.060	84	128241	5.217	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.400%
26) 1,2-Dichloroethane-d4	5.700	65	70436	5.556	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.200%
32) Benzene-d6	5.726	84	217148	4.271	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
36) 1,2-Dichloropropane-d6	6.690	67	81452	4.717	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.896	98	160562	3.530	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.600%
43) trans-1,3-Dichloroprop...	8.179	79	23398	4.124	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.632	63	77370	40.465	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.940%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	72190	5.234	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	62343	5.120	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	11650	5.351	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051363.D
Acq On : 11 Oct 2022 06:37
Operator : JC/MD
Sample : N5071-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BD3

Quant Time: Oct 11 08:18:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 11 02:38:56 2022
Response via : Initial Calibration

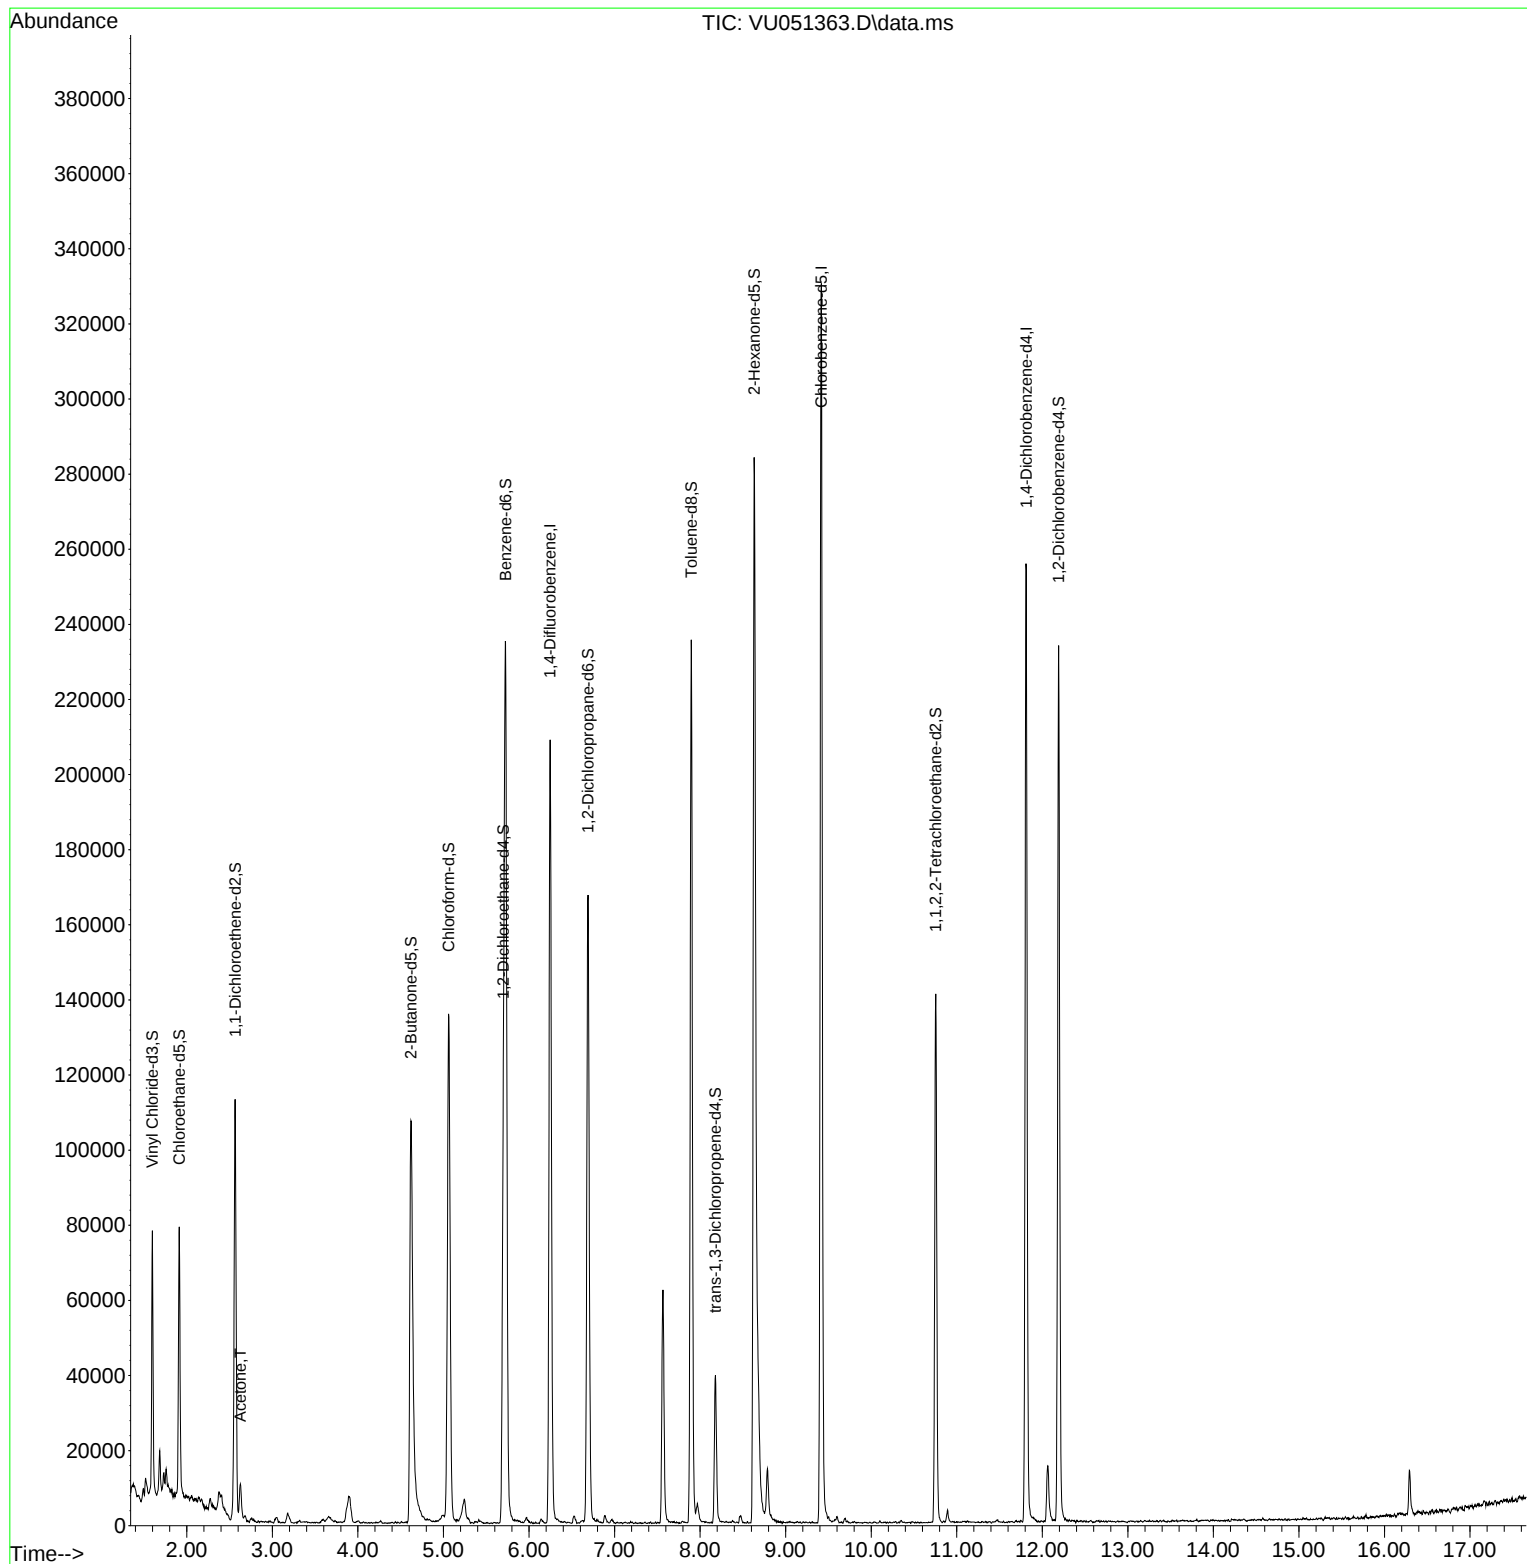

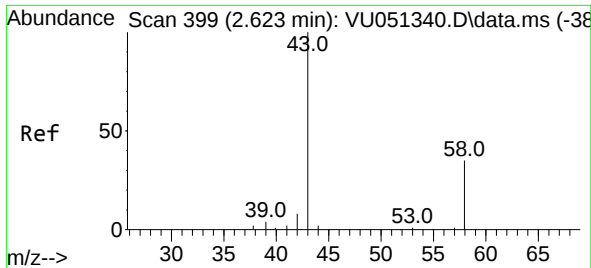

#13
 Acetone
 Concen: 5.351 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051363.D
 Acq: 11 Oct 2022 06:37

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BD3

Tgt Ion: 43 Resp: 11650
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 68.8

