

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051316.D
 Acq On : 10 Oct 2022 10:35
 Operator : JC/MD
 Sample : VU1010WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK110

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	92	rBV	95354	109014	13.92%	1.766%
2	1.912	170	178	195	rVB	91432	118467	15.13%	1.919%
3	2.565	366	381	402	rVB	148853	242243	30.94%	3.924%
4	3.044	520	530	545	rVB2	9853	17479	2.23%	0.283%
5	3.825	755	773	787	rBV	5474	16192	2.07%	0.262%
6	4.639	1010	1026	1069	rBV	99749	335707	42.87%	5.438%
7	5.063	1142	1158	1177	rBV	156984	345710	44.15%	5.600%
8	5.173	1178	1192	1206	rVB	5743	17959	2.29%	0.291%
9	5.723	1342	1363	1386	rBV2	279470	747345	95.45%	12.106%
10	6.247	1513	1526	1547	rBV	238186	458643	58.57%	7.430%
11	6.690	1647	1664	1687	rBV	193361	382199	48.81%	6.191%
12	7.565	1922	1936	1960	rBV2	78515	143601	18.34%	2.326%
13	7.896	2025	2039	2057	rBV	293803	519210	66.31%	8.411%
14	7.967	2057	2061	2074	rVB3	5027	8135	1.04%	0.132%
15	8.179	2115	2127	2144	rBV	50821	88373	11.29%	1.432%
16	8.636	2256	2269	2303	rBV3	342432	783004	100.00%	12.684%
17	9.417	2498	2512	2538	rBV	377378	636450	81.28%	10.310%
18	10.754	2913	2928	2941	rBV	152387	249005	31.80%	4.034%
19	11.812	3245	3257	3280	rBV	306172	500585	63.93%	8.109%
20	12.192	3363	3375	3398	rBV	276326	453891	57.97%	7.353%




Sum of corrected areas: 6173212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051316.D
Acq On : 10 Oct 2022 10:35
Operator : JC/MD
Sample : VU1010WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

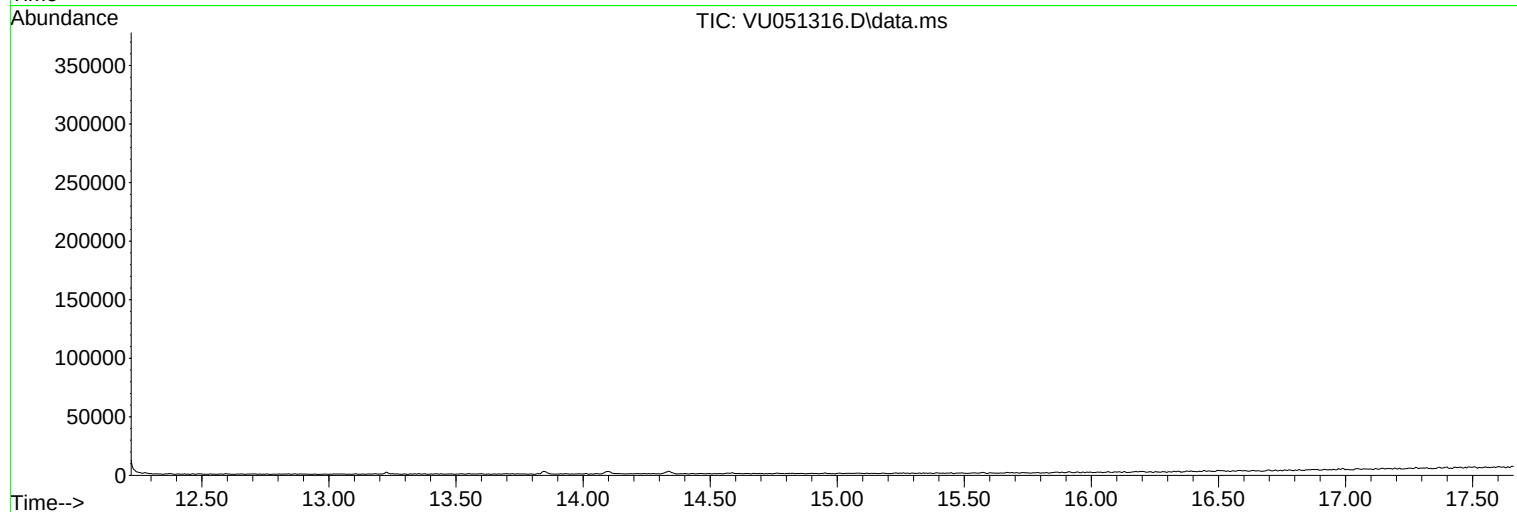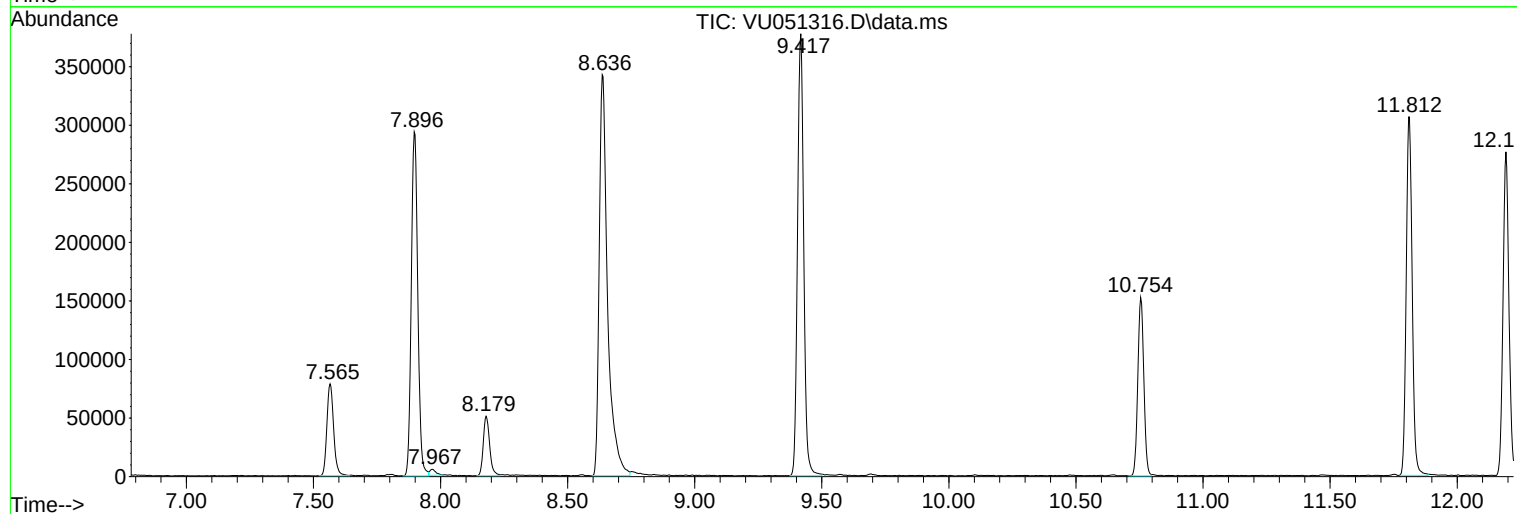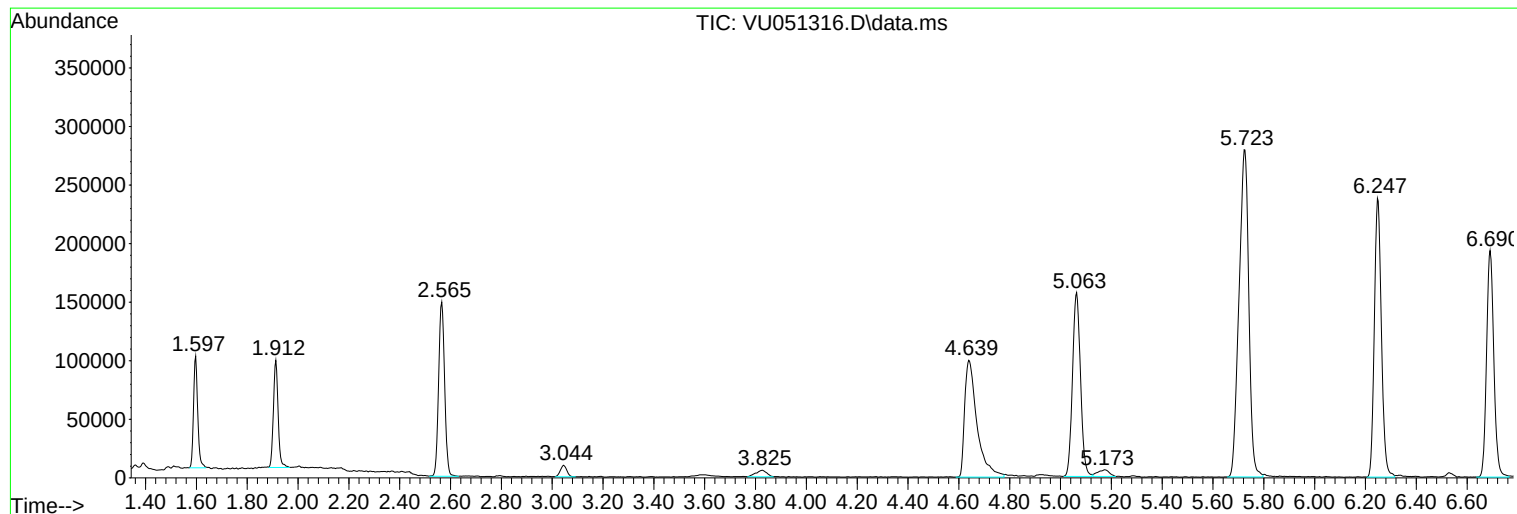

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051316.D
Acq On : 10 Oct 2022 10:35
Operator : JC/MD
Sample : VU1010WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051316.D
Acq On : 10 Oct 2022 10:35
Operator : JC/MD
Sample : VU1010WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc