

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051319.D
 Acq On : 10 Oct 2022 11:57
 Operator : JC/MD
 Sample : N4922-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.388	11	15	26	rVB3	5761	7888	1.03%	0.128%
2	1.594	72	79	93	rBV	89642	107003	14.00%	1.740%
3	1.912	170	178	190	rBV	83826	108791	14.23%	1.769%
4	2.565	368	381	401	rBV	142257	229135	29.97%	3.726%
5	3.044	517	530	545	rVB2	16326	31264	4.09%	0.508%
6	3.835	756	776	777	rBV	7903	16151	2.11%	0.263%
7	4.636	1012	1025	1060	rBV	108792	332509	43.49%	5.407%
8	5.060	1140	1157	1177	rBV	151937	340552	44.54%	5.537%
9	5.722	1343	1363	1392	rBV2	280467	734702	96.09%	11.946%
10	6.247	1508	1526	1549	rBV	252326	487302	63.74%	7.923%
11	6.690	1648	1664	1683	rBV2	190393	375866	49.16%	6.111%
12	7.565	1923	1936	1952	rBV	77743	138955	18.17%	2.259%
13	7.896	2026	2039	2057	rBV	290497	506029	66.18%	8.228%
14	8.179	2112	2127	2146	rBV	50391	88507	11.58%	1.439%
15	8.475	2208	2219	2229	rBV3	5227	9426	1.23%	0.153%
16	8.636	2256	2269	2304	rBV2	341165	764574	100.00%	12.432%
17	9.417	2495	2512	2534	rBV	392921	657666	86.02%	10.693%
18	10.754	2915	2928	2944	rBV	151324	243251	31.82%	3.955%
19	10.889	2960	2970	2981	rVB3	8495	14103	1.84%	0.229%
20	11.809	3244	3256	3278	rBV	311086	511475	66.90%	8.316%
21	12.192	3363	3375	3399	rBV	265589	445017	58.20%	7.236%




Sum of corrected areas: 6150166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051319.D
Acq On : 10 Oct 2022 11:57
Operator : JC/MD
Sample : N4922-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

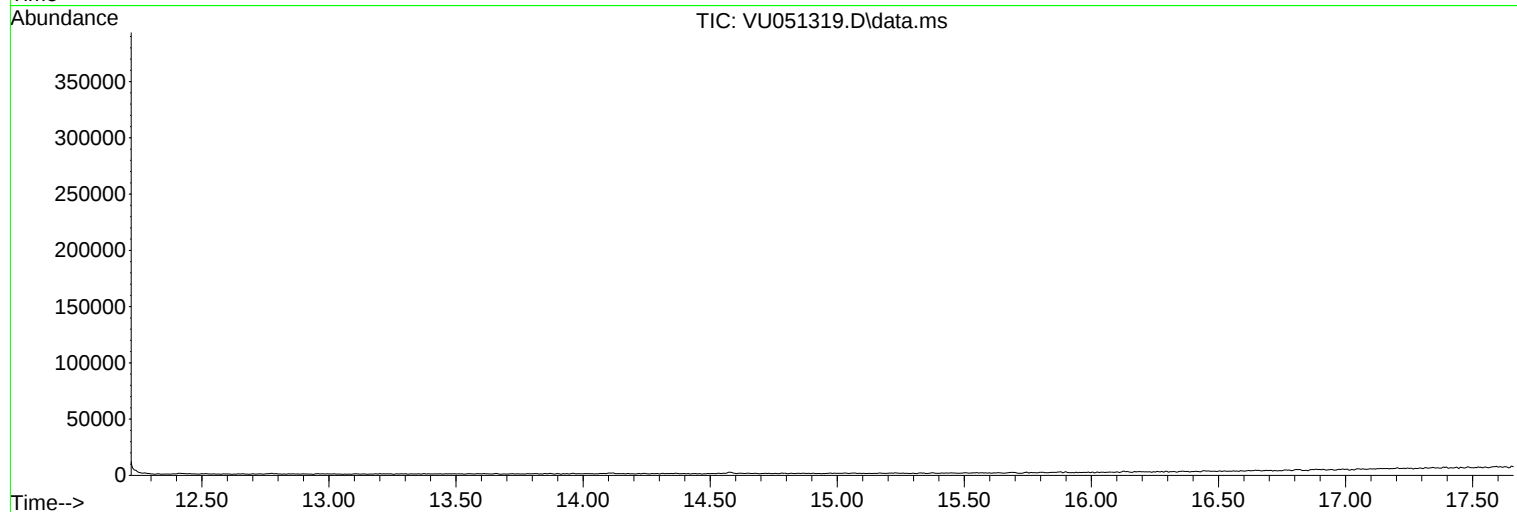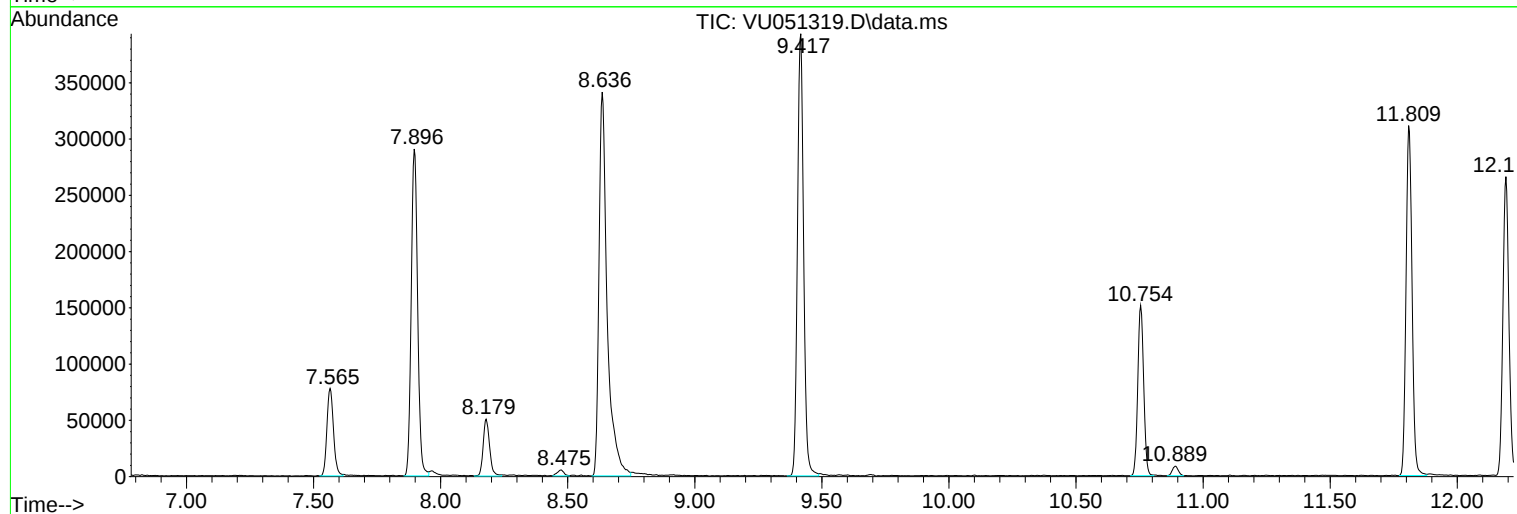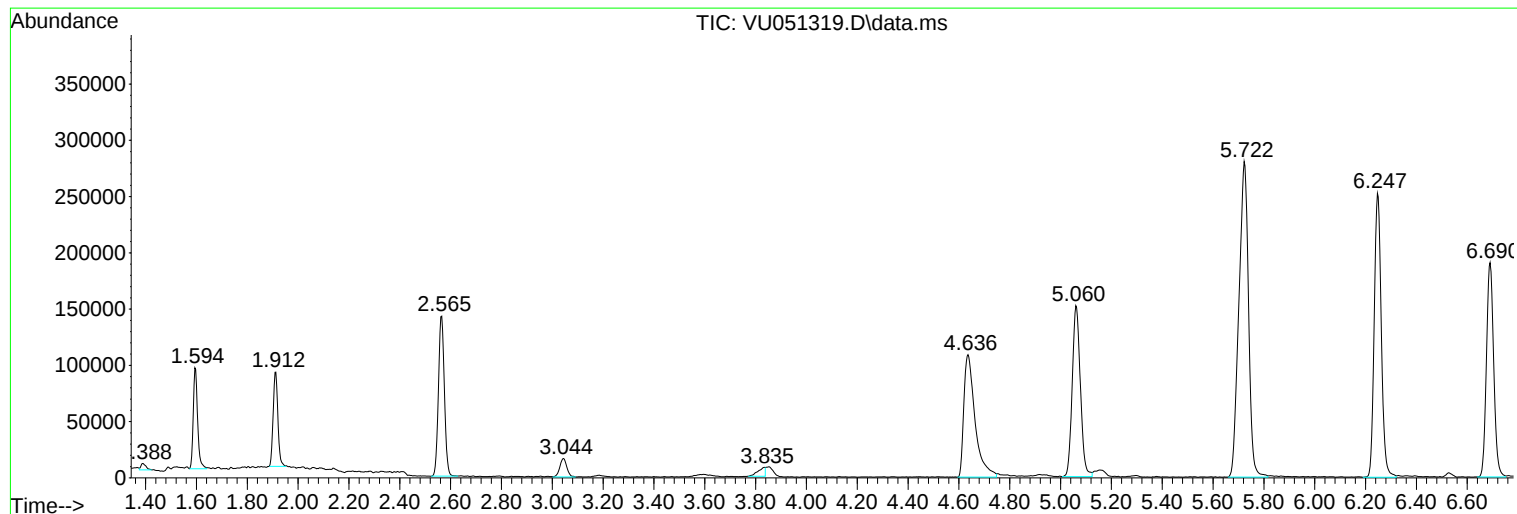

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051319.D
Acq On : 10 Oct 2022 11:57
Operator : JC/MD
Sample : N4922-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051319.D
Acq On : 10 Oct 2022 11:57
Operator : JC/MD
Sample : N4922-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc