

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051331.D
 Acq On : 10 Oct 2022 16:52
 Operator : JC/MD
 Sample : N5041-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	92	rBV	70897	84259	3.70%	1.064%
2	1.912	170	178	193	rVB	70316	93902	4.12%	1.186%
3	2.565	369	381	395	rBV	115556	188170	8.26%	2.376%
4	3.359	616	628	646	rVB3	13914	31591	1.39%	0.399%
5	3.841	755	778	802	rVB	10382	39206	1.72%	0.495%
6	4.665	1009	1034	1075	rBV2	874693	2279294	100.00%	28.785%
7	5.063	1142	1158	1176	rBV	142109	312934	13.73%	3.952%
8	5.722	1343	1363	1399	rBV2	257227	686234	30.11%	8.666%
9	6.247	1513	1526	1543	rBV	224964	431374	18.93%	5.448%
10	6.542	1604	1618	1634	rBV2	101559	194868	8.55%	2.461%
11	6.690	1649	1664	1686	rBV	177734	350113	15.36%	4.422%
12	7.565	1924	1936	1956	rBV2	73367	130795	5.74%	1.652%
13	7.896	2026	2039	2055	rBV	259006	452214	19.84%	5.711%
14	8.176	2112	2126	2153	rBV4	51043	99982	4.39%	1.263%
15	8.401	2185	2196	2209	rVB3	21374	36974	1.62%	0.467%
16	8.632	2256	2268	2302	rBV2	361870	793258	34.80%	10.018%
17	9.417	2498	2512	2540	rBV	351868	590932	25.93%	7.463%
18	10.754	2916	2928	2953	rVB	151787	243066	10.66%	3.070%
19	11.812	3244	3257	3276	rBV	278471	461352	20.24%	5.826%
20	12.192	3359	3375	3395	rBV	251444	417854	18.33%	5.277%




Sum of corrected areas: 7918372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051331.D
Acq On : 10 Oct 2022 16:52
Operator : JC/MD
Sample : N5041-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

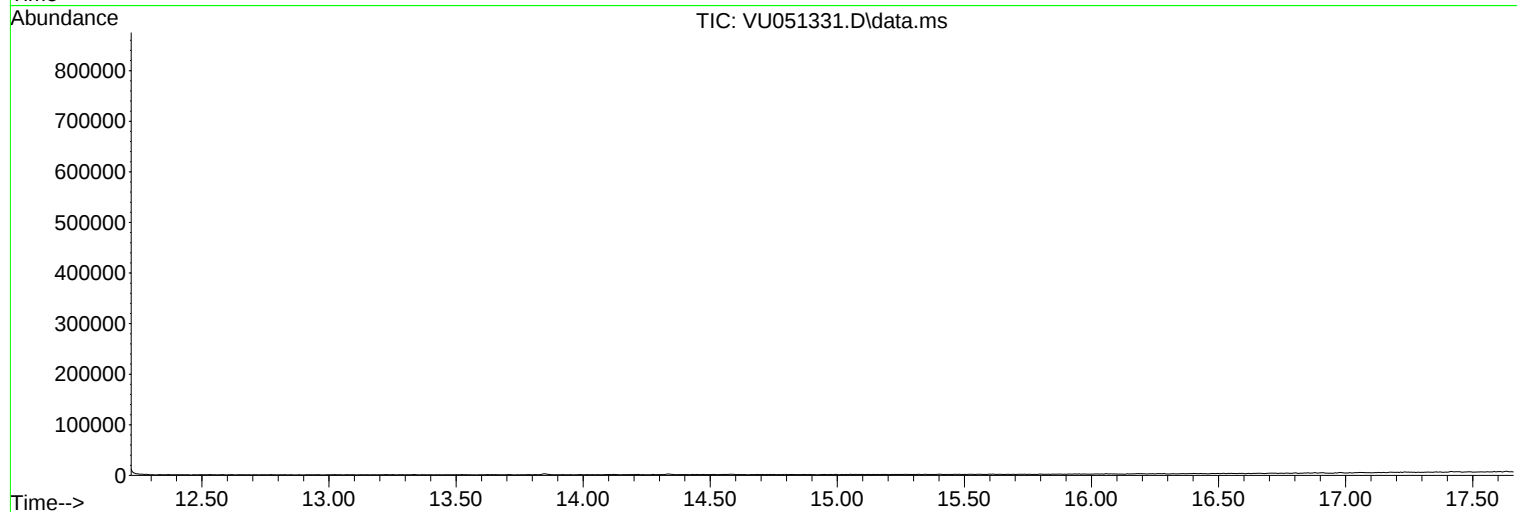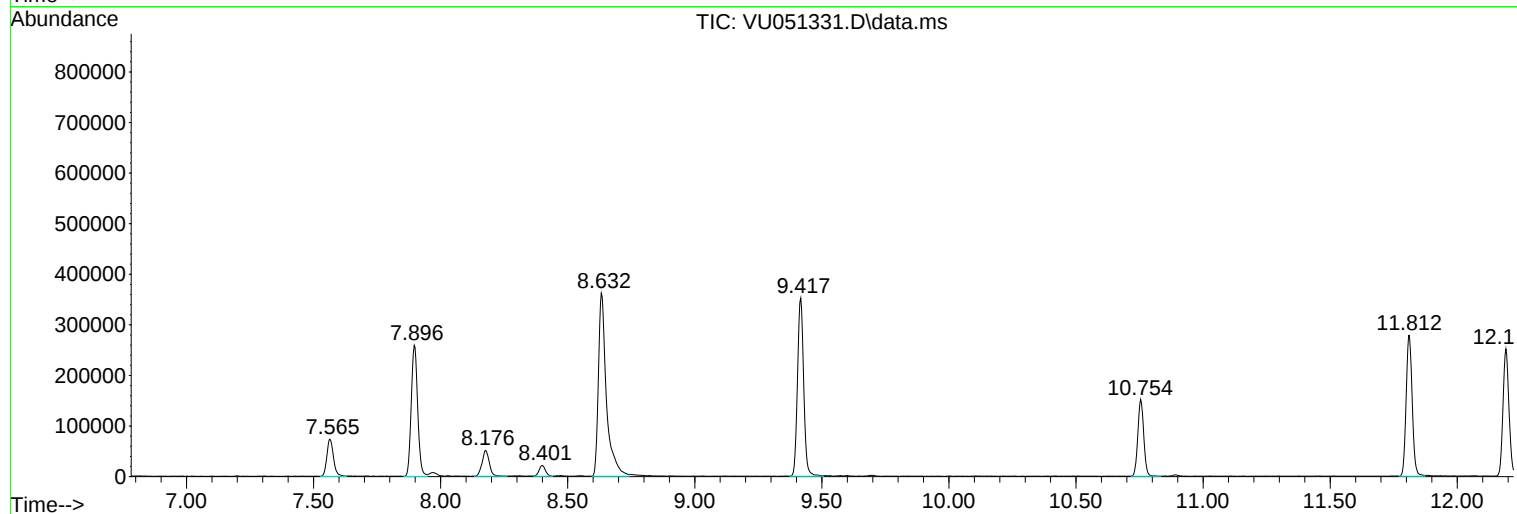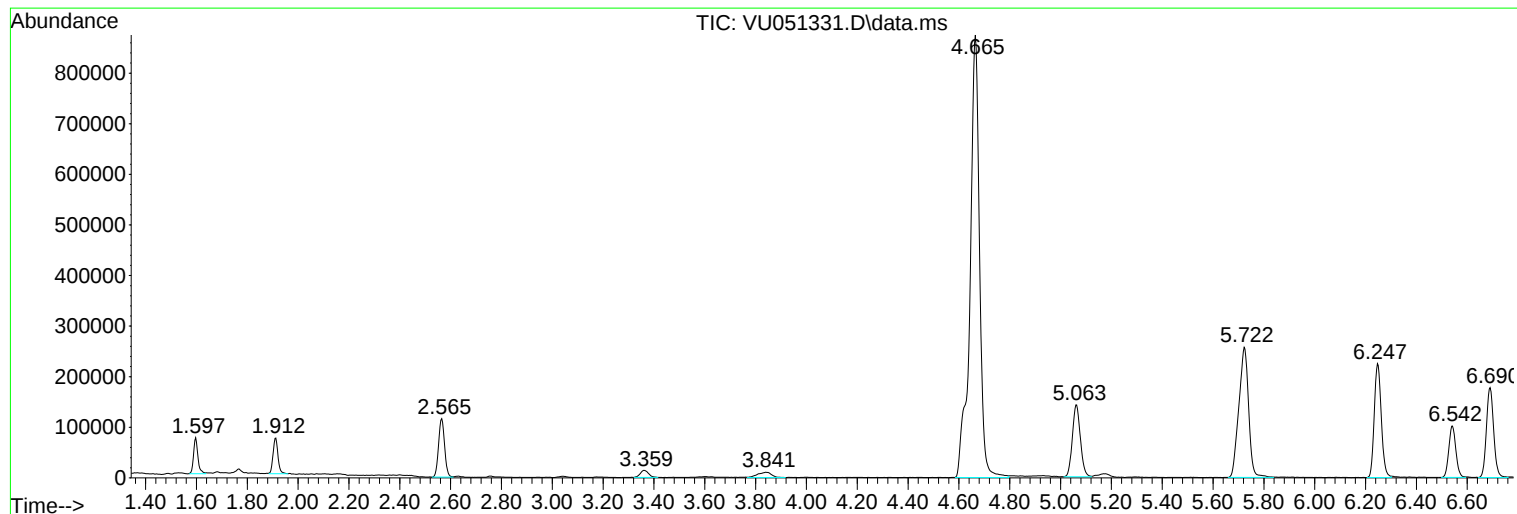

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051331.D
Acq On : 10 Oct 2022 16:52
Operator : JC/MD
Sample : N5041-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051331.D
Acq On : 10 Oct 2022 16:52
Operator : JC/MD
Sample : N5041-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc