

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051332.D
 Acq On : 10 Oct 2022 17:17
 Operator : JC/MD
 Sample : N5041-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	70128	79717	9.88%	1.400%
2	1.687	102	108	124	rVB2	5773	9349	1.16%	0.164%
3	1.912	169	178	189	rBV	72732	96222	11.92%	1.690%
4	2.565	369	381	398	rVB	115576	186722	23.13%	3.280%
5	3.842	755	778	798	rVB	7236	27390	3.39%	0.481%
6	4.636	1012	1025	1065	rBV	108039	352476	43.67%	6.192%
7	5.060	1140	1157	1176	rBV	139844	305636	37.87%	5.369%
8	5.726	1342	1364	1386	rBV2	249463	656000	81.27%	11.523%
9	6.250	1512	1527	1550	rBV	221602	432098	53.53%	7.590%
10	6.539	1605	1617	1631	rBV7	10394	22258	2.76%	0.391%
11	6.690	1650	1664	1692	rBV	176896	346746	42.96%	6.091%
12	7.565	1923	1936	1951	rBV2	71469	127074	15.74%	2.232%
13	7.896	2027	2039	2055	rBV	251112	435025	53.90%	7.642%
14	7.970	2055	2062	2075	rVB2	6837	12143	1.50%	0.213%
15	8.179	2117	2127	2141	rBV	44461	77374	9.59%	1.359%
16	8.636	2256	2269	2308	rBV3	353665	807140	100.00%	14.178%
17	9.417	2500	2512	2534	rBV	361540	605857	75.06%	10.642%
18	10.754	2915	2928	2942	rBV	145879	235823	29.22%	4.142%
19	11.812	3243	3257	3283	rBV	285193	468984	58.10%	8.238%
20	12.192	3362	3375	3396	rBV	247944	408782	50.65%	7.181%




Sum of corrected areas: 5692816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051332.D
Acq On : 10 Oct 2022 17:17
Operator : JC/MD
Sample : N5041-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

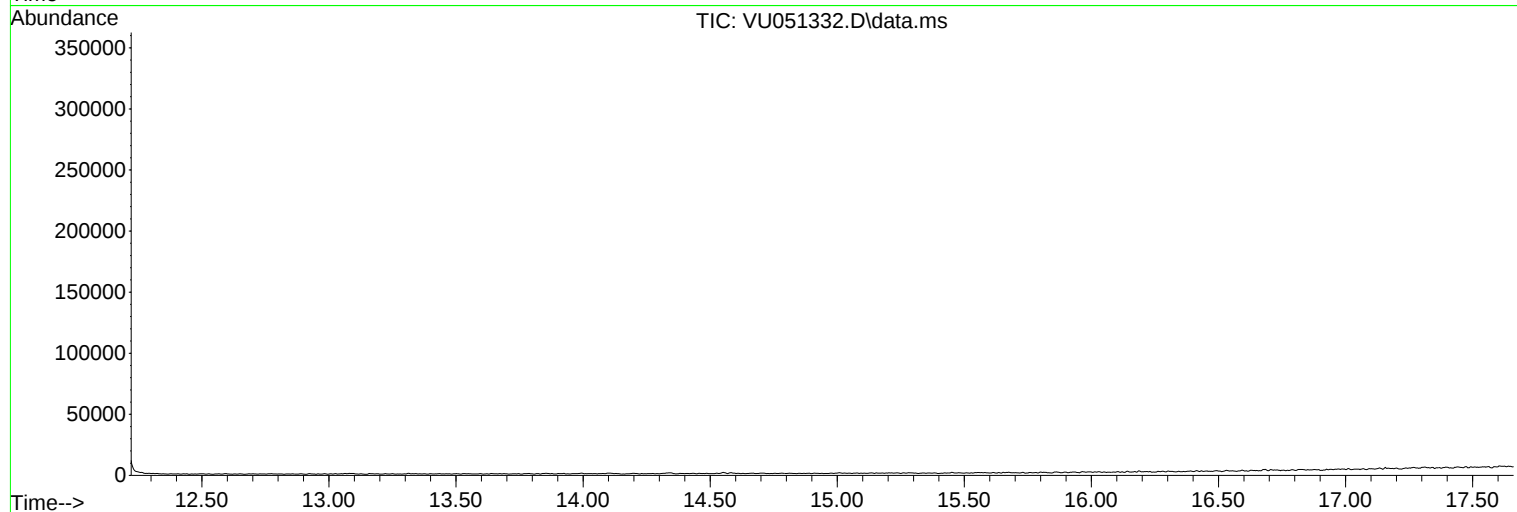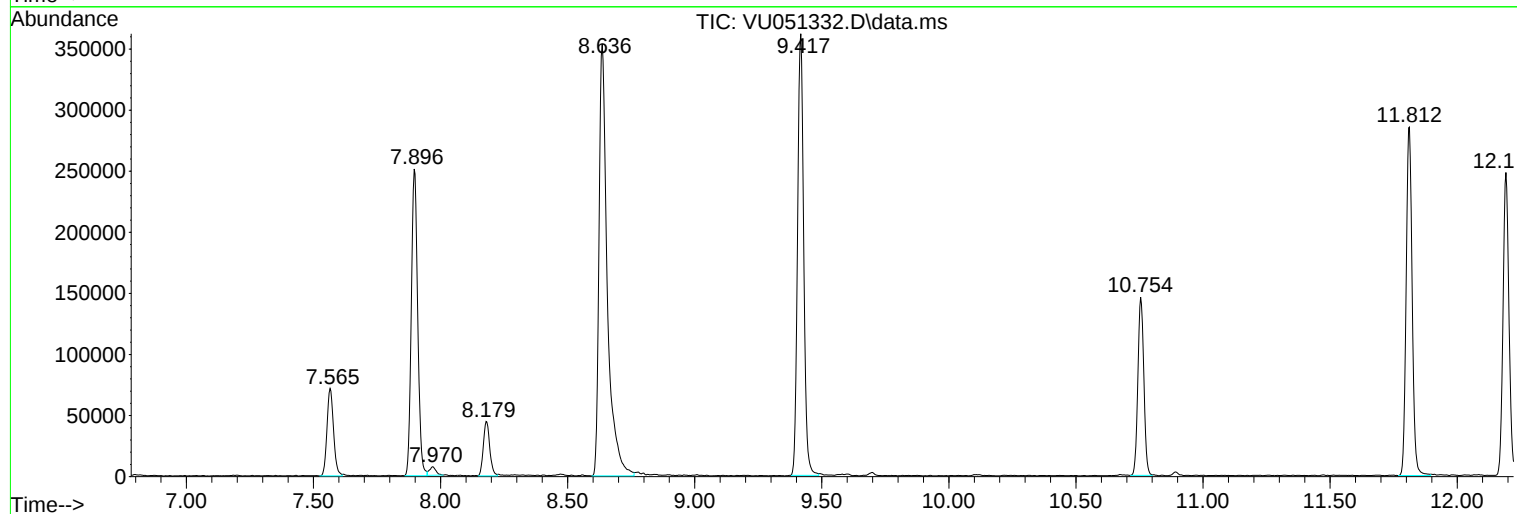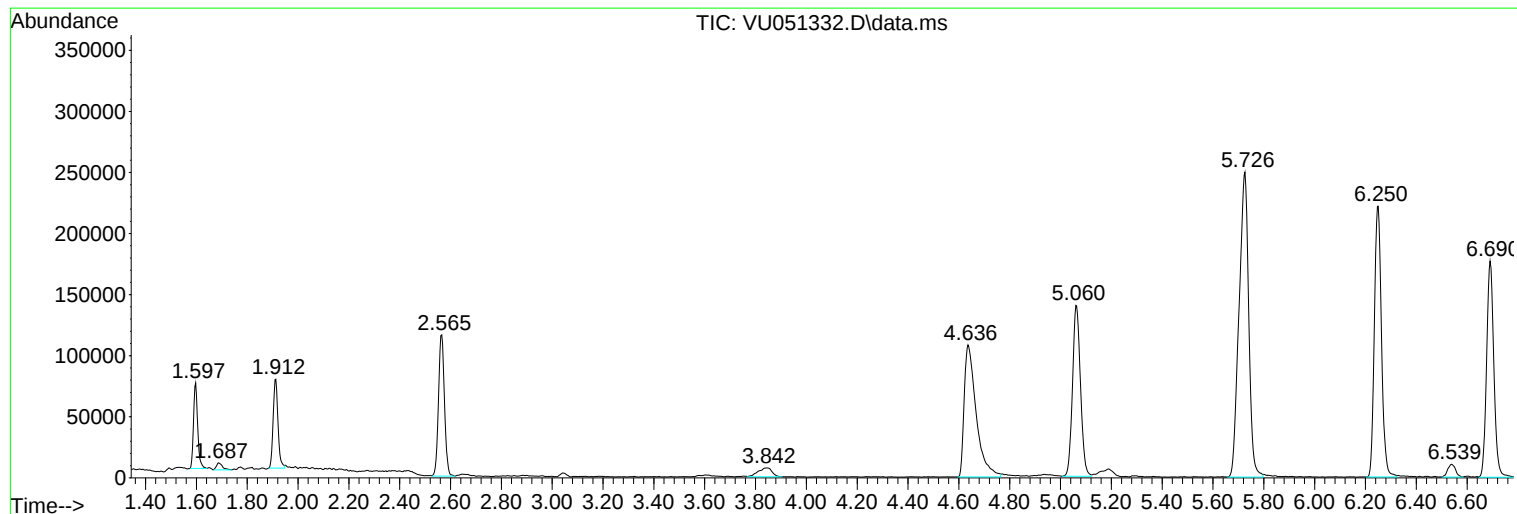

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051332.D
Acq On : 10 Oct 2022 17:17
Operator : JC/MD
Sample : N5041-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051332.D
Acq On : 10 Oct 2022 17:17
Operator : JC/MD
Sample : N5041-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc