

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051333.D
 Acq On : 10 Oct 2022 17:42
 Operator : JC/MD
 Sample : N5026-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B96

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rVB	68134	78298	9.57%	1.347%
2	1.912	170	178	189	rBV	73921	96890	11.84%	1.667%
3	2.565	367	381	395	rBV	116423	187478	22.91%	3.225%
4	2.652	397	408	421	rVB2	4935	11605	1.42%	0.200%
5	3.861	761	784	801	rVB	7458	26897	3.29%	0.463%
6	4.633	1011	1024	1059	rBV	123207	358105	43.76%	6.159%
7	5.063	1142	1158	1179	rBV	148348	330123	40.34%	5.678%
8	5.723	1340	1363	1389	rBV3	255500	677022	82.74%	11.645%
9	6.247	1513	1526	1546	rBV	229203	443247	54.17%	7.624%
10	6.690	1648	1664	1683	rBV	179127	350875	42.88%	6.035%
11	7.565	1923	1936	1950	rBV	72478	129955	15.88%	2.235%
12	7.896	2022	2039	2056	rBV	259134	451411	55.17%	7.764%
13	7.967	2057	2061	2076	rVB3	6562	10034	1.23%	0.173%
14	8.179	2116	2127	2140	rBV2	46326	78046	9.54%	1.342%
15	8.636	2257	2269	2308	rBV3	361910	818263	100.00%	14.074%
16	9.417	2497	2512	2531	rBV	365513	618952	75.64%	10.646%
17	10.755	2915	2928	2944	rBV	150737	240997	29.45%	4.145%
18	10.890	2961	2970	2983	rVB	7130	11141	1.36%	0.192%
19	11.809	3245	3256	3287	rBV	290356	479761	58.63%	8.252%
20	12.192	3362	3375	3402	rBV	250693	414820	50.70%	7.135%




Sum of corrected areas: 5813920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051333.D
Acq On : 10 Oct 2022 17:42
Operator : JC/MD
Sample : N5026-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

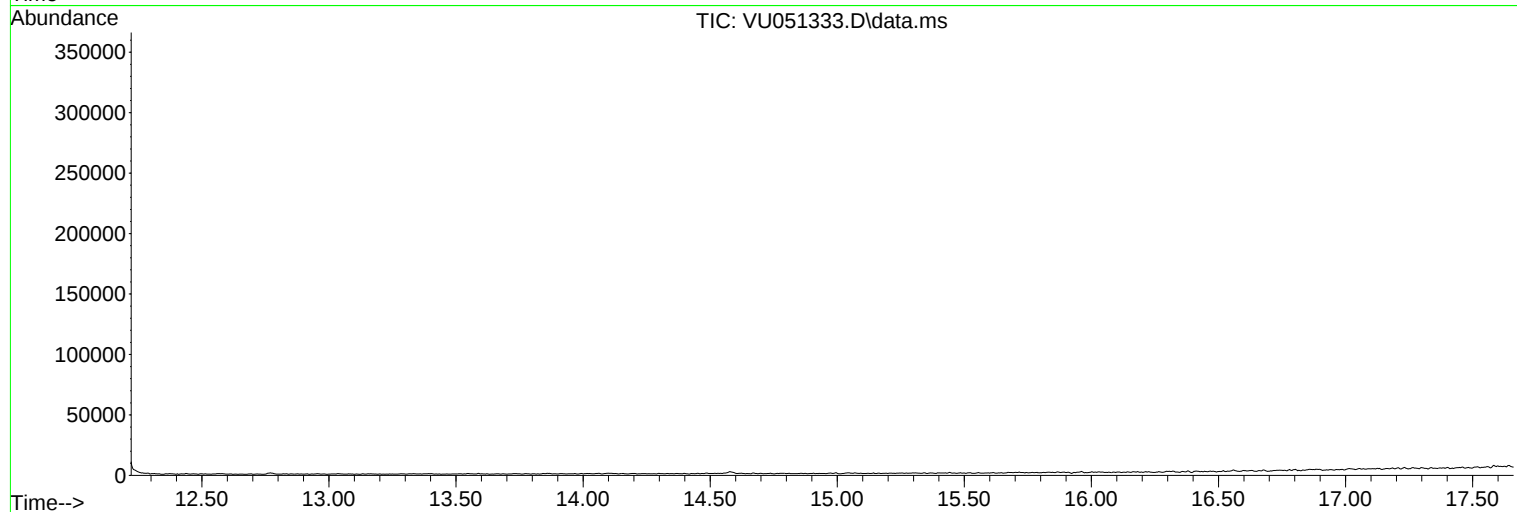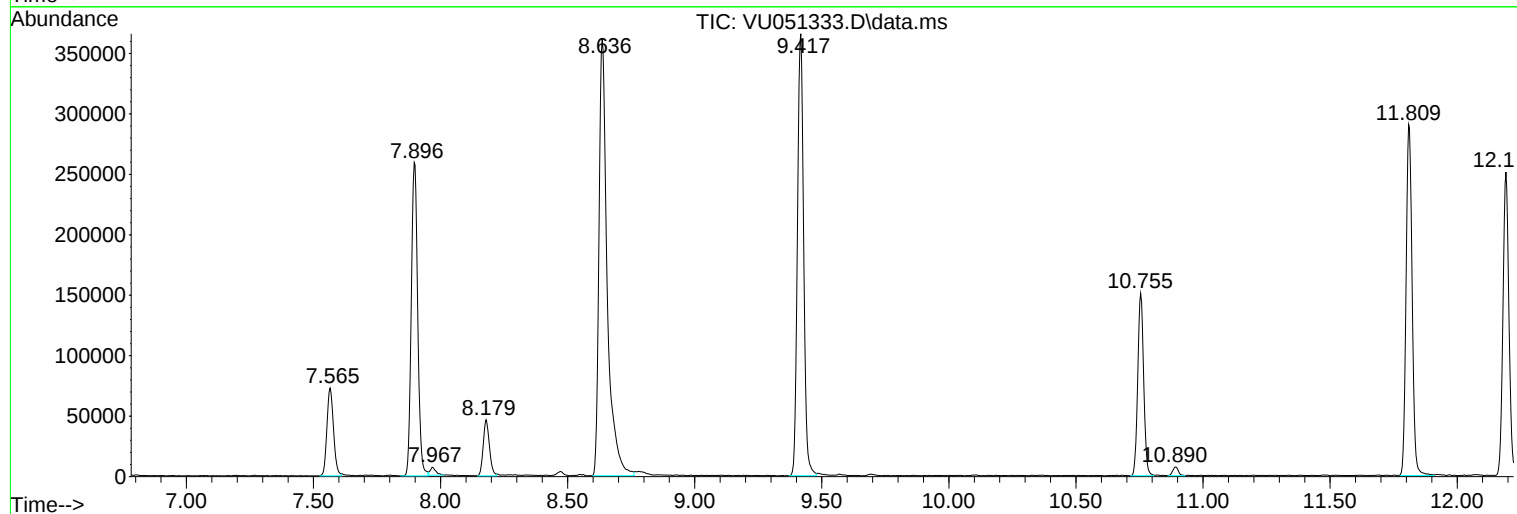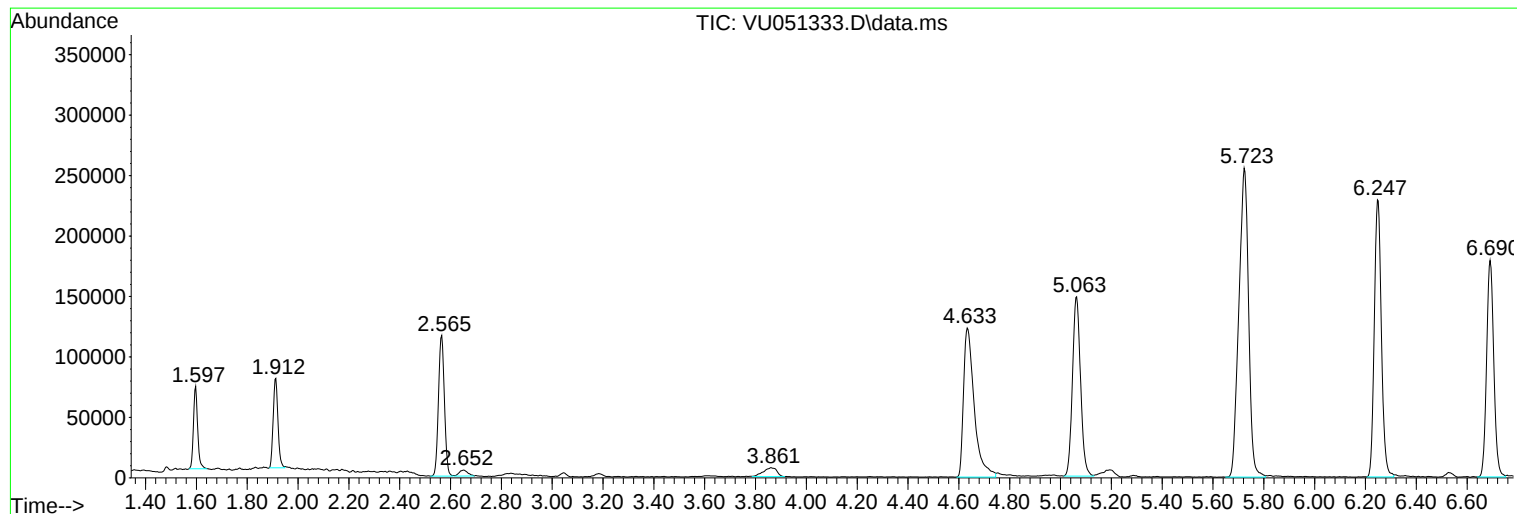

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051333.D
Acq On : 10 Oct 2022 17:42
Operator : JC/MD
Sample : N5026-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051333.D
Acq On : 10 Oct 2022 17:42
Operator : JC/MD
Sample : N5026-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc