

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051336.D
 Acq On : 10 Oct 2022 18:56
 Operator : JC/MD
 Sample : N5026-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B97

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	72	80	94	rBV	69517	79726	11.38%	1.438%
2	1.768	127	133	141	rVB4	7020	7978	1.14%	0.144%
3	1.913	170	178	194	rVB	72595	94710	13.52%	1.709%
4	2.565	369	381	393	rBV	114975	185737	26.52%	3.351%
5	2.623	393	399	415	rVB	8566	14754	2.11%	0.266%
6	2.755	430	440	457	rBV2	9205	18550	2.65%	0.335%
7	3.186	562	574	587	rVB2	4405	9081	1.30%	0.164%
8	3.842	755	778	799	rVB	9689	33284	4.75%	0.600%
9	4.620	1007	1020	1055	rBV	116383	304958	43.54%	5.502%
10	5.060	1142	1157	1179	rBV	145984	321978	45.97%	5.809%
11	5.186	1180	1196	1208	rVB	6734	21282	3.04%	0.384%
12	5.723	1343	1363	1389	rBV2	249846	659835	94.20%	11.904%
13	6.247	1512	1526	1546	rBV	218949	418331	59.72%	7.547%
14	6.691	1649	1664	1684	rBV	176256	348017	49.68%	6.279%
15	7.565	1925	1936	1958	rBV	69658	124283	17.74%	2.242%
16	7.896	2023	2039	2054	rBV	257463	443710	63.34%	8.005%
17	7.974	2058	2063	2074	rVB3	4711	7343	1.05%	0.132%
18	8.179	2116	2127	2145	rBV2	43440	73184	10.45%	1.320%
19	8.633	2253	2268	2306	rBV3	308679	700474	100.00%	12.637%
20	9.417	2496	2512	2530	rBV	352636	592711	84.62%	10.693%
21	10.755	2915	2928	2945	rBV	141819	228684	32.65%	4.126%
22	11.809	3240	3256	3274	rBV	278709	454622	64.90%	8.202%
23	12.192	3363	3375	3389	rBV	242687	399639	57.05%	7.210%




Sum of corrected areas: 5542871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051336.D
Acq On : 10 Oct 2022 18:56
Operator : JC/MD
Sample : N5026-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

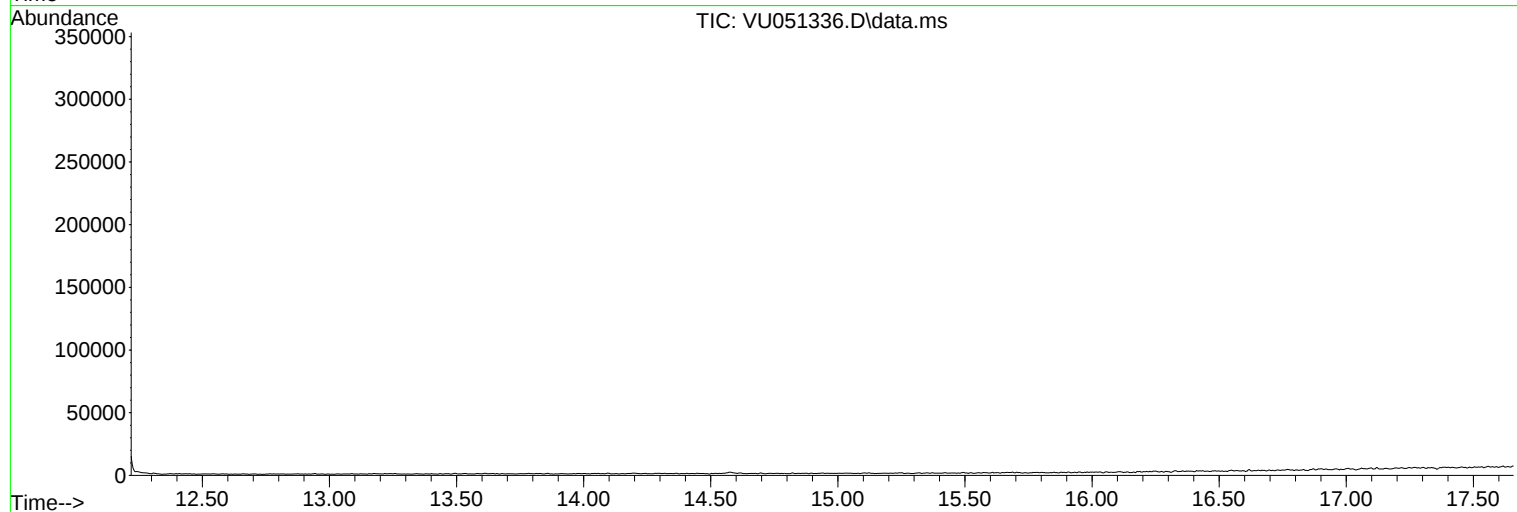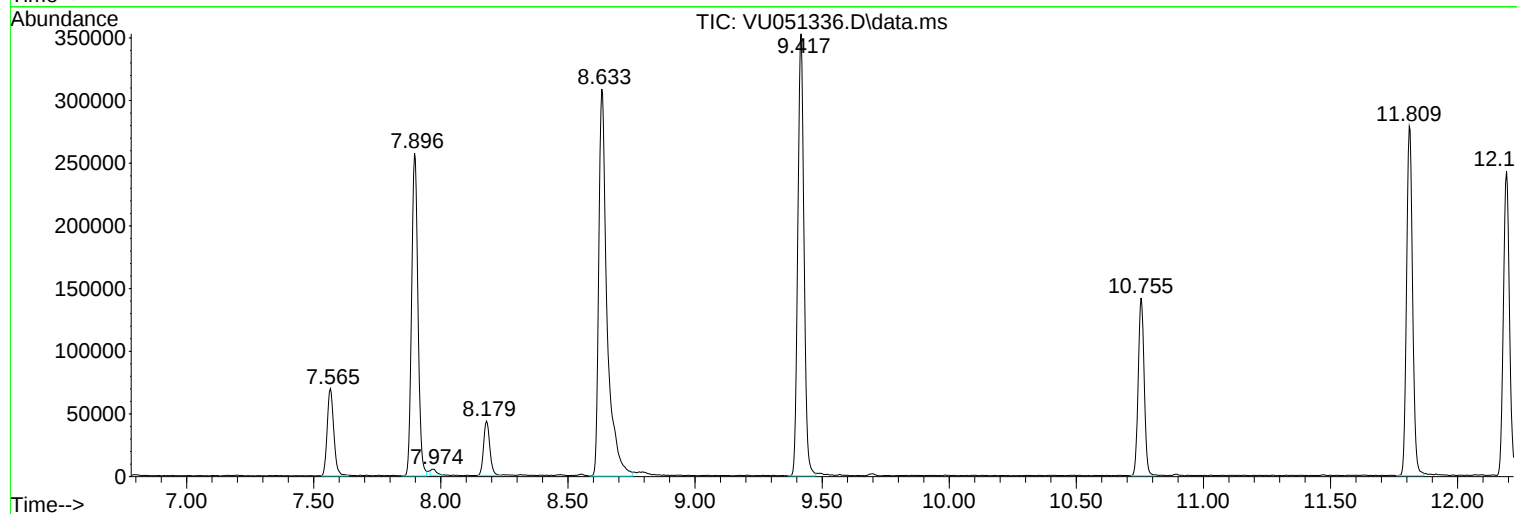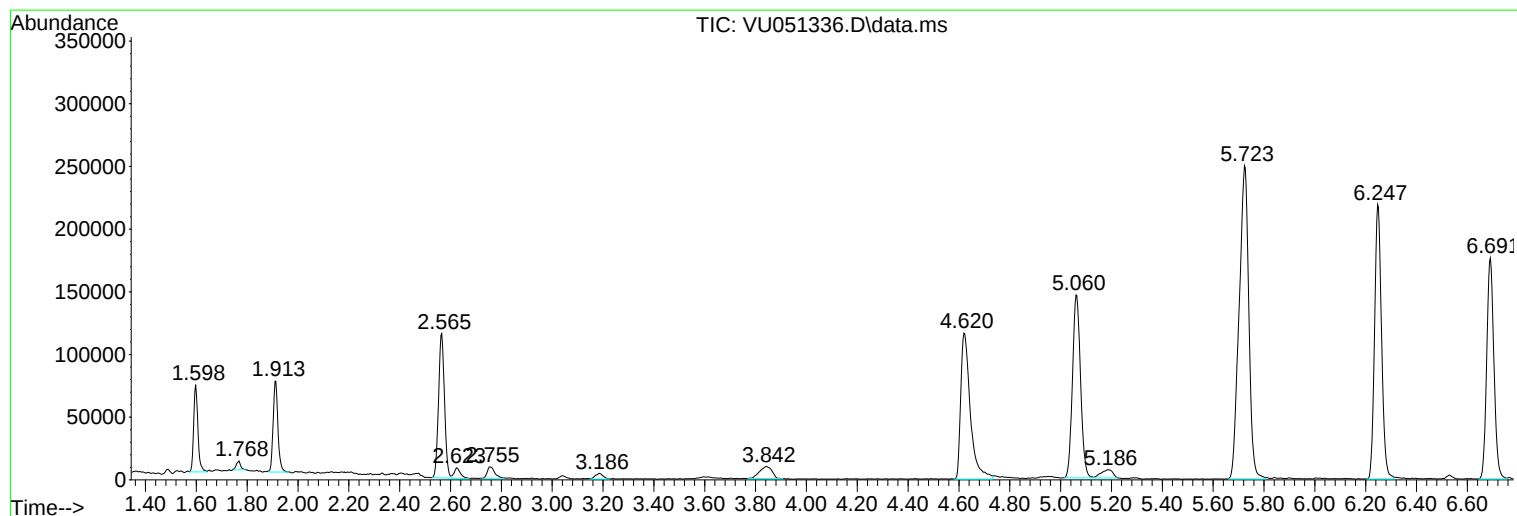

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051336.D
Acq On : 10 Oct 2022 18:56
Operator : JC/MD
Sample : N5026-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051336.D
Acq On : 10 Oct 2022 18:56
Operator : JC/MD
Sample : N5026-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc