

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051339.D
 Acq On : 10 Oct 2022 20:10
 Operator : JC/MD
 Sample : N5026-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	69770	79202	11.73%	1.459%
2	1.912	169	178	190	rBV	74837	97672	14.47%	1.799%
3	2.565	369	381	393	rBV	113130	185183	27.43%	3.410%
4	2.626	393	400	412	rVB	8312	13819	2.05%	0.254%
5	2.755	428	440	454	rBV	8344	17645	2.61%	0.325%
6	3.919	784	802	818	rVB	6401	20148	2.98%	0.371%
7	4.620	1009	1020	1048	rBV	111069	283413	41.98%	5.219%
8	5.060	1141	1157	1185	rVB	141925	317052	46.96%	5.839%
9	5.250	1196	1216	1218	rBV3	5347	10938	1.62%	0.201%
10	5.723	1343	1363	1385	rBV2	242771	650026	96.28%	11.970%
11	6.247	1513	1526	1556	rBV	214100	415775	61.58%	7.657%
12	6.690	1650	1664	1687	rBV	176523	344561	51.04%	6.345%
13	7.565	1920	1936	1951	rBV	67724	120422	17.84%	2.218%
14	7.896	2023	2039	2056	rBV	247749	435449	64.50%	8.019%
15	7.970	2056	2062	2074	rVB	7093	10827	1.60%	0.199%
16	8.179	2116	2127	2142	rBV2	44628	74266	11.00%	1.368%
17	8.632	2254	2268	2300	rBV3	294555	675130	100.00%	12.433%
18	9.417	2499	2512	2532	rBV	355319	595840	88.26%	10.973%
19	10.754	2913	2928	2952	rBV	142084	228683	33.87%	4.211%
20	11.809	3241	3256	3275	rBV	276924	451097	66.82%	8.307%
21	12.192	3362	3375	3396	rBV	241983	403098	59.71%	7.423%




Sum of corrected areas: 5430246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051339.D
Acq On : 10 Oct 2022 20:10
Operator : JC/MD
Sample : N5026-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

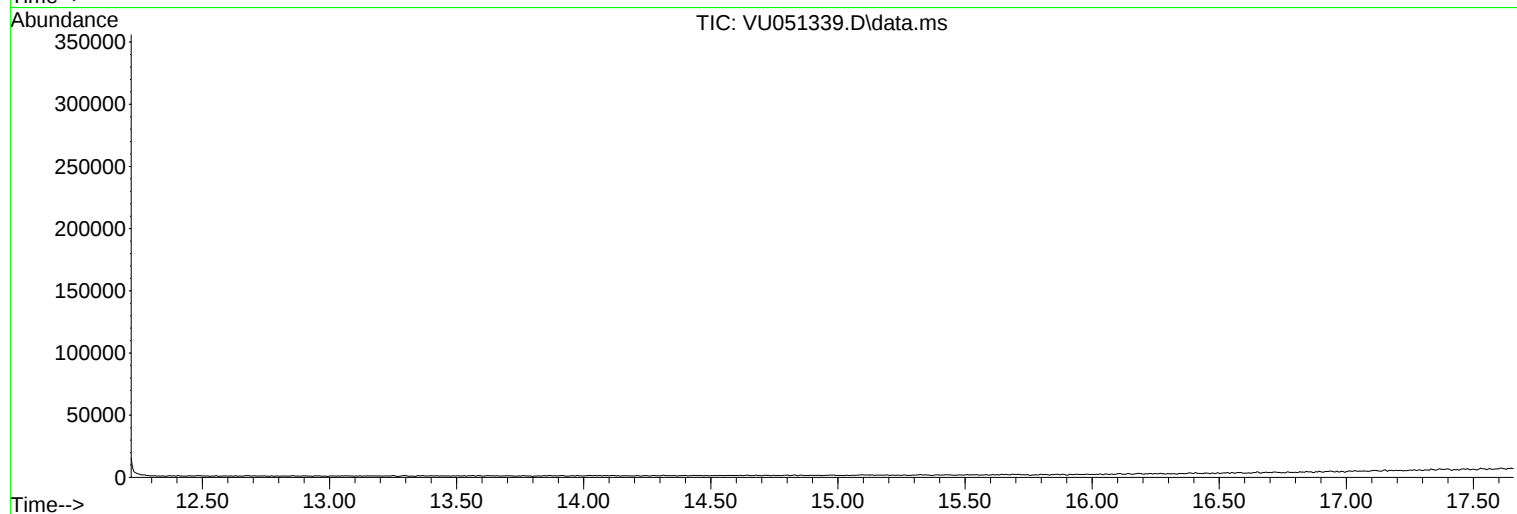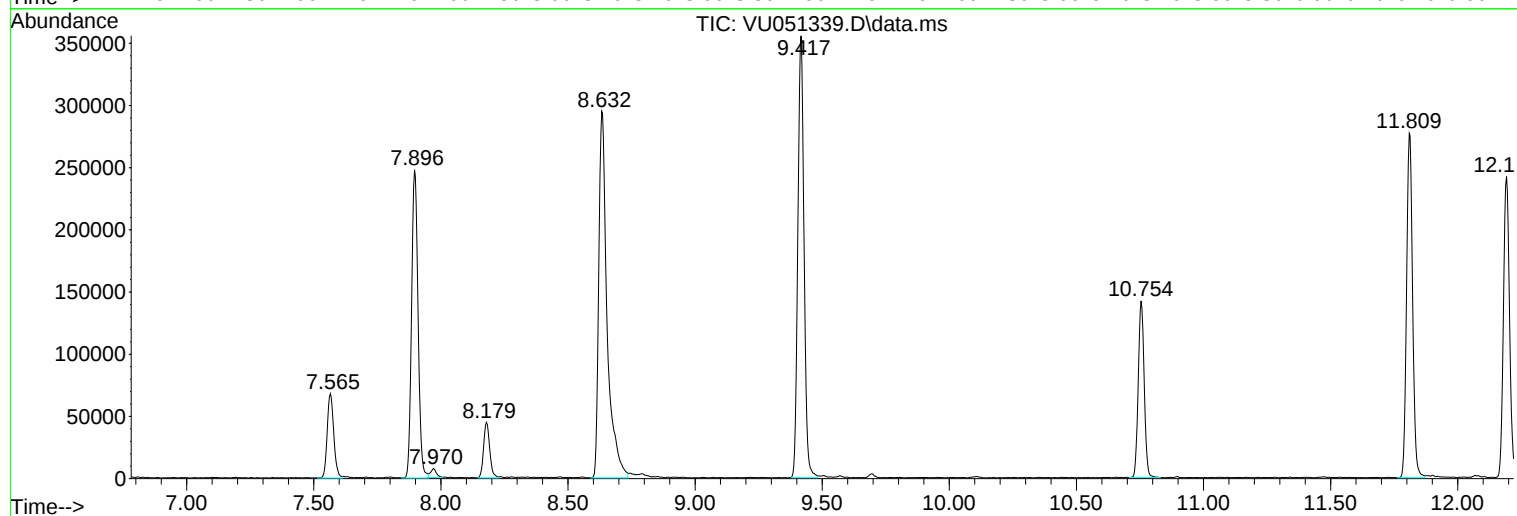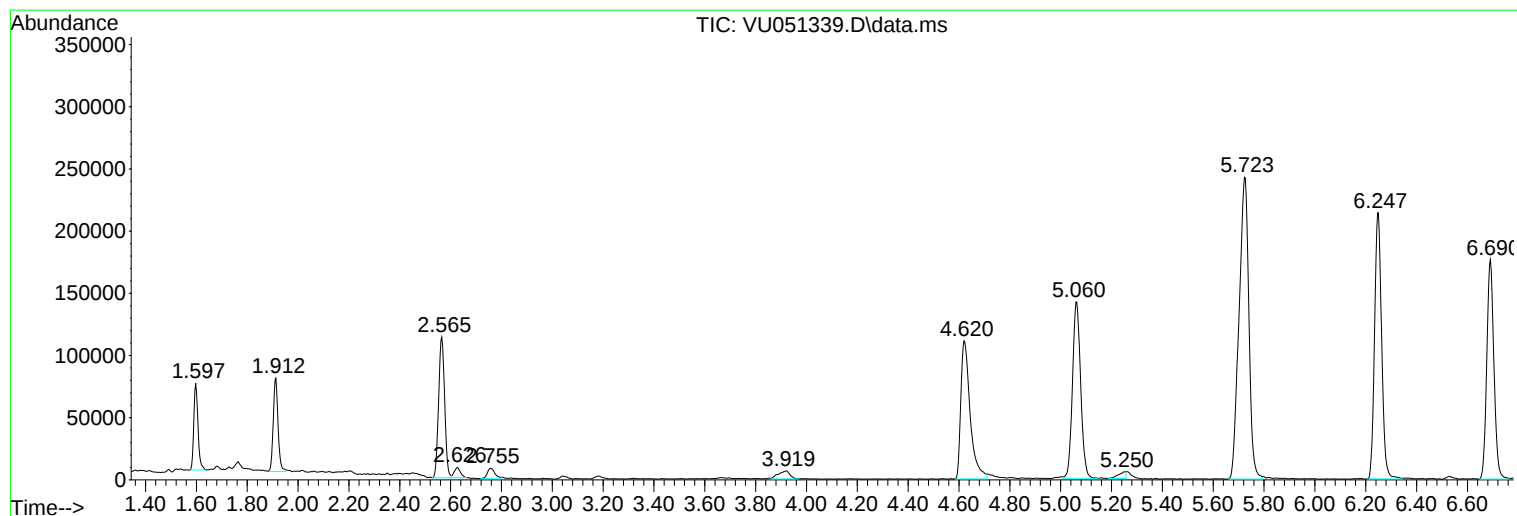

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051339.D
Acq On : 10 Oct 2022 20:10
Operator : JC/MD
Sample : N5026-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051339.D
Acq On : 10 Oct 2022 20:10
Operator : JC/MD
Sample : N5026-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
