

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051344.D
 Acq On : 10 Oct 2022 22:47
 Operator : JC/MD
 Sample : N5013-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	82634	96563	13.06%	1.618%
2	1.909	169	177	192	rVB	82483	110094	14.89%	1.844%
3	2.565	368	381	399	rBV	129293	211214	28.56%	3.538%
4	3.044	518	530	545	rVB2	20878	38506	5.21%	0.645%
5	3.179	558	572	587	rBV3	4478	9718	1.31%	0.163%
6	3.838	759	777	795	rVB	5771	19909	2.69%	0.334%
7	4.633	1008	1024	1054	rBV2	126398	348142	47.07%	5.832%
8	5.060	1141	1157	1176	rBV	149368	329005	44.49%	5.511%
9	5.179	1181	1194	1212	rVB	5977	20032	2.71%	0.336%
10	5.723	1339	1363	1396	rBV2	263744	712548	96.35%	11.936%
11	6.247	1513	1526	1548	rBV	241404	463079	62.61%	7.757%
12	6.690	1650	1664	1686	rBV	186268	363000	49.08%	6.081%
13	7.565	1925	1936	1957	rBV2	70592	128576	17.39%	2.154%
14	7.896	2025	2039	2054	rBV	270862	477482	64.56%	7.999%
15	7.970	2055	2062	2073	rVB2	8384	15011	2.03%	0.251%
16	8.179	2115	2127	2147	rBV	45619	80213	10.85%	1.344%
17	8.636	2257	2269	2305	rBV3	328208	739579	100.00%	12.389%
18	9.417	2499	2512	2531	rBV	378696	642893	86.93%	10.770%
19	10.755	2915	2928	2947	rBV	147134	235374	31.83%	3.943%
20	11.809	3244	3256	3274	rBV	308700	500612	67.69%	8.386%
21	12.192	3362	3375	3392	rBV	264145	427985	57.87%	7.169%




Sum of corrected areas: 5969535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051344.D
Acq On : 10 Oct 2022 22:47
Operator : JC/MD
Sample : N5013-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

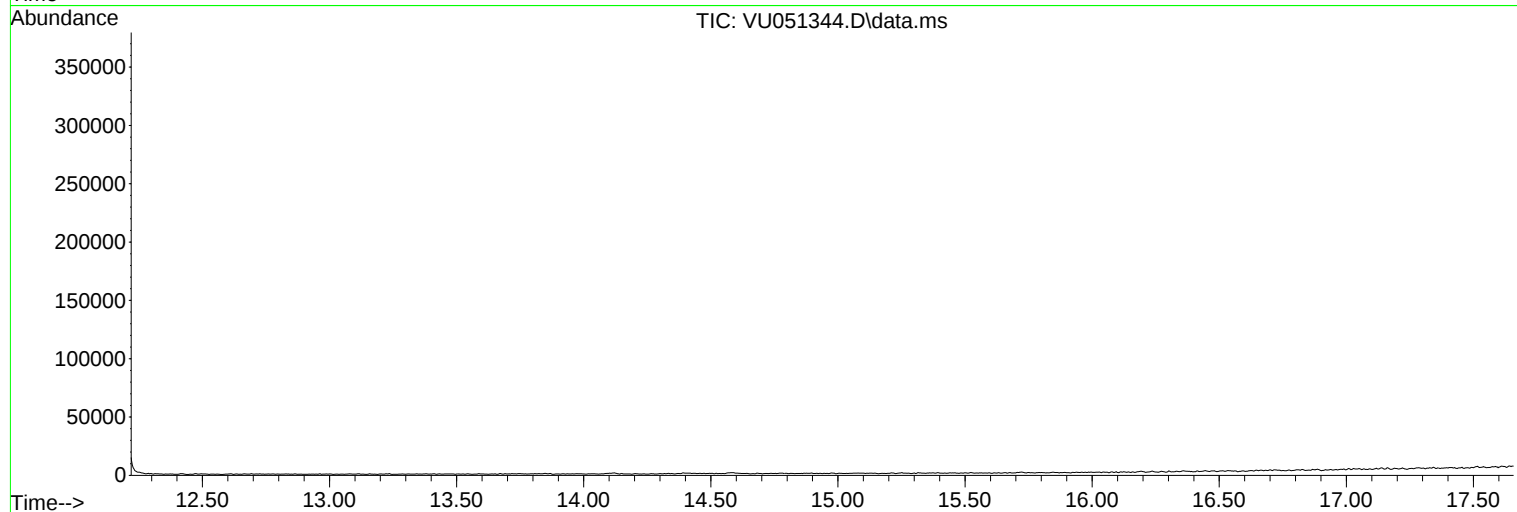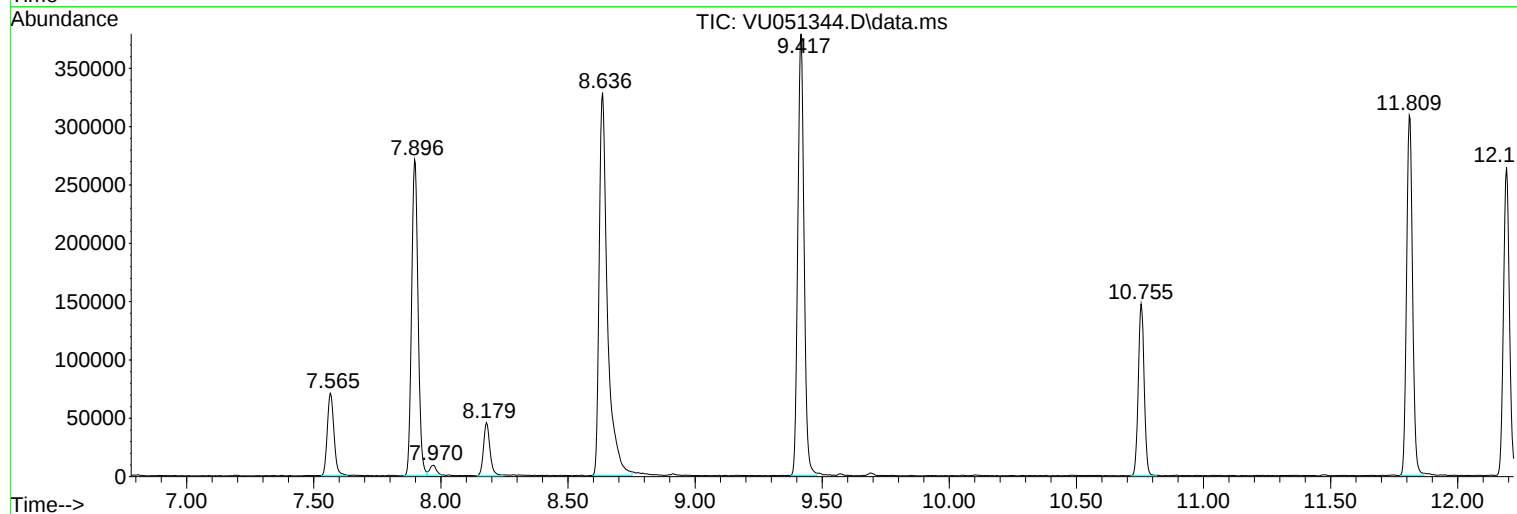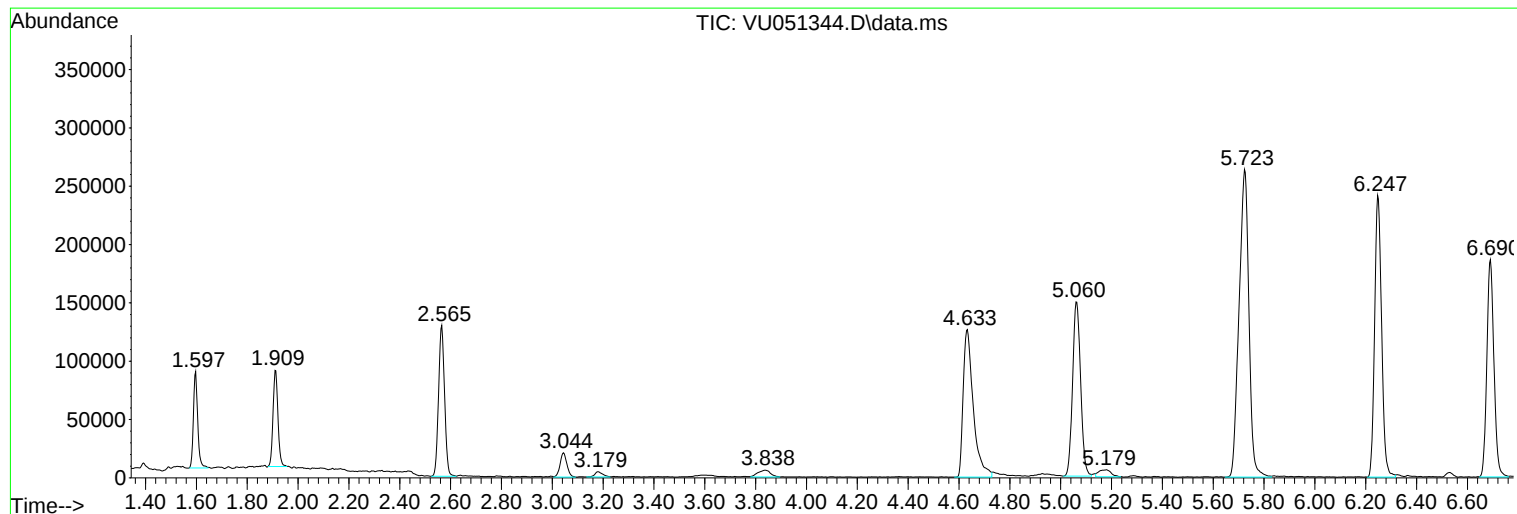

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051344.D
Acq On : 10 Oct 2022 22:47
Operator : JC/MD
Sample : N5013-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051344.D
Acq On : 10 Oct 2022 22:47
Operator : JC/MD
Sample : N5013-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
