

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051346.D
 Acq On : 10 Oct 2022 23:37
 Operator : JC/MD
 Sample : N5071-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	52	57	67	rBV2	6017	9547	1.42%	0.176%
2	1.597	73	80	93	rVB	70612	78999	11.73%	1.455%
3	1.912	170	178	192	rBV	71388	92585	13.75%	1.705%
4	2.565	369	381	393	rBV	110987	177903	26.42%	3.276%
5	2.626	393	400	414	rVB	10108	16778	2.49%	0.309%
6	3.845	758	779	804	rVB	10984	38031	5.65%	0.700%
7	4.620	1008	1020	1058	rBV	105835	286721	42.59%	5.279%
8	5.063	1141	1158	1178	rBV	134644	302133	44.87%	5.563%
9	5.189	1178	1197	1214	rVB	8922	30563	4.54%	0.563%
10	5.726	1342	1364	1392	rBV2	240135	642300	95.40%	11.826%
11	6.250	1513	1527	1549	rBV	217561	421919	62.67%	7.769%
12	6.690	1649	1664	1680	rBV2	170846	336125	49.92%	6.189%
13	7.565	1923	1936	1954	rBV	64653	118169	17.55%	2.176%
14	7.896	2026	2039	2056	rBV	245277	425454	63.19%	7.834%
15	7.970	2057	2062	2073	rVB3	4815	7764	1.15%	0.143%
16	8.179	2116	2127	2141	rBV	41384	70946	10.54%	1.306%
17	8.632	2256	2268	2306	rBV2	288142	673284	100.00%	12.397%
18	8.787	2310	2316	2329	rVB5	7578	12298	1.83%	0.226%
19	9.417	2499	2512	2535	rBV	353556	593300	88.12%	10.924%
20	10.755	2915	2928	2942	rBV	137086	224711	33.38%	4.138%
21	11.812	3245	3257	3275	rBV	271484	450331	66.89%	8.292%
22	12.063	3325	3335	3349	rBV3	14489	27376	4.07%	0.504%
23	12.192	3361	3375	3392	rBV	237032	393813	58.49%	7.251%




Sum of corrected areas: 5431050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051346.D
Acq On : 10 Oct 2022 23:37
Operator : JC/MD
Sample : N5071-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

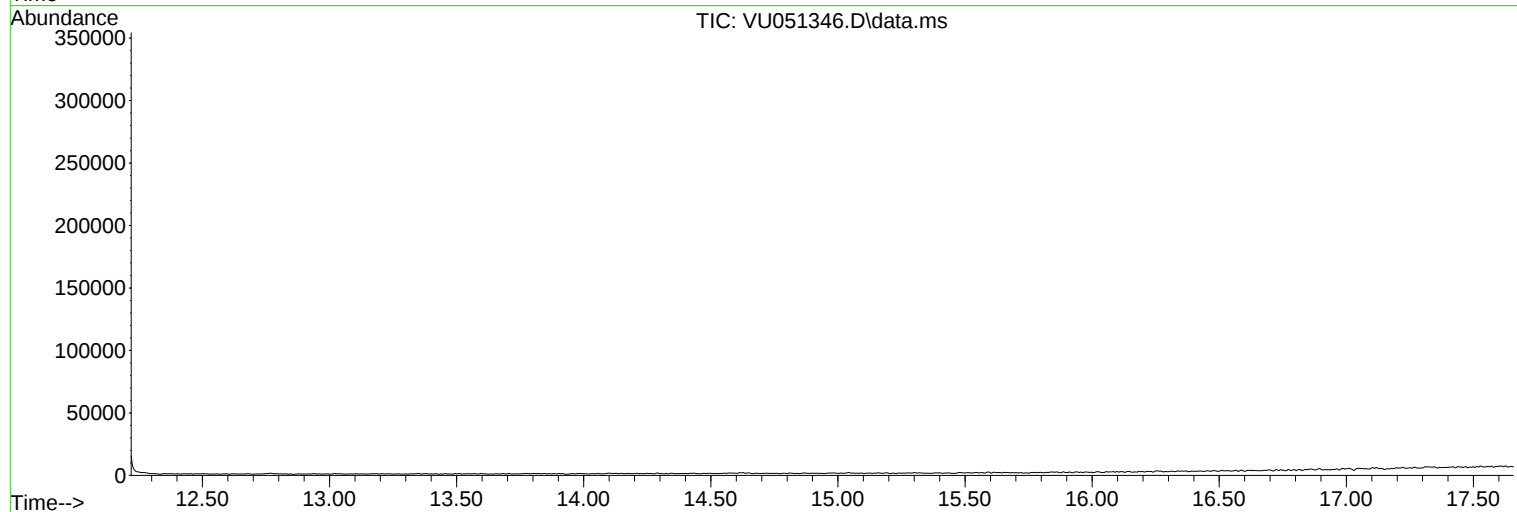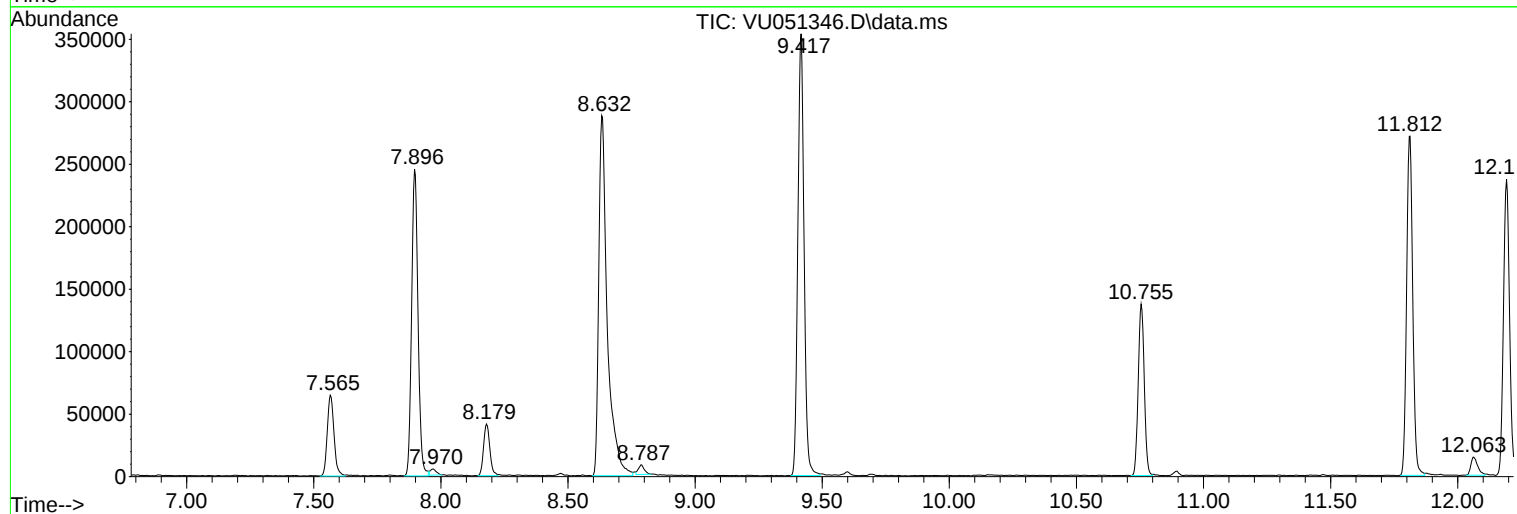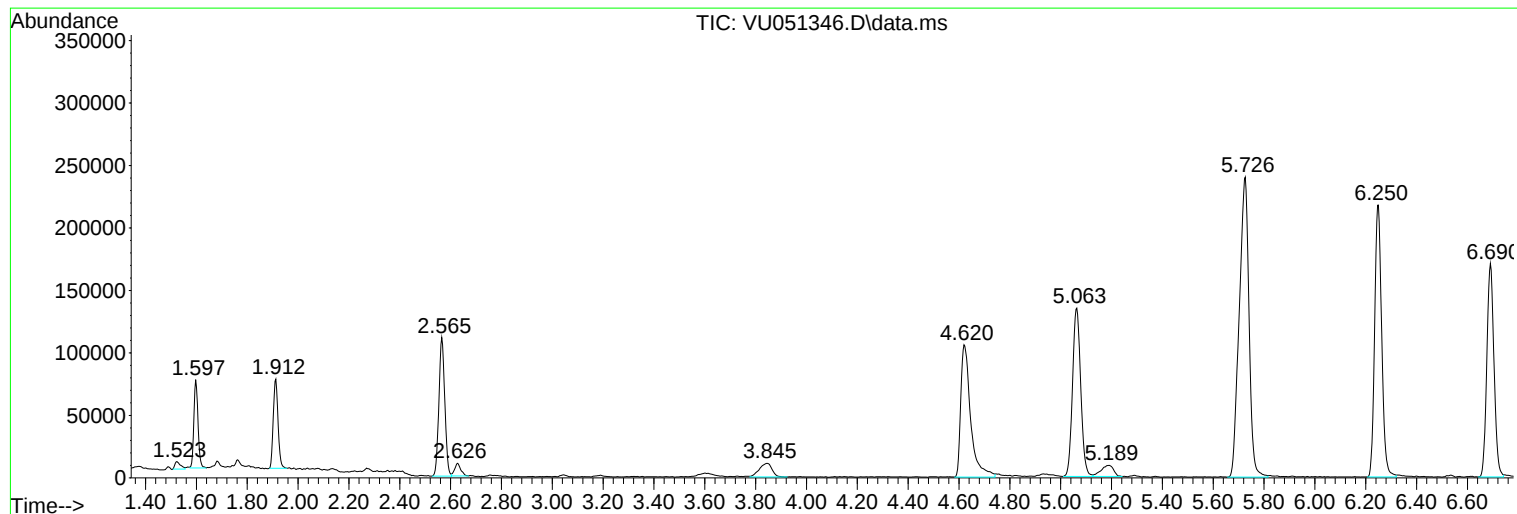

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051346.D
Acq On : 10 Oct 2022 23:37
Operator : JC/MD
Sample : N5071-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051346.D
Acq On : 10 Oct 2022 23:37
Operator : JC/MD
Sample : N5071-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc