

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
 Data File : VU051350.D
 Acq On : 11 Oct 2022 01:16
 Operator : JC/MD
 Sample : N5071-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1BB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	51	57	67	rBV2	10496	14974	2.22%	0.284%
2	1.597	73	80	93	rVB	68010	77710	11.54%	1.471%
3	1.912	170	178	200	rVB	69299	93073	13.82%	1.762%
4	2.565	367	381	392	rBV	107756	176573	26.22%	3.343%
5	2.626	393	400	413	rVB2	6706	11550	1.72%	0.219%
6	3.842	755	778	796	rVB	10820	38030	5.65%	0.720%
7	4.623	1006	1021	1060	rBV	108142	285158	42.35%	5.399%
8	5.063	1142	1158	1177	rBV	136480	299683	44.50%	5.674%
9	5.179	1181	1194	1195	rBV3	5936	8617	1.28%	0.163%
10	5.726	1343	1364	1384	rBV2	232252	626504	93.04%	11.863%
11	6.250	1513	1527	1544	rBV	205075	398017	59.11%	7.536%
12	6.690	1648	1664	1685	rBV	169133	331207	49.19%	6.271%
13	7.565	1924	1936	1956	rBV2	62953	112397	16.69%	2.128%
14	7.896	2026	2039	2057	rBV	234757	411208	61.07%	7.786%
15	7.970	2057	2062	2073	rVB2	5088	8426	1.25%	0.160%
16	8.179	2116	2127	2151	rBV2	39231	68594	10.19%	1.299%
17	8.636	2257	2269	2304	rBV3	286773	673376	100.00%	12.750%
18	8.783	2311	2315	2328	rVB10	4301	7893	1.17%	0.149%
19	9.417	2495	2512	2531	rBV	337010	564431	83.82%	10.687%
20	10.754	2914	2928	2948	rBV	136324	225176	33.44%	4.264%
21	11.812	3245	3257	3284	rBV	264914	427916	63.55%	8.102%
22	12.063	3324	3335	3347	rBV3	17634	32244	4.79%	0.611%
23	12.192	3362	3375	3398	rBV	232696	388587	57.71%	7.358%




Sum of corrected areas: 5281344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051350.D
Acq On : 11 Oct 2022 01:16
Operator : JC/MD
Sample : N5071-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

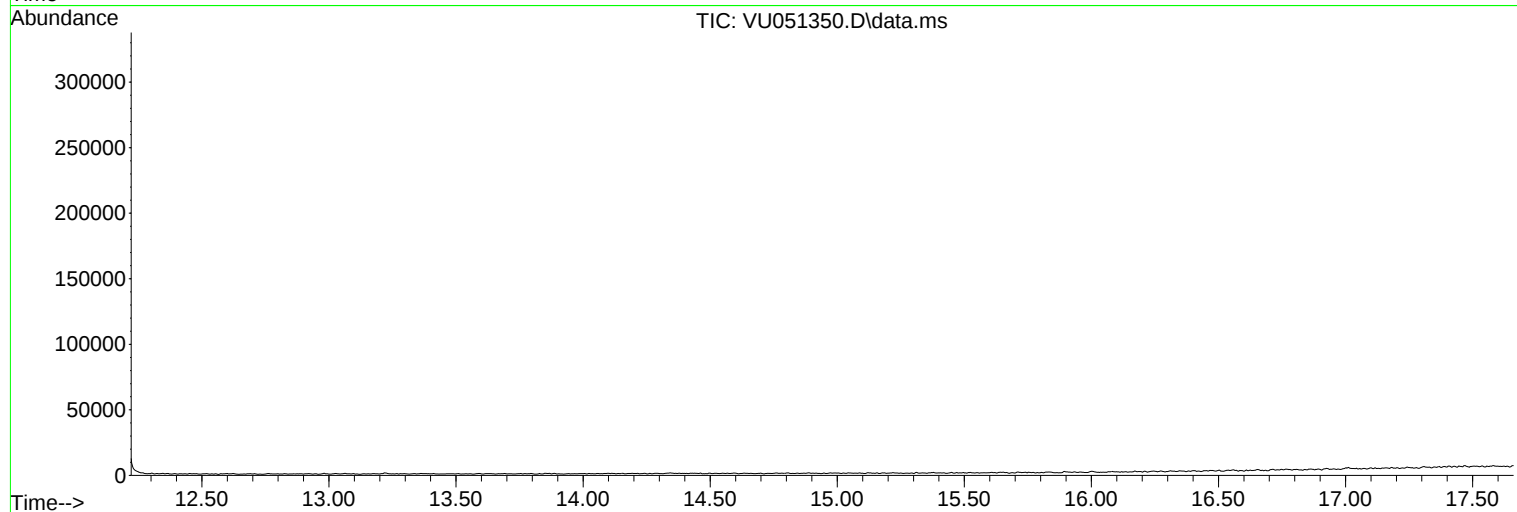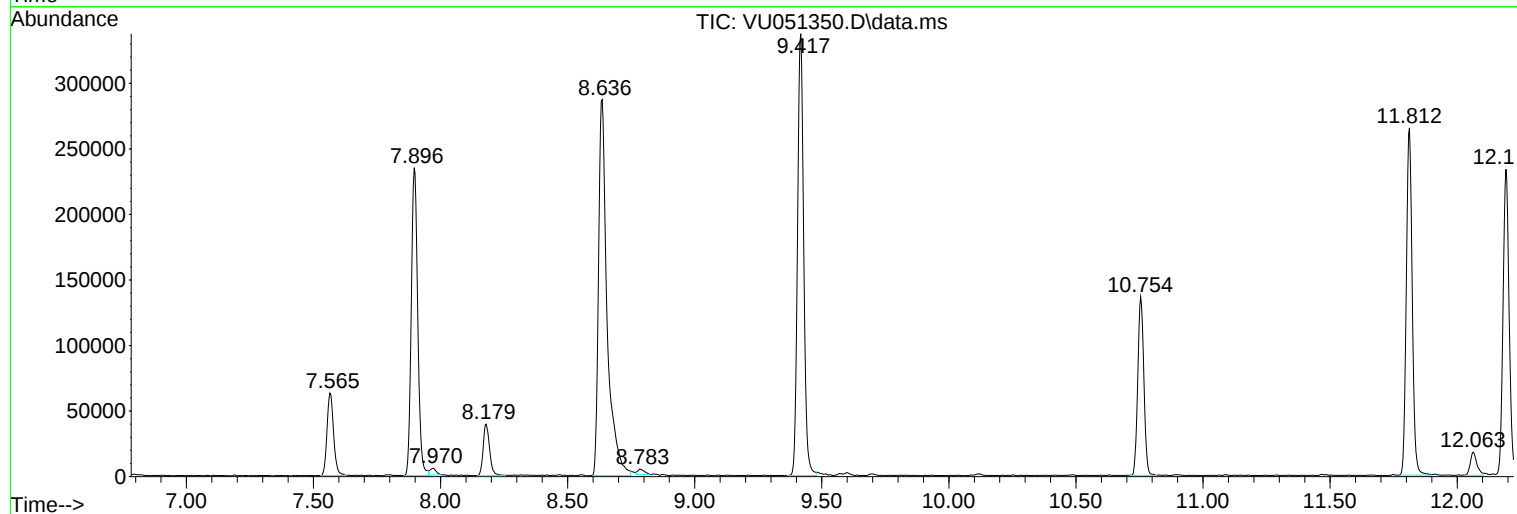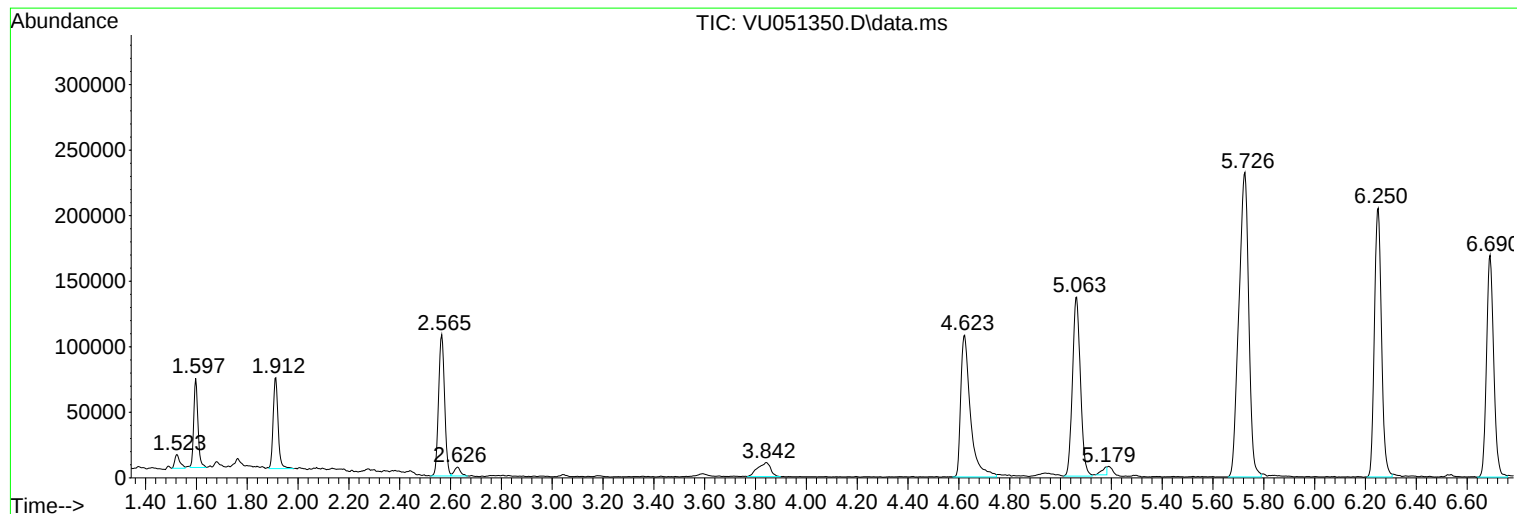

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051350.D
Acq On : 11 Oct 2022 01:16
Operator : JC/MD
Sample : N5071-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101022\
Data File : VU051350.D
Acq On : 11 Oct 2022 01:16
Operator : JC/MD
Sample : N5071-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1BB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc