

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055722.D
 Acq On : 10 Oct 2023 15:35
 Operator : MD/SY
 Sample : 04360-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	116	rBV	220049	266927	14.61%	1.899%
2	1.888	179	186	204	rVB	171199	252568	13.82%	1.797%
3	2.557	383	394	408	rBV	365302	600775	32.88%	4.273%
4	2.911	501	504	507	rBV2	481	331	0.02%	0.002%
5	3.036	535	543	556	rVB2	10957	20141	1.10%	0.143%
6	3.126	568	571	573	rBV2	303	211	0.01%	0.002%
7	3.177	574	587	602	rBV	16055	37200	2.04%	0.265%
8	3.341	633	638	647	rBV2	965	1286	0.07%	0.009%
9	3.380	647	650	654	rVB2	358	165	0.01%	0.001%
10	3.399	654	656	660	rVB2	243	173	0.01%	0.001%
11	3.422	660	663	665	rBV2	231	171	0.01%	0.001%
12	3.448	669	671	673	rBV2	260	119	0.01%	0.001%
13	3.512	686	691	693	rBV2	325	156	0.01%	0.001%
14	3.644	730	732	735	rBV	283	197	0.01%	0.001%
15	3.692	745	747	748	rBV2	283	130	0.01%	0.001%
16	3.769	767	771	774	rVV2	598	525	0.03%	0.004%
17	3.795	778	779	782	rVV2	330	118	0.01%	0.001%
18	3.817	782	786	790	rVB2	402	306	0.02%	0.002%
19	3.869	798	802	807	rVB2	469	371	0.02%	0.003%
20	4.020	843	849	852	rBV2	333	381	0.02%	0.003%
21	4.036	852	854	857	rBV2	234	158	0.01%	0.001%
22	4.097	871	873	877	rVB2	380	220	0.01%	0.002%
23	4.116	877	879	881	rBV2	408	203	0.01%	0.001%
24	4.139	883	886	890	rVB	502	301	0.02%	0.002%
25	4.267	923	926	929	rBV2	321	245	0.01%	0.002%
26	4.287	929	932	936	rVB	318	228	0.01%	0.002%
27	4.348	949	951	957	rVB2	296	205	0.01%	0.001%
28	4.396	962	966	968	rBV	449	298	0.02%	0.002%
29	4.454	981	984	987	rBV2	282	193	0.01%	0.001%
30	4.489	987	995	996	rBV2	286	264	0.01%	0.002%
31	4.544	1009	1012	1016	rBV2	379	273	0.01%	0.002%
32	4.563	1016	1018	1021	rBV2	433	247	0.01%	0.002%
33	4.615	1021	1034	1063	rBV	169901	444595	24.33%	3.162%
34	5.055	1155	1171	1196	rBV	325686	724679	39.66%	5.155%
35	5.451	1285	1294	1298	rBV2	231	317	0.02%	0.002%
36	5.579	1329	1334	1337	rBV2	314	300	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055722.D
 Acq On : 10 Oct 2023 15:35
 Operator : MD/SY
 Sample : 04360-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	5.599	1337	1340	1346	rVB3	351	335	0.02%	0.002%
38	5.634	1347	1351	1354	rBV	403	332	0.02%	0.002%
39	5.718	1354	1377	1407	rBV2	659190	1827187	100.00%	12.997%
40	6.091	1489	1493	1496	rBV3	534	466	0.03%	0.003%
41	6.110	1496	1499	1500	rVV2	402	198	0.01%	0.001%
42	6.245	1528	1541	1565	rBV	480333	932136	51.01%	6.630%
43	6.528	1618	1629	1642	rBV4	13598	26223	1.44%	0.187%
44	6.685	1664	1678	1699	rBV2	413923	816911	44.71%	5.811%
45	7.193	1825	1836	1840	rBV7	3063	5456	0.30%	0.039%
46	7.312	1870	1873	1874	rBV	211	123	0.01%	0.001%
47	7.325	1874	1877	1880	rVV2	492	331	0.02%	0.002%
48	7.345	1881	1883	1888	rVB2	624	513	0.03%	0.004%
49	7.373	1888	1892	1894	rBV2	247	230	0.01%	0.002%
50	7.422	1905	1907	1911	rVB2	441	229	0.01%	0.002%
51	7.447	1911	1915	1917	rVB2	604	357	0.02%	0.003%
52	7.473	1917	1923	1926	rBV2	223	274	0.01%	0.002%
53	7.496	1927	1930	1934	rBV2	465	454	0.02%	0.003%
54	7.563	1939	1951	1968	rBV	224610	403129	22.06%	2.867%
55	7.685	1986	1989	1990	rBV	948	580	0.03%	0.004%
56	7.894	2040	2054	2073	rBV	790152	1389057	76.02%	9.880%
57	8.074	2108	2110	2113	rVB	740	314	0.02%	0.002%
58	8.177	2130	2142	2162	rBV	161385	280814	15.37%	1.997%
59	8.322	2186	2187	2189	rBV	275	123	0.01%	0.001%
60	8.386	2204	2207	2210	rBV	476	251	0.01%	0.002%
61	8.457	2224	2229	2231	rBV3	1088	988	0.05%	0.007%
62	8.557	2253	2260	2263	rBV5	1832	2097	0.11%	0.015%
63	8.634	2271	2284	2315	rBV2	550189	1197711	65.55%	8.519%
64	9.065	2414	2418	2420	rBV	329	180	0.01%	0.001%
65	9.078	2420	2422	2426	rVV2	325	182	0.01%	0.001%
66	9.110	2430	2432	2435	rVV2	325	182	0.01%	0.001%
67	9.155	2445	2446	2449	rBV	274	126	0.01%	0.001%
68	9.171	2449	2451	2456	rVV3	555	420	0.02%	0.003%
69	9.213	2459	2464	2471	rVB4	1333	1826	0.10%	0.013%
70	9.299	2487	2491	2493	rBV2	383	336	0.02%	0.002%
71	9.415	2514	2527	2551	rBV	703530	1201476	65.76%	8.546%
72	9.553	2569	2570	2572	rBV2	606	297	0.02%	0.002%
73	9.743	2626	2629	2631	rBV	282	145	0.01%	0.001%
74	9.759	2631	2634	2637	rVB2	591	340	0.02%	0.002%
75	9.779	2637	2640	2644	rBV2	262	220	0.01%	0.002%
76	9.814	2649	2651	2653	rBV	432	198	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055722.D
 Acq On : 10 Oct 2023 15:35
 Operator : MD/SY
 Sample : 04360-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	9.849	2660	2662	2666	rBV2	214	150	0.01%	0.001%
78	9.936	2687	2689	2693	rVB	208	94	0.01%	0.001%
79	10.026	2714	2717	2719	rBV2	428	205	0.01%	0.001%
80	10.097	2736	2739	2740	rBV2	375	187	0.01%	0.001%
81	10.106	2740	2742	2745	rBV3	642	455	0.02%	0.003%
82	10.290	2796	2799	2801	rVB	346	165	0.01%	0.001%
83	10.380	2824	2827	2829	rVB	487	255	0.01%	0.002%
84	10.447	2845	2848	2851	rBV2	266	193	0.01%	0.001%
85	10.528	2870	2873	2877	rBB	471	292	0.02%	0.002%
86	10.553	2877	2881	2884	rBV3	280	269	0.01%	0.002%
87	10.692	2922	2924	2929	rBV2	326	233	0.01%	0.002%
88	10.753	2930	2943	2964	rVV	650977	1069215	58.52%	7.605%
89	11.010	3021	3023	3026	rBV2	348	251	0.01%	0.002%
90	11.045	3032	3034	3036	rBV	272	125	0.01%	0.001%
91	11.409	3143	3147	3150	rBV2	404	347	0.02%	0.002%
92	11.521	3176	3182	3184	rBV2	471	496	0.03%	0.004%
93	11.704	3237	3239	3241	rBV2	388	161	0.01%	0.001%
94	11.811	3259	3272	3295	rBV	736161	1191903	65.23%	8.478%
95	12.190	3376	3390	3414	rBV	805258	1343166	73.51%	9.554%
96	12.540	3494	3499	3504	rBV2	677	734	0.04%	0.005%
97	12.618	3521	3523	3527	rVB	762	492	0.03%	0.003%
98	12.711	3548	3552	3554	rBV2	827	607	0.03%	0.004%
99	13.418	3769	3772	3776	rBV	593	535	0.03%	0.004%
100	13.528	3803	3806	3809	rBV3	607	406	0.02%	0.003%




Sum of corrected areas: 14058660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055722.D
Acq On : 10 Oct 2023 15:35
Operator : MD/SY
Sample : 04360-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JLDA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

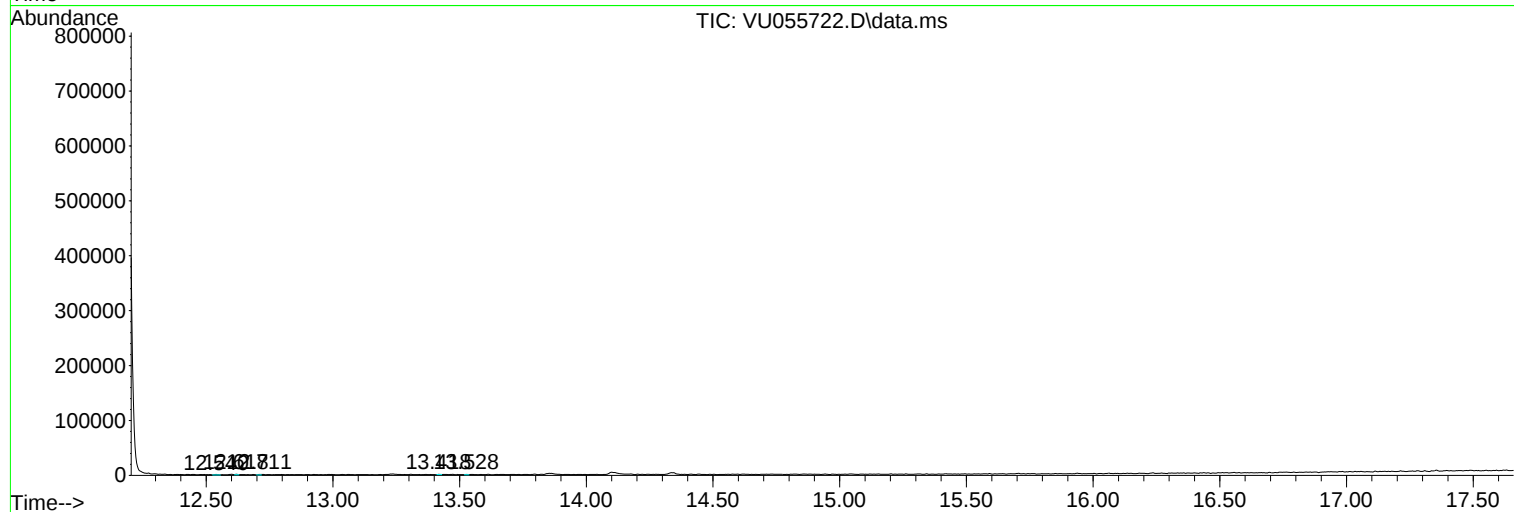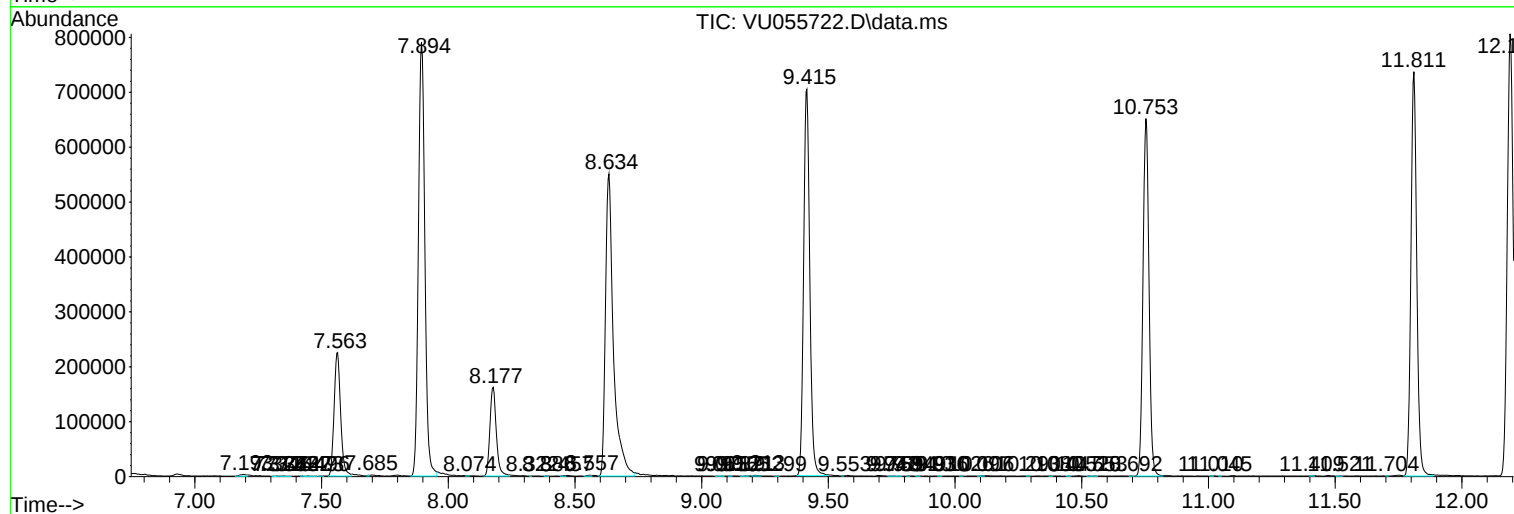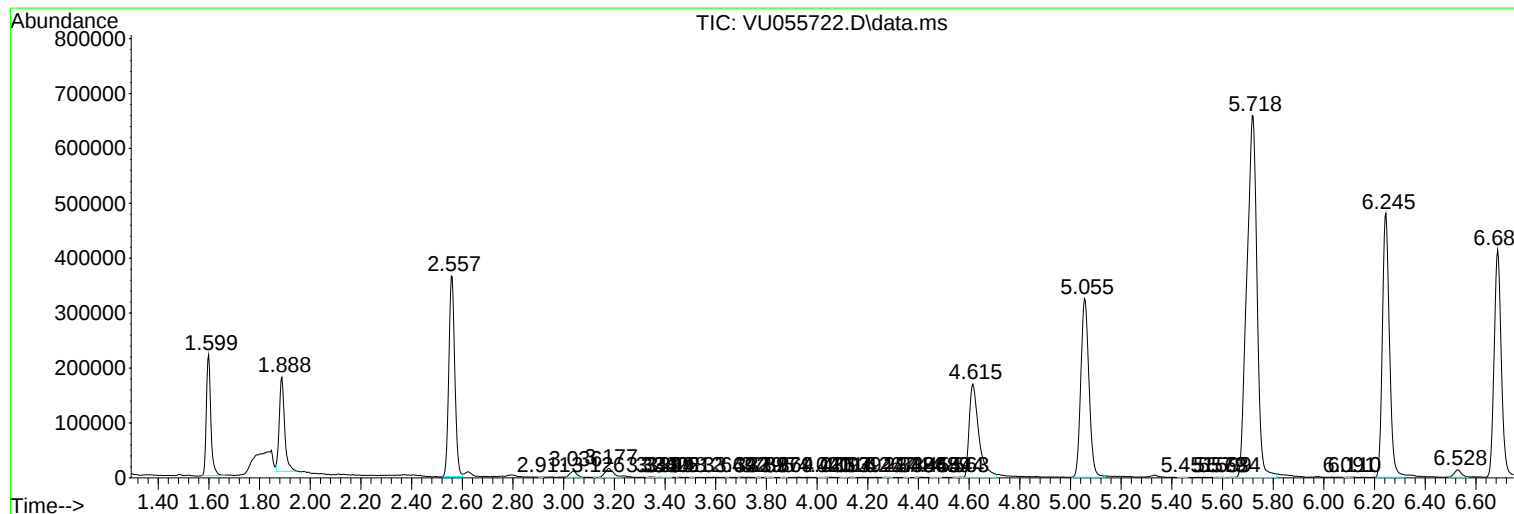

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055722.D
Acq On : 10 Oct 2023 15:35
Operator : MD/SY
Sample : 04360-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JLDA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055722.D
Acq On : 10 Oct 2023 15:35
Operator : MD/SY
Sample : 04360-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JLDA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc