

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055727.D
 Acq On : 10 Oct 2023 17:36
 Operator : MD/SY
 Sample : 04747-05ME
 Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EX840ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	124	rVB	158783	328815	14.22%	1.837%
2	2.531	375	386	410	rVB	461374	765665	33.12%	4.277%
3	3.171	570	585	602	rBV	28004	71260	3.08%	0.398%
4	3.560	704	706	707	rBV	258	66	0.00%	0.000%
5	3.592	714	716	719	rBV2	584	260	0.01%	0.001%
6	3.615	720	723	727	rVV3	900	762	0.03%	0.004%
7	3.673	730	741	751	rVB6	2146	4417	0.19%	0.025%
8	3.714	751	754	755	rBV	342	197	0.01%	0.001%
9	3.814	781	785	787	rBV3	441	334	0.01%	0.002%
10	3.853	794	797	799	rBV3	341	252	0.01%	0.001%
11	3.952	824	828	834	rVB	461	511	0.02%	0.003%
12	3.991	834	840	841	rBV	354	312	0.01%	0.002%
13	4.010	844	846	850	rVV3	285	157	0.01%	0.001%
14	4.033	852	853	856	rVB2	251	95	0.00%	0.001%
15	4.052	856	859	865	rVB2	267	237	0.01%	0.001%
16	4.087	865	870	871	rBV	292	212	0.01%	0.001%
17	4.100	871	874	875	rBV2	203	117	0.01%	0.001%
18	4.136	882	885	889	rVB2	267	170	0.01%	0.001%
19	4.158	889	892	896	rBV2	335	291	0.01%	0.002%
20	4.255	920	922	926	rVB2	274	136	0.01%	0.001%
21	4.300	931	936	938	rBV2	283	250	0.01%	0.001%
22	4.345	947	950	952	rBV	291	213	0.01%	0.001%
23	4.406	966	969	974	rBV3	561	590	0.03%	0.003%
24	4.473	988	990	994	rBV	296	260	0.01%	0.001%
25	4.525	1005	1006	1008	rBV	335	160	0.01%	0.001%
26	4.631	1024	1039	1091	rBV2	145736	590627	25.55%	3.299%
27	5.055	1155	1171	1203	rBV	377983	926885	40.09%	5.177%
28	5.309	1238	1250	1267	rBV7	6222	18485	0.80%	0.103%
29	5.467	1297	1299	1300	rBV	205	95	0.00%	0.001%
30	5.512	1300	1313	1327	rVV3	9029	20735	0.90%	0.116%
31	5.566	1329	1330	1333	rVB	312	113	0.00%	0.001%
32	5.592	1333	1338	1341	rBV	507	411	0.02%	0.002%
33	5.714	1356	1376	1405	rBV2	873989	2312027	100.00%	12.914%
34	6.100	1494	1496	1499	rBV	489	322	0.01%	0.002%
35	6.129	1503	1505	1508	rBV2	537	320	0.01%	0.002%
36	6.168	1515	1517	1518	rBV2	299	94	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055727.D
 Acq On : 10 Oct 2023 17:36
 Operator : MD/SY
 Sample : 04747-05ME
 Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EX840ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.242	1526	1540	1569	rBV	587528	1260536	54.52%	7.041%
38	6.528	1617	1629	1642	rBV9	18014	42110	1.82%	0.235%
39	6.685	1665	1678	1703	rBV	487119	1036267	44.82%	5.788%
40	6.881	1738	1739	1740	rBV	243	71	0.00%	0.000%
41	6.936	1752	1756	1757	rBV	440	270	0.01%	0.002%
42	7.004	1775	1777	1781	rVB2	387	243	0.01%	0.001%
43	7.023	1781	1783	1784	rBV	308	130	0.01%	0.001%
44	7.090	1800	1804	1808	rBV2	762	482	0.02%	0.003%
45	7.168	1826	1828	1829	rBV	403	190	0.01%	0.001%
46	7.193	1829	1836	1839	rBV4	2457	3297	0.14%	0.018%
47	7.351	1883	1885	1888	rBV3	528	225	0.01%	0.001%
48	7.444	1910	1914	1916	rBV2	449	347	0.02%	0.002%
49	7.563	1938	1951	1981	rBV	252468	529840	22.92%	2.959%
50	7.894	2040	2054	2079	rBV	973055	1852651	80.13%	10.348%
51	8.180	2130	2143	2170	rBV	153365	362843	15.69%	2.027%
52	8.396	2208	2210	2213	rBV	579	308	0.01%	0.002%
53	8.409	2213	2214	2215	rBV	312	99	0.00%	0.001%
54	8.438	2221	2223	2225	rBV	307	135	0.01%	0.001%
55	8.460	2226	2230	2231	rBV2	491	374	0.02%	0.002%
56	8.550	2243	2258	2274	rBV	275408	480318	20.77%	2.683%
57	8.663	2275	2293	2322	rVV2	537940	1380272	59.70%	7.710%
58	9.129	2435	2438	2440	rBV2	567	369	0.02%	0.002%
59	9.206	2459	2462	2463	rBV2	440	238	0.01%	0.001%
60	9.306	2489	2493	2495	rBV2	665	435	0.02%	0.002%
61	9.418	2514	2528	2554	rBV	732585	1610069	69.64%	8.993%
62	9.682	2606	2610	2611	rBV2	586	385	0.02%	0.002%
63	9.859	2663	2665	2666	rBV	321	112	0.00%	0.001%
64	9.920	2681	2684	2686	rBV	364	222	0.01%	0.001%
65	9.952	2691	2694	2701	rVB2	519	604	0.03%	0.003%
66	10.167	2758	2761	2764	rBV2	624	389	0.02%	0.002%
67	10.290	2796	2799	2801	rBV	269	172	0.01%	0.001%
68	10.518	2868	2870	2874	rVB	506	238	0.01%	0.001%
69	10.540	2874	2877	2878	rBV	388	230	0.01%	0.001%
70	10.650	2908	2911	2913	rBV	400	184	0.01%	0.001%
71	10.663	2913	2915	2917	rBV2	308	122	0.01%	0.001%
72	10.762	2932	2946	2966	rBV	782123	1302387	56.33%	7.275%
73	10.936	2997	3000	3004	rVB2	786	554	0.02%	0.003%
74	11.232	3090	3092	3093	rBV	316	163	0.01%	0.001%
75	11.415	3143	3149	3158	rVB5	2027	2652	0.11%	0.015%
76	11.466	3163	3165	3167	rBV3	935	521	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
 Data File : VU055727.D
 Acq On : 10 Oct 2023 17:36
 Operator : MD/SY
 Sample : 04747-05ME
 Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EX840ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

77	11.624	3212	3214	3215	rBV3	401	132	0.01%	0.001%
78	11.656	3218	3224	3231	rVB3	714	852	0.04%	0.005%
79	11.692	3231	3235	3237	rBV2	630	453	0.02%	0.003%
80	11.743	3248	3251	3253	rBV	677	526	0.02%	0.003%
81	11.814	3261	3273	3293	rBV	893233	1436737	62.14%	8.025%
82	12.058	3346	3349	3353	rBV4	722	627	0.03%	0.004%
83	12.081	3353	3356	3358	rBV	469	278	0.01%	0.002%
84	12.193	3379	3391	3418	rBV	926658	1544699	66.81%	8.628%
85	12.762	3564	3568	3574	rBV4	1271	1116	0.05%	0.006%
86	13.515	3797	3802	3808	rBV4	919	1057	0.05%	0.006%




Sum of corrected areas: 17903384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055727.D
Acq On : 10 Oct 2023 17:36
Operator : MD/SY
Sample : 04747-05ME
Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EX840ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

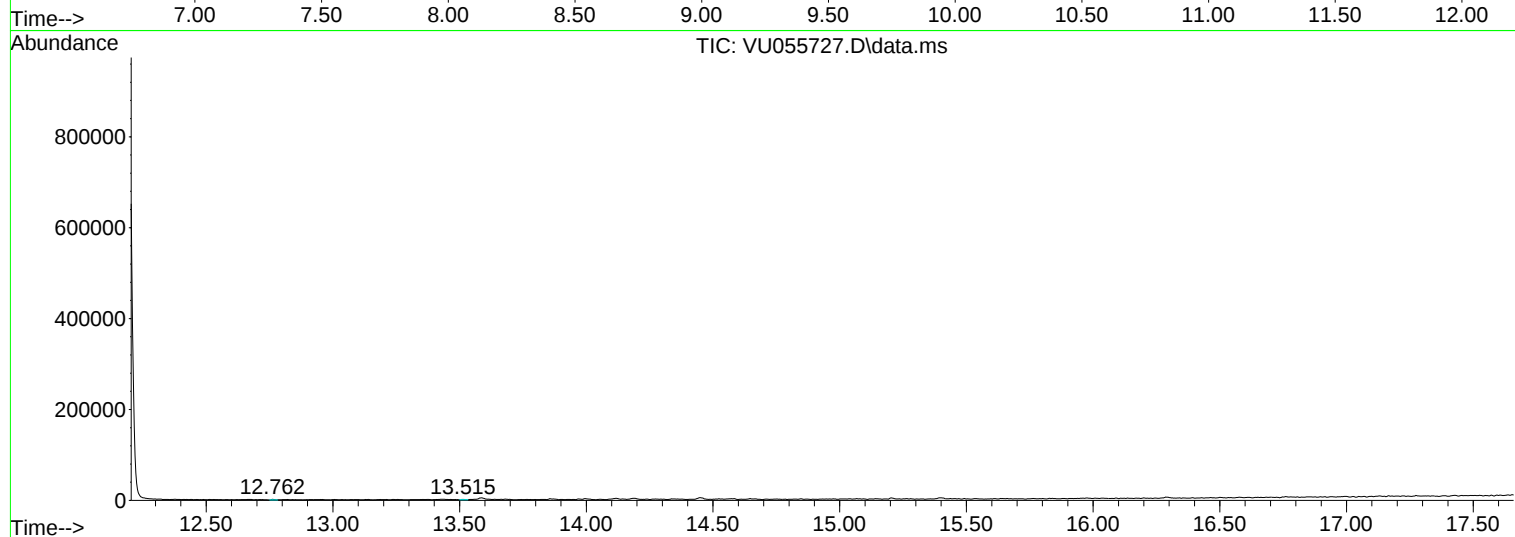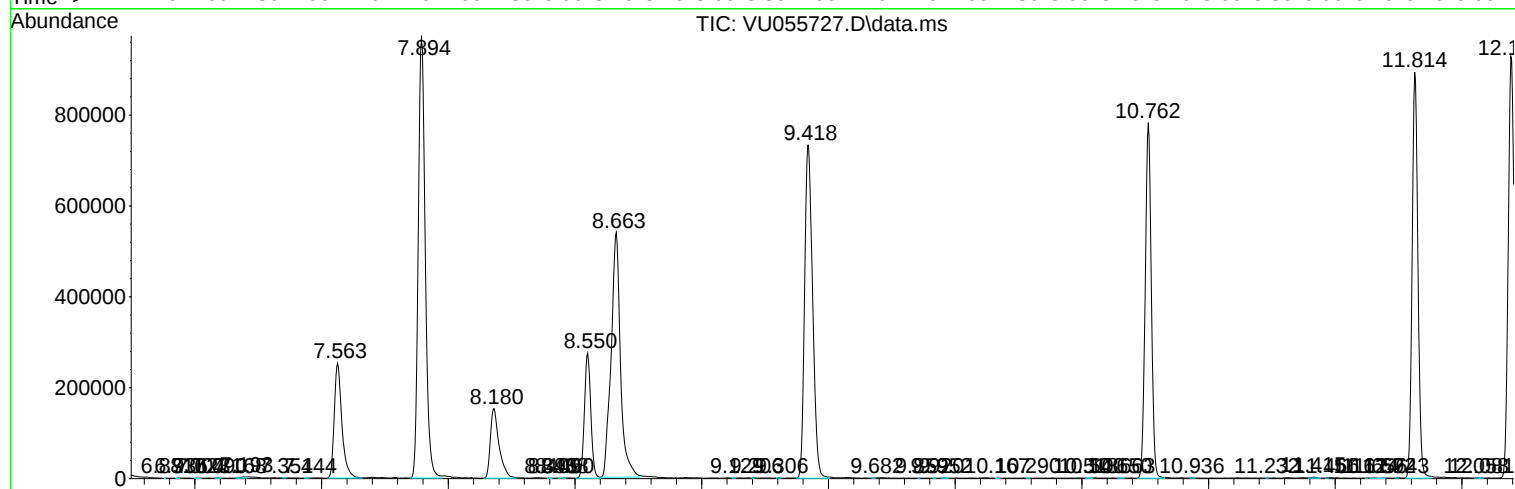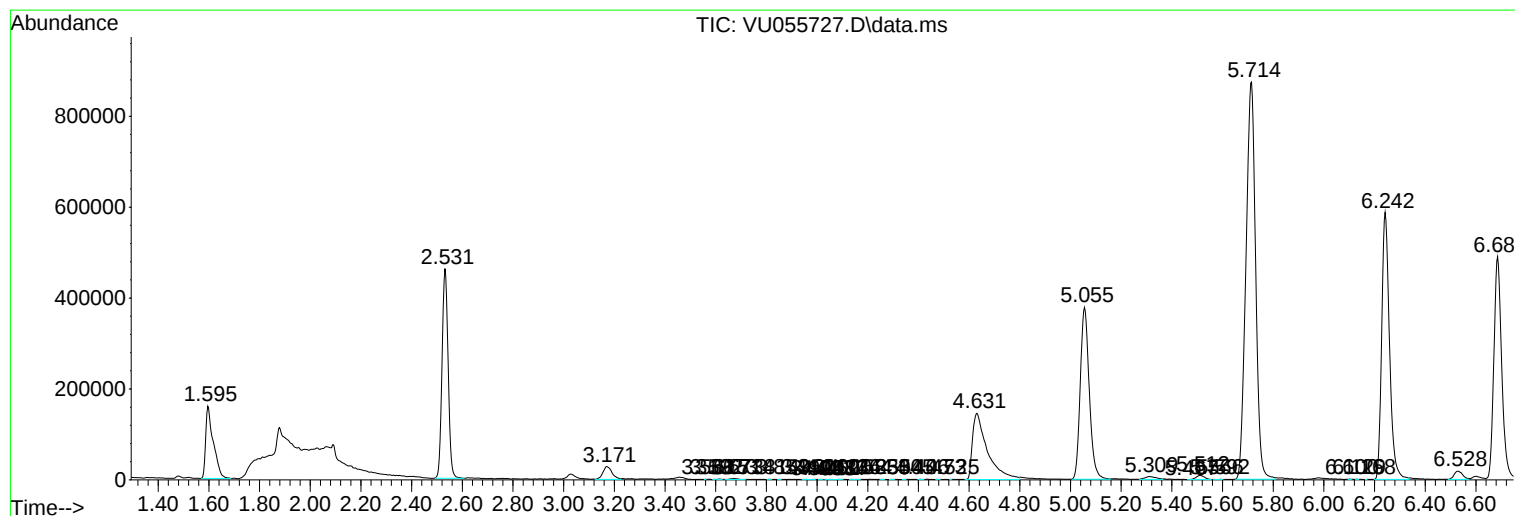

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055727.D
Acq On : 10 Oct 2023 17:36
Operator : MD/SY
Sample : 04747-05ME
Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EX840ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055727.D
Acq On : 10 Oct 2023 17:36
Operator : MD/SY
Sample : 04747-05ME
Misc : 4.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EX840ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------