


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101023\
Data File : VU055709.D
Acq On : 10 Oct 2023 09:22
Operator : MD/SY
Sample : BFB020
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Wed Oct 11 05:51:51 2023

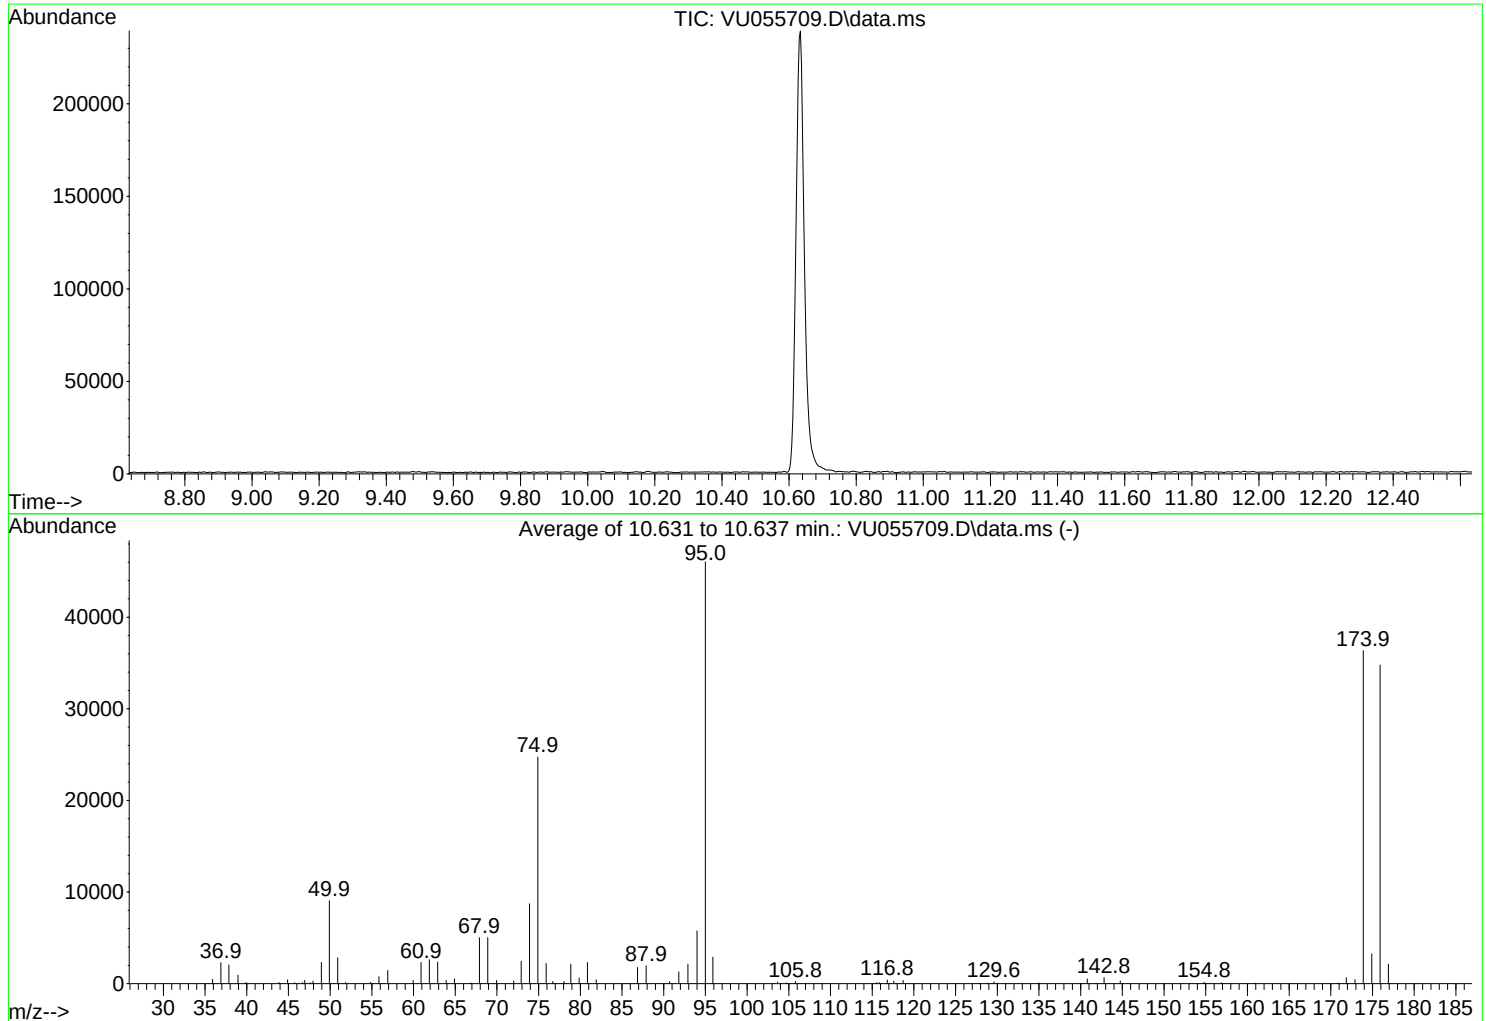

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	9049	PASS
75	95	30	80	53.7	24741	PASS
95	95	100	100	100.0	46040	PASS
96	95	5	9	6.3	2892	PASS
173	174	0.00	2	1.2	437	PASS
174	95	50	120	78.9	36344	PASS
175	174	5	9	8.9	3251	PASS
176	174	95	101	95.7	34773	PASS
177	176	5	9	6.1	2134	PASS

m/z	Abundance
39.90	406.0
43.90	538.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	445.0
36.90	2451.0
37.80	1941.0
39.00	935.0
39.90	582.0
43.80	698.0
44.90	295.0
45.80	138.0
46.70	321.0
47.10	294.0
48.00	234.0
48.90	2521.0
49.90	9479.0
50.90	3051.0
51.90	109.0
54.80	138.0
55.80	805.0
56.90	1575.0
60.00	433.0
60.90	2226.0
61.90	2500.0
62.90	2276.0
64.00	349.0
64.90	407.0
66.80	104.0
67.90	5191.0
68.90	5125.0
70.00	388.0
72.00	273.0
72.90	2393.0
73.90	8935.0
74.90	24640.0
75.90	2234.0
76.70	324.0
78.10	238.0
78.90	2027.0
79.80	726.0
80.90	2205.0
81.90	409.0
85.70	126.0
86.90	1915.0
87.90	2013.0
90.70	275.0
91.80	1330.0
92.90	2317.0
94.00	6127.0
95.00	46648.0
95.90	3025.0
97.00	132.0
103.60	178.0
105.80	274.0
115.90	190.0
116.80	381.0
117.60	269.0
118.70	323.0
127.80	102.0
128.80	113.0
129.60	211.0
135.00	101.0
140.80	565.0
142.80	737.0
144.70	309.0
154.70	180.0
156.90	126.0
171.80	705.0
172.90	340.0
173.90	36384.0
174.90	3536.0
175.90	35232.0
176.90	2192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	509.0
36.90	2387.0
37.90	2094.0
38.90	929.0
39.90	554.0
43.90	639.0
44.90	458.0
45.70	113.0
46.90	367.0
47.60	289.0
48.00	293.0
48.90	2413.0
49.90	9459.0
50.90	2946.0
51.80	127.0
54.90	152.0
55.90	792.0
56.90	1470.0
60.00	378.0
60.90	2425.0
61.90	2713.0
62.90	2423.0
63.90	338.0
64.90	517.0
66.90	103.0
67.90	5173.0
68.90	5281.0
69.90	355.0
72.00	275.0
72.90	2592.0
73.90	9070.0
74.90	25496.0
75.90	2251.0
76.70	247.0
78.00	267.0
78.80	2193.0
79.90	650.0
80.90	2355.0
81.90	440.0
86.90	1731.0
87.90	1993.0
90.70	209.0
91.80	1308.0
92.90	2185.0
94.00	5906.0
95.00	47352.0
95.90	2996.0
103.60	180.0
104.70	109.0
105.80	233.0
115.50	153.0
115.80	141.0
116.80	406.0
117.60	297.0
118.70	377.0
129.60	200.0
135.00	107.0
140.80	518.0
141.80	113.0
142.80	659.0
144.70	298.0
154.80	153.0
156.90	121.0
170.90	120.0
171.90	667.0
172.90	441.0
173.90	37440.0
174.90	3316.0
175.90	35888.0
176.90	2164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	469.0
36.90	2023.0
37.90	2110.0
38.90	889.0
39.90	515.0
43.90	669.0
44.90	531.0
46.90	452.0
47.90	292.0
49.00	2045.0
49.90	8208.0
50.90	2460.0
51.90	149.0
54.90	133.0
55.90	698.0
56.90	1308.0
59.90	286.0
60.90	2294.0
61.90	2667.0
62.90	2372.0
63.80	356.0
64.90	629.0
67.90	4697.0
68.90	4637.0
69.90	301.0
72.00	321.0
72.90	2362.0
73.90	8131.0
74.90	24088.0
75.90	2177.0
76.80	167.0
78.00	232.0
78.80	2151.0
79.80	482.0
80.80	2338.0
81.90	414.0
86.80	1653.0
87.90	1807.0
90.70	150.0
91.80	1185.0
92.90	1899.0
94.00	5260.0
95.00	44120.0
95.90	2656.0
103.70	154.0
104.70	131.0
105.80	171.0
115.60	204.0
116.80	445.0
117.60	261.0
118.70	371.0
129.60	154.0
140.80	445.0
142.80	568.0
144.80	268.0
154.90	117.0
160.90	137.0
170.80	104.0
171.90	552.0
172.90	531.0
173.90	35208.0
174.90	2901.0
175.90	33200.0
176.90	2046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020