
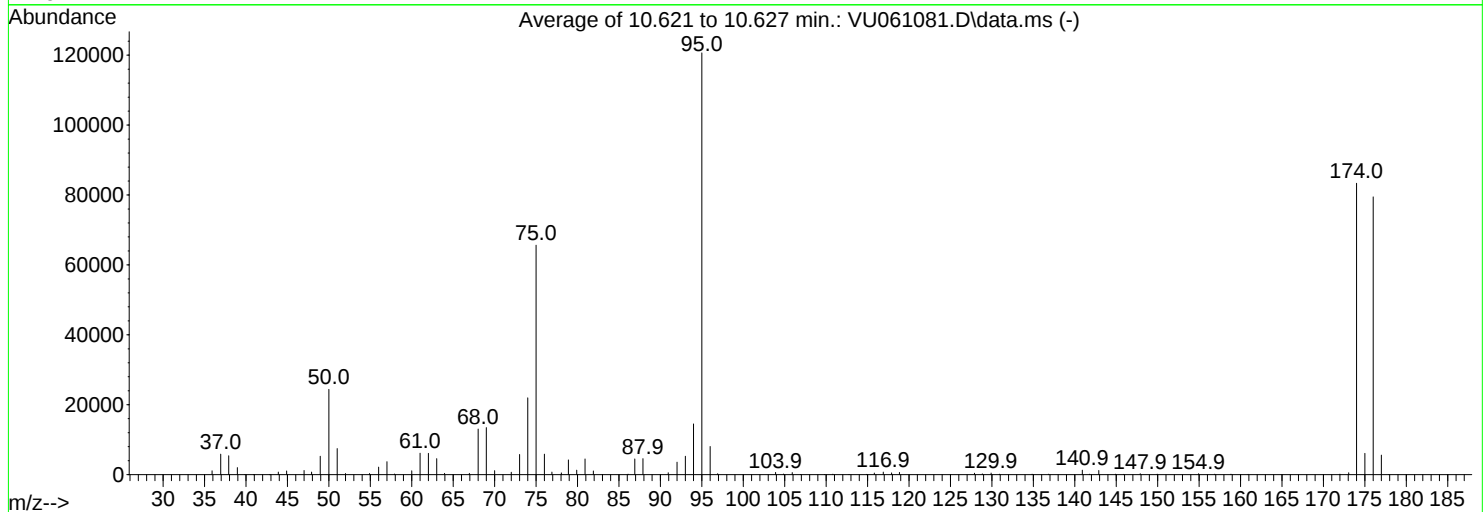


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101024\
Data File : VU061081.D
Acq On : 10 Oct 2024 09:18
Operator : MD/SY
Sample : BFB010
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB010

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 11 06:46:55 2024

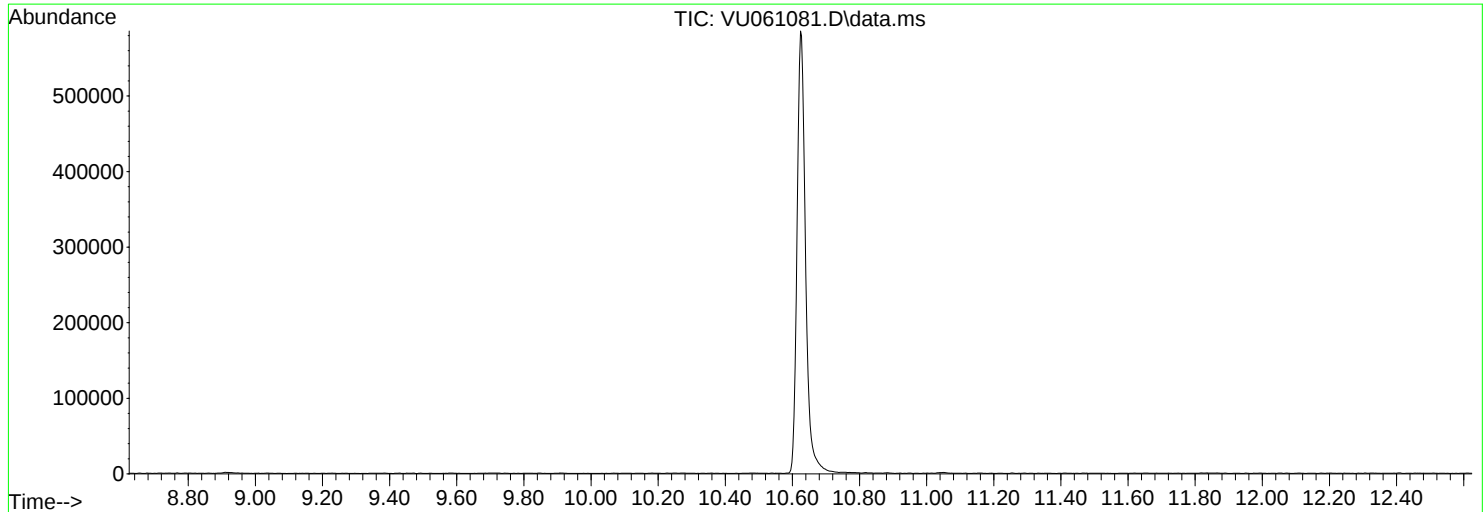

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	24405	PASS
75	95	30	80	54.4	65632	PASS
95	95	100	100	100.0	120667	PASS
96	95	5	9	6.7	8067	PASS
173	174	0.00	2	0.7	571	PASS
174	95	50	120	69.1	83341	PASS
175	174	5	9	7.3	6110	PASS
176	174	95	101	95.4	79475	PASS
177	176	5	9	7.0	5586	PASS

m/z	Abundance
39.80	182.0
41.00	125.0
42.80	118.0
43.90	515.0
54.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	1107.0
36.90	5723.0
37.90	5247.0
38.90	1975.0
39.90	261.0
40.90	117.0
42.90	145.0
44.00	1253.0
44.90	1025.0
47.10	1167.0
47.90	708.0
48.90	5184.0
50.00	23632.0
51.00	7273.0
52.00	312.0
55.00	457.0
56.00	2144.0
57.00	3650.0
57.90	187.0
60.00	1032.0
61.00	6104.0
62.00	5990.0
63.00	4358.0
64.00	382.0
66.90	322.0
68.00	12620.0
69.00	13047.0
70.00	1061.0
72.00	614.0
73.00	5549.0
74.00	21056.0
75.00	62400.0
76.00	5708.0
76.90	679.0
78.00	479.0
78.90	3983.0
79.90	1260.0
80.90	4333.0
81.90	1023.0
83.00	119.0
86.10	117.0
86.90	4368.0
87.90	4422.0
91.00	523.0
92.00	3482.0
93.00	5011.0
94.00	13692.0
95.00	115168.0
96.00	7872.0
96.90	252.0
103.90	630.0
104.90	144.0
105.90	599.0
106.90	107.0
110.80	106.0
115.80	461.0
116.90	731.0
117.90	459.0
118.90	611.0
127.90	424.0
128.80	259.0
129.90	451.0
130.90	106.0
134.90	134.0
136.80	141.0
140.90	1178.0
141.80	118.0
142.90	1120.0
144.90	137.0
147.90	257.0
150.00	176.0
154.90	257.0
156.90	130.0
158.80	135.0
172.00	153.0
173.00	498.0
174.00	77608.0
175.00	5693.0
176.00	73152.0
177.00	5316.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	1102.0
37.00	6045.0
37.90	5574.0
39.00	2073.0
39.90	257.0
40.90	160.0
42.90	131.0
44.00	1263.0
44.90	1100.0
47.00	1220.0
47.90	768.0
49.00	5418.0
50.00	25144.0
51.00	7675.0
52.00	341.0
54.90	436.0
56.00	2218.0
57.00	3823.0
57.90	171.0
60.00	1133.0
61.00	6305.0
62.00	6279.0
63.00	4703.0
64.00	361.0
66.90	366.0
68.00	13488.0
69.00	13947.0
70.00	1192.0
72.00	707.0
73.00	5906.0
74.00	22672.0
75.00	67784.0
76.00	6047.0
76.90	789.0
78.10	514.0
78.90	4336.0
79.90	1338.0
80.90	4648.0
81.90	1105.0
86.10	156.0
86.90	4591.0
87.90	4664.0
90.90	552.0
92.00	3675.0
93.00	5412.0
94.00	14975.0
95.00	124120.0
96.00	8296.0
96.90	279.0
103.90	678.0
104.80	159.0
105.90	650.0
106.90	101.0
109.80	113.0
110.80	123.0
112.70	112.0
114.90	107.0
115.80	473.0
116.90	758.0
117.90	512.0
118.80	668.0
127.90	417.0
128.80	253.0
129.90	474.0
130.90	122.0
134.80	153.0
136.80	159.0
140.90	1356.0
141.80	123.0
142.90	1215.0
144.90	138.0
145.90	119.0
147.90	287.0
150.00	175.0
154.90	282.0
156.90	141.0
158.80	144.0
160.90	119.0
172.00	163.0
173.10	585.0
174.00	85992.0
175.00	6303.0
176.00	81744.0
177.00	5830.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
35.90	1048.0
36.90	5878.0
37.90	5318.0
39.00	2018.0
39.90	214.0
40.90	173.0
42.90	131.0
43.90	1255.0
44.90	1091.0
46.90	1219.0
47.90	715.0
49.00	5153.0
50.00	24440.0
51.00	7402.0
52.00	337.0
54.90	418.0
56.00	2103.0
57.00	3662.0
57.90	149.0
60.00	1161.0
61.00	5995.0
62.00	6037.0
63.00	4715.0
63.90	333.0
67.00	375.0
68.00	12997.0
69.00	13438.0
70.00	1235.0
72.00	701.0
73.00	5813.0
74.00	22176.0
75.00	66712.0
76.00	5826.0
76.90	746.0
78.00	486.0
78.90	4300.0
79.90	1264.0
80.90	4492.0
81.90	1059.0
86.10	123.0
86.90	4456.0
87.90	4583.0
90.90	519.0
92.00	3542.0
93.00	5351.0
94.00	14833.0
95.00	122712.0
96.00	8033.0
96.90	254.0
103.90	617.0
104.80	192.0
105.90	581.0
110.80	142.0
112.80	101.0
114.90	115.0
115.80	458.0
116.90	734.0
117.90	523.0
118.90	646.0
127.90	360.0
128.90	222.0
129.90	478.0
130.90	131.0
134.80	181.0
136.90	178.0
140.90	1366.0
141.80	122.0
142.90	1188.0
144.90	116.0
145.90	166.0
147.90	280.0
149.80	126.0
155.00	282.0
156.90	152.0
158.90	128.0
160.90	138.0
172.00	138.0
173.10	629.0
174.00	86424.0
175.00	6334.0
176.00	83528.0
177.00	5611.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010