


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101118\
 Data File : VU027581.D
 Acq On : 11 Oct 2018 07:45
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U101118W.M
 Title : SW846 8260
 Last Update : Fri Oct 12 09:38:49 2018

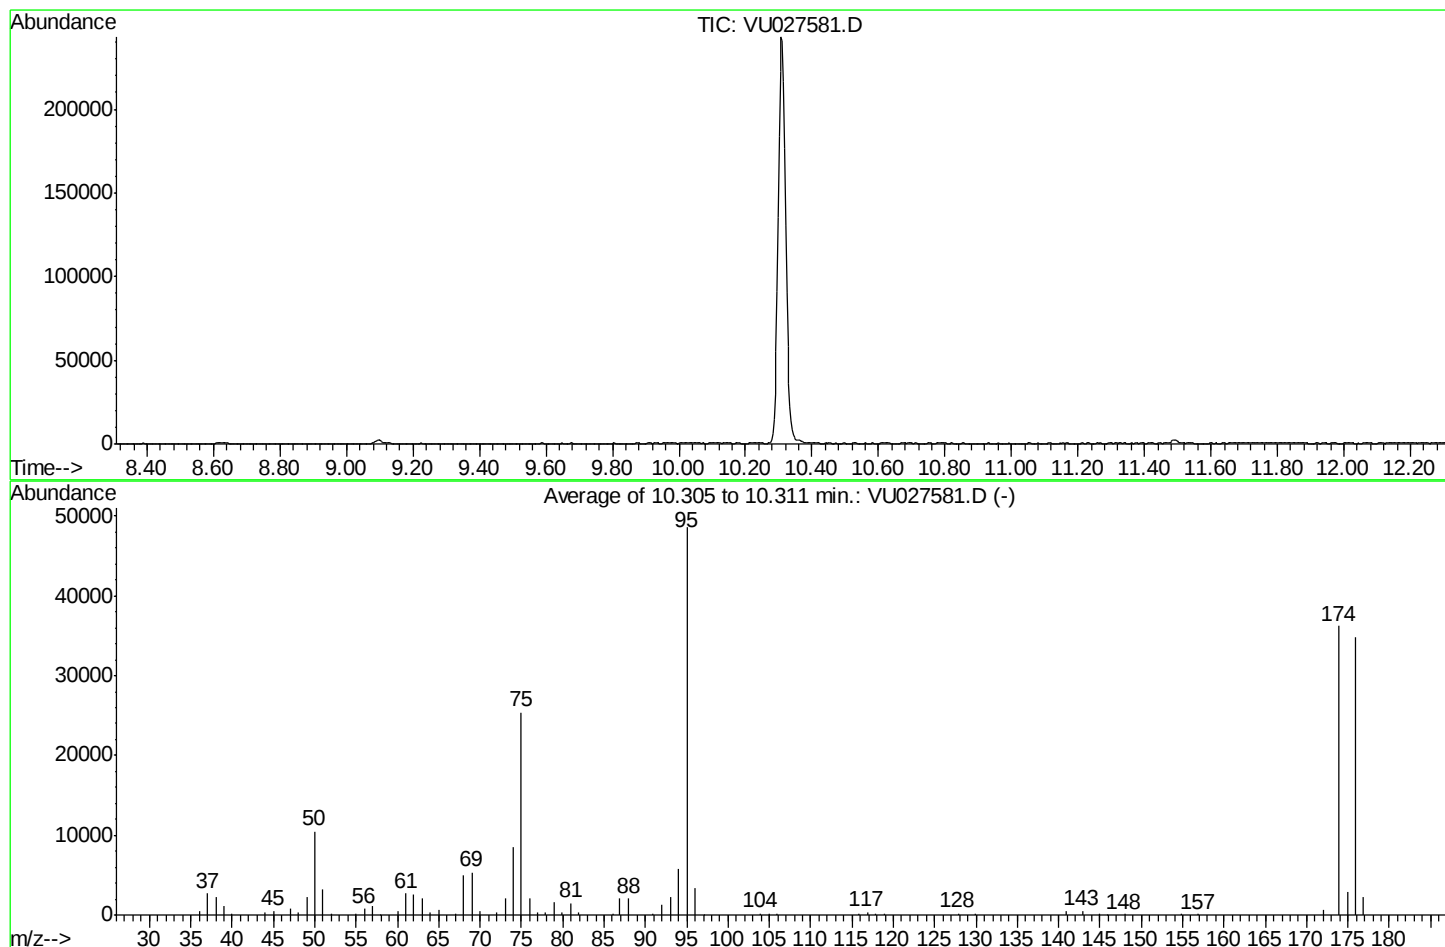

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	10470	PASS
75	95	30	60	52.2	25397	PASS
95	95	100	100	100.0	48608	PASS
96	95	5	9	7.0	3379	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.5	36213	PASS
175	174	5	9	7.8	2829	PASS
176	174	95	101	96.0	34781	PASS
177	176	5	9	6.6	2280	PASS