

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101119\
 Data File : VU035048.D
 Acq On : 10 Oct 2019 15:09
 Operator : JC/SP
 Sample : K5268-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBAW8

Quant Time: Oct 11 04:29:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 11 02:39:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	150228	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	154176	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	61886	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	35745	4.03	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.60%
7) Chloroethane-d5	1.67	69	36264	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.26	63	53576	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	4.18	46	151481	57.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.84%
24) Chloroform-d	4.62	84	79268	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.29	65	49608	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.32	84	163755	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.31	67	60732	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.55	98	138602	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
43) trans-1,3-Dichloropropene-	7.84	79	19070	4.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.80%
46) 2-Hexanone-d5	8.30	63	107084	51.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.52%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	55165	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.40%
64) 1,2-Dichlorobenzene-d4	11.84	152	55231	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	10002	4.670 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101119\
Data File : VU035048.D
Acq On : 10 Oct 2019 15:09
Operator : JC/SP
Sample : K5268-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBAW8

Quant Time: Oct 11 04:29:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 11 02:39:08 2019
Response via : Initial Calibration

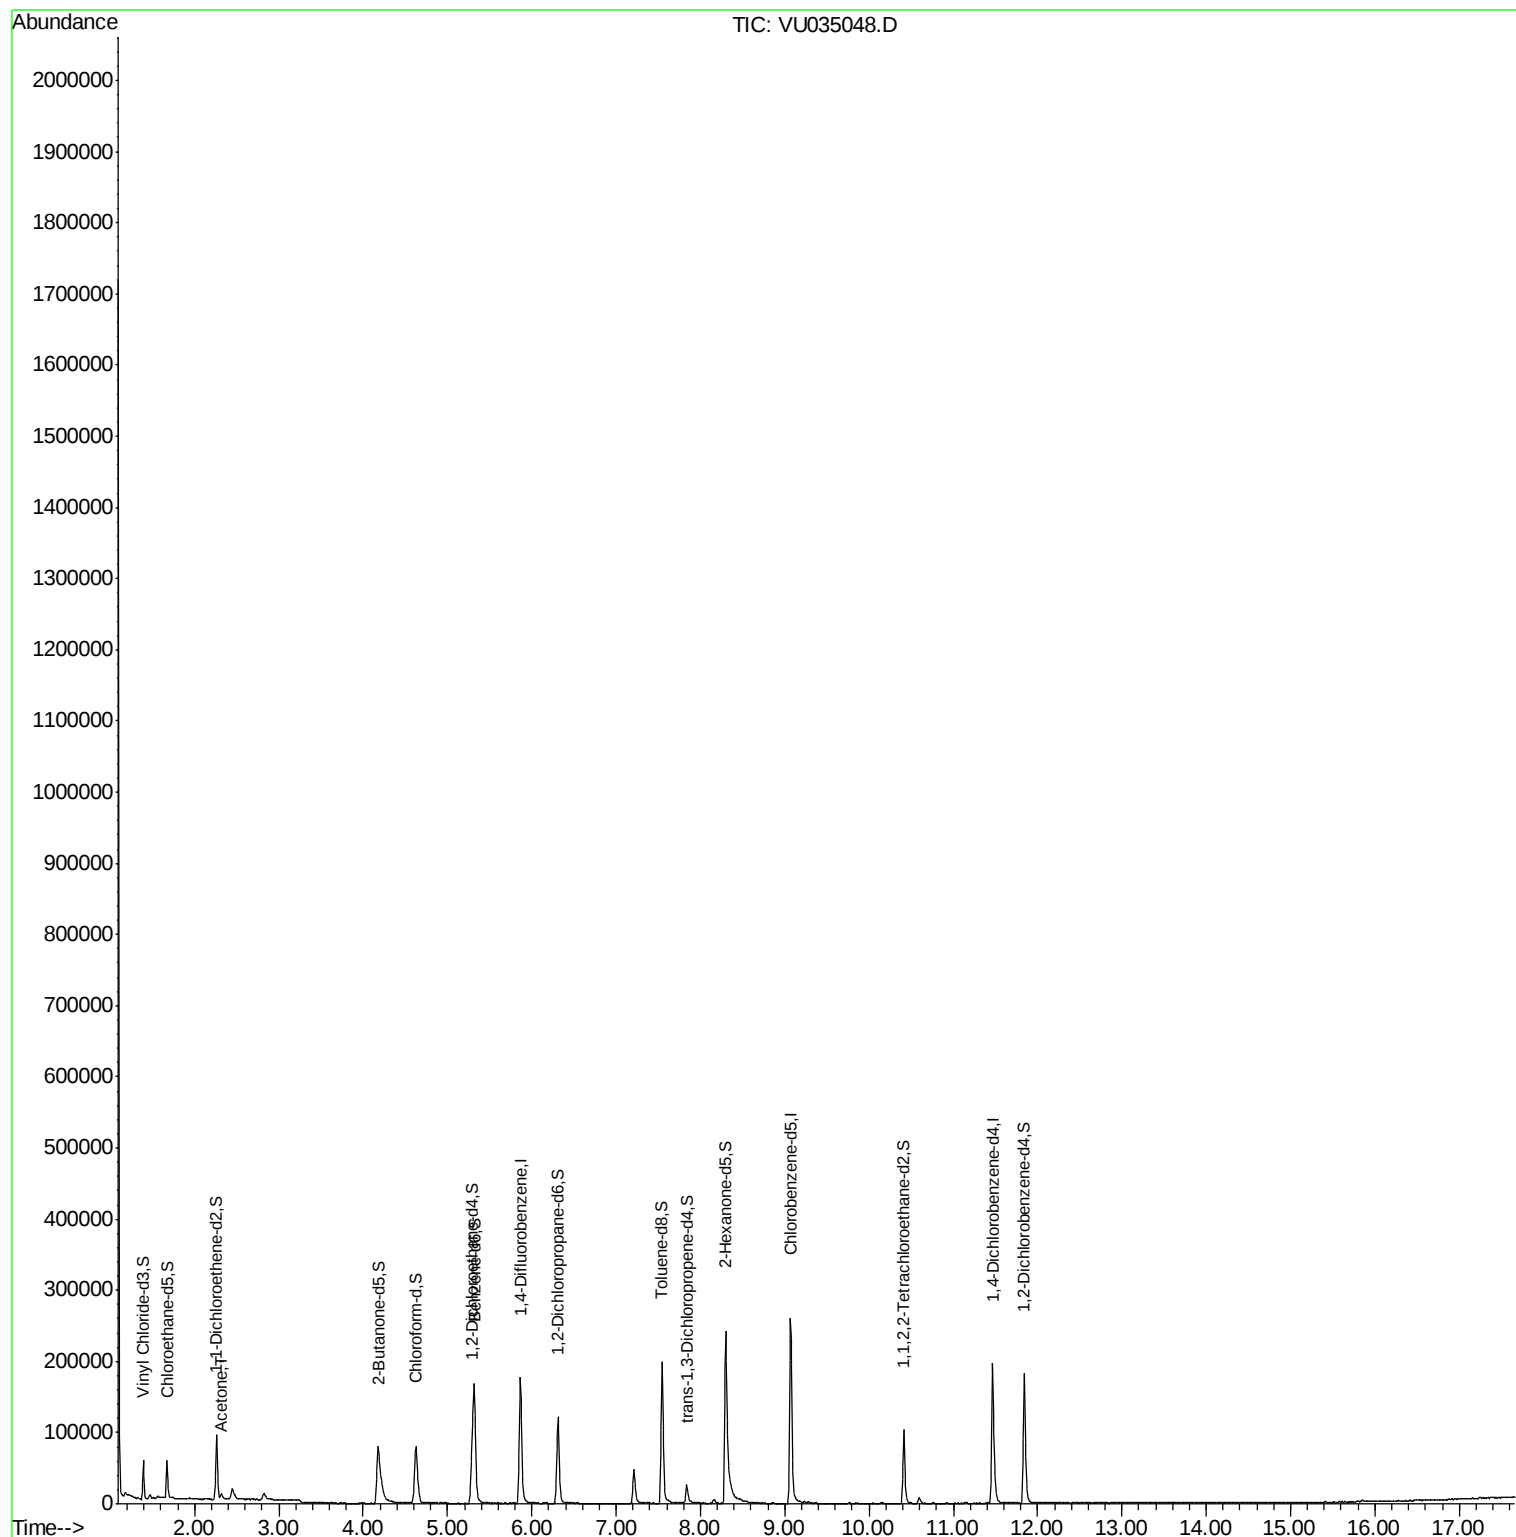

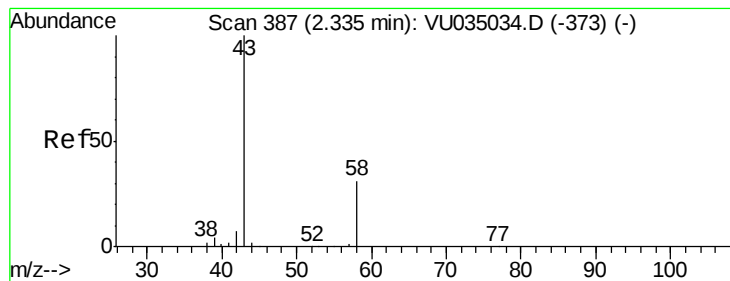

#13

Acetone

Concen: 4.670 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.01 min

Lab File: VU035048.D

Acq: 10 Oct 2019 15:09

Instrument :
MSVOA_U
ClientSampleId :
DBAW8

Tot Ion: 43 Resp: 10002

Ion Ratio Lower Upper

43 100

58 30.4 0.0 66.6

