

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
 Data File : VU045278.D
 Acq On : 11 Oct 2021 13:09
 Operator : SY/MD
 Sample : VU1011WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	34	41	53	rBV	9714	18473	1.35%	0.184%
2	1.600	74	81	103	rVB	191562	209818	15.35%	2.086%
3	1.890	163	171	185	rVB	139588	187224	13.70%	1.861%
4	2.562	367	380	399	rBV	268988	455091	33.30%	4.524%
5	2.690	418	420	424	rVB	325	227	0.02%	0.002%
6	2.790	443	451	458	rVB2	930	1613	0.12%	0.016%
7	2.967	496	506	510	rBV3	627	1141	0.08%	0.011%
8	3.044	521	530	543	rBV4	3181	6299	0.46%	0.063%
9	3.314	611	614	617	rBV	236	181	0.01%	0.002%
10	3.694	727	732	738	rBV2	209	268	0.02%	0.003%
11	3.806	763	767	769	rBV	213	198	0.01%	0.002%
12	4.054	840	844	850	rVB2	226	191	0.01%	0.002%
13	4.083	850	853	855	rBV	200	168	0.01%	0.002%
14	4.141	868	871	875	rBV2	206	187	0.01%	0.002%
15	4.218	891	895	898	rBV2	214	156	0.01%	0.002%
16	4.269	904	911	916	rBV2	224	265	0.02%	0.003%
17	4.514	983	987	990	rVB2	191	168	0.01%	0.002%
18	4.629	1008	1023	1053	rBV	149568	353701	25.88%	3.516%
19	5.067	1139	1159	1182	rBV	233887	518949	37.97%	5.159%
20	5.214	1199	1205	1211	rVB2	382	362	0.03%	0.004%
21	5.250	1211	1216	1219	rVB2	192	193	0.01%	0.002%
22	5.285	1222	1227	1230	rBV2	523	550	0.04%	0.005%
23	5.359	1246	1250	1253	rVB2	244	168	0.01%	0.002%
24	5.430	1267	1272	1276	rVB2	148	186	0.01%	0.002%
25	5.546	1303	1308	1312	rBV2	210	265	0.02%	0.003%
26	5.587	1317	1321	1326	rBV	218	269	0.02%	0.003%
27	5.729	1342	1365	1392	rBV2	504403	1366736	100.00%	13.586%
28	5.973	1435	1441	1443	rBV3	319	368	0.03%	0.004%
29	6.005	1449	1451	1457	rVB	249	222	0.02%	0.002%
30	6.044	1457	1463	1465	rBV2	400	372	0.03%	0.004%
31	6.253	1507	1528	1549	rBV	341919	639310	46.78%	6.355%
32	6.362	1557	1562	1564	rBV	397	348	0.03%	0.003%
33	6.533	1606	1615	1624	rVB5	3896	7100	0.52%	0.071%
34	6.693	1650	1665	1687	rBV	325360	622878	45.57%	6.192%
35	6.793	1693	1696	1697	rBV	307	166	0.01%	0.002%
36	6.809	1697	1701	1708	rVB4	718	912	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
 Data File : VU045278.D
 Acq On : 11 Oct 2021 13:09
 Operator : SY/MD
 Sample : VU1011WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.047	1772	1775	1788	rVB2	662	836	0.06%	0.008%
38	7.182	1808	1817	1827	rBV6	1634	2997	0.22%	0.030%
39	7.420	1886	1891	1892	rBV	198	199	0.01%	0.002%
40	7.459	1900	1903	1905	rBV	223	172	0.01%	0.002%
41	7.568	1924	1937	1959	rBV	180644	310295	22.70%	3.085%
42	7.661	1963	1966	1970	rVV2	345	273	0.02%	0.003%
43	7.687	1970	1974	1982	rVB	881	1184	0.09%	0.012%
44	7.800	2002	2009	2015	rBV5	1229	1579	0.12%	0.016%
45	7.902	2027	2041	2056	rBV	617791	1054074	77.12%	10.478%
46	7.973	2058	2063	2081	rVB	9334	14364	1.05%	0.143%
47	8.128	2109	2111	2115	rBV2	158	152	0.01%	0.002%
48	8.182	2115	2128	2148	rBV	129618	211445	15.47%	2.102%
49	8.475	2215	2219	2225	rVB3	249	341	0.02%	0.003%
50	8.539	2236	2239	2242	rVB2	237	178	0.01%	0.002%
51	8.584	2249	2253	2257	rBV2	178	231	0.02%	0.002%
52	8.639	2257	2270	2304	rBV	443767	786913	57.58%	7.822%
53	8.851	2333	2336	2339	rVV	187	175	0.01%	0.002%
54	9.079	2404	2407	2413	rBV2	214	227	0.02%	0.002%
55	9.420	2500	2513	2535	rBV	504525	807202	59.06%	8.024%
56	9.552	2549	2554	2555	rBV	186	181	0.01%	0.002%
57	9.574	2555	2561	2569	rVB2	648	960	0.07%	0.010%
58	9.693	2591	2598	2606	rVV3	1068	1578	0.12%	0.016%
59	9.928	2666	2671	2674	rBV2	263	287	0.02%	0.003%
60	9.960	2678	2681	2690	rBV2	275	418	0.03%	0.004%
61	10.002	2690	2694	2696	rBV2	206	190	0.01%	0.002%
62	10.102	2721	2725	2728	rBV2	526	501	0.04%	0.005%
63	10.150	2738	2740	2746	rBV2	162	164	0.01%	0.002%
64	10.279	2776	2780	2783	rBV	270	269	0.02%	0.003%
65	10.455	2830	2835	2838	rBV2	221	254	0.02%	0.003%
66	10.529	2851	2858	2860	rBV	292	389	0.03%	0.004%
67	10.616	2878	2885	2889	rBV	293	387	0.03%	0.004%
68	10.677	2894	2904	2912	rVB3	3570	5754	0.42%	0.057%
69	10.761	2916	2930	2950	rBV	464771	740195	54.16%	7.358%
70	10.864	2959	2962	2963	rBV2	363	213	0.02%	0.002%
71	10.957	2987	2991	2994	rBV	232	234	0.02%	0.002%
72	11.063	3021	3024	3028	rBV	232	255	0.02%	0.003%
73	11.089	3028	3032	3035	rBV2	392	382	0.03%	0.004%
74	11.156	3050	3053	3056	rBV2	374	278	0.02%	0.003%
75	11.465	3139	3149	3158	rVB4	2911	5038	0.37%	0.050%
76	11.574	3180	3183	3184	rBV	286	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
 Data File : VU045278.D
 Acq On : 11 Oct 2021 13:09
 Operator : SY/MD
 Sample : VU1011WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.700	3215	3222	3231	rVB3	1808	2628	0.19%	0.026%
78	11.751	3231	3238	3243	rVB3	1117	1333	0.10%	0.013%
79	11.815	3243	3258	3281	rBV	474267	744235	54.45%	7.398%
80	11.928	3290	3293	3294	rBV	471	238	0.02%	0.002%
81	11.947	3294	3299	3302	rVV2	1242	1546	0.11%	0.015%
82	11.976	3304	3308	3317	rVB4	2649	3382	0.25%	0.034%
83	12.076	3333	3339	3340	rBV2	377	328	0.02%	0.003%
84	12.195	3361	3376	3399	rBV	576481	928844	67.96%	9.233%
85	12.333	3414	3419	3424	rBV4	841	873	0.06%	0.009%
86	12.394	3434	3438	3439	rBV2	336	231	0.02%	0.002%
87	12.639	3510	3514	3521	rVB3	487	589	0.04%	0.006%
88	12.822	3568	3571	3573	rBV	226	170	0.01%	0.002%
89	12.909	3595	3598	3601	rBV2	209	185	0.01%	0.002%
90	12.954	3609	3612	3614	rBV	244	185	0.01%	0.002%
91	12.999	3622	3626	3631	rVB4	508	401	0.03%	0.004%
92	13.150	3669	3673	3675	rBV2	524	438	0.03%	0.004%
93	13.227	3690	3697	3707	rVB4	1401	1927	0.14%	0.019%
94	13.716	3843	3849	3853	rBV2	281	415	0.03%	0.004%
95	13.848	3882	3890	3900	rBV5	3165	4513	0.33%	0.045%
96	14.092	3958	3966	3977	rBV2	9514	15018	1.10%	0.149%
97	14.333	4035	4041	4052	rVB2	4141	5621	0.41%	0.056%
98	14.725	4159	4163	4166	rBV2	520	473	0.03%	0.005%
99	14.838	4196	4198	4202	rBV	281	239	0.02%	0.002%
100	14.909	4217	4220	4222	rBV2	402	291	0.02%	0.003%




Sum of corrected areas: 10059779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
Data File : VU045278.D
Acq On : 11 Oct 2021 13:09
Operator : SY/MD
Sample : VU1011WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

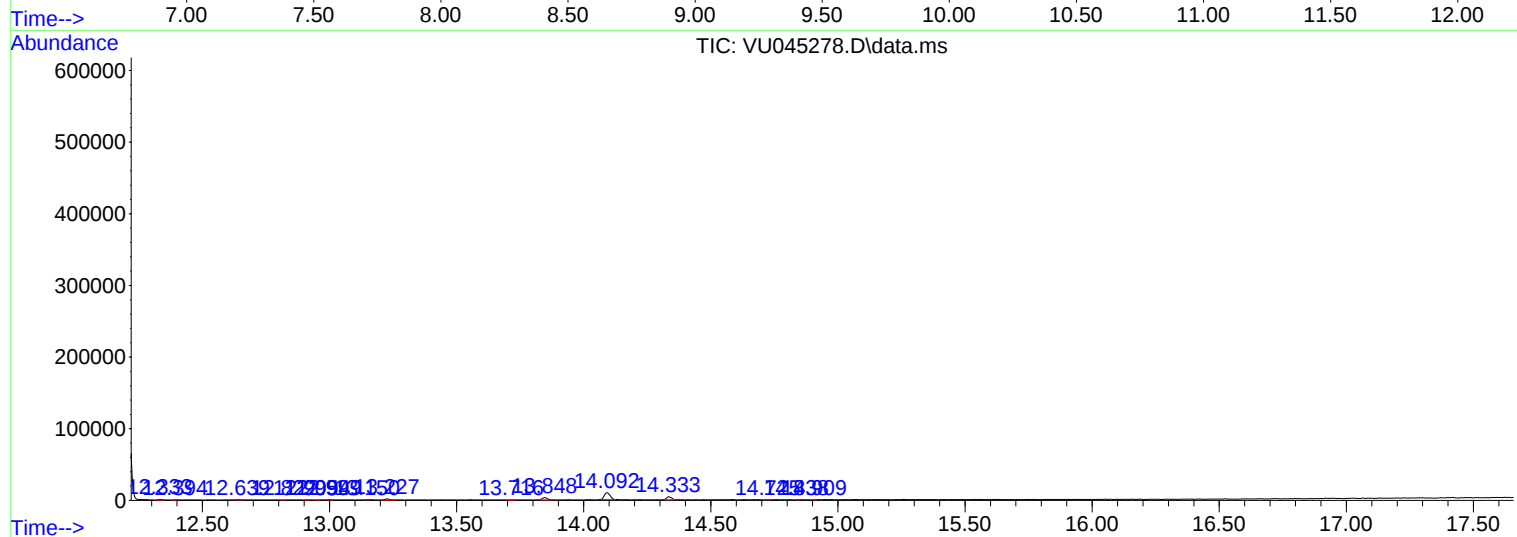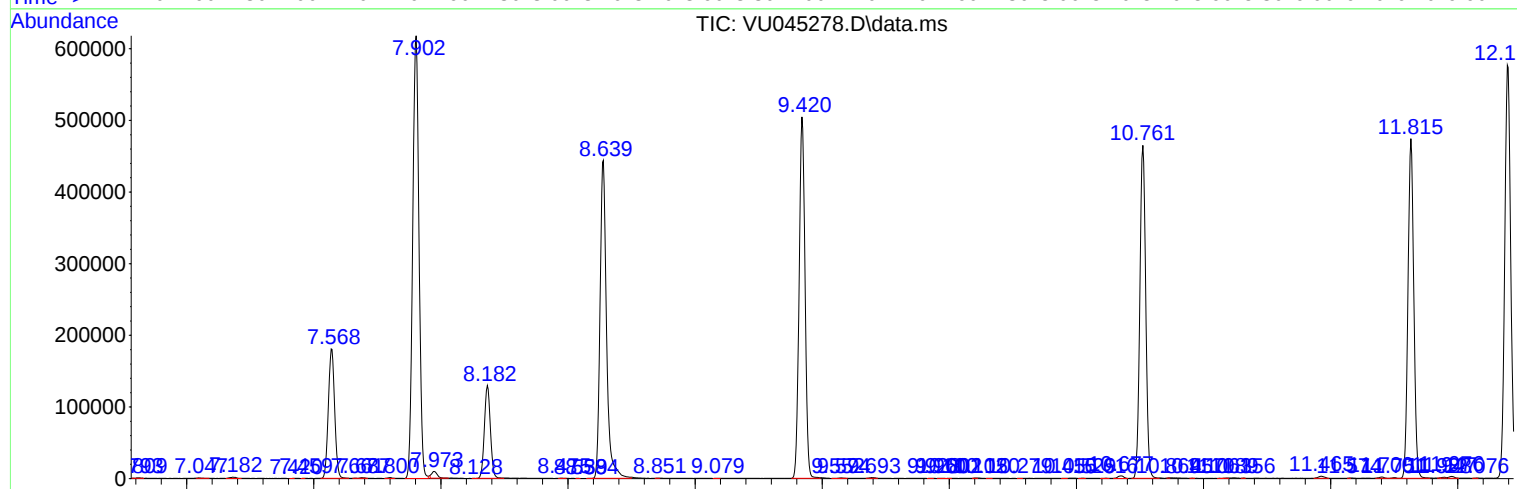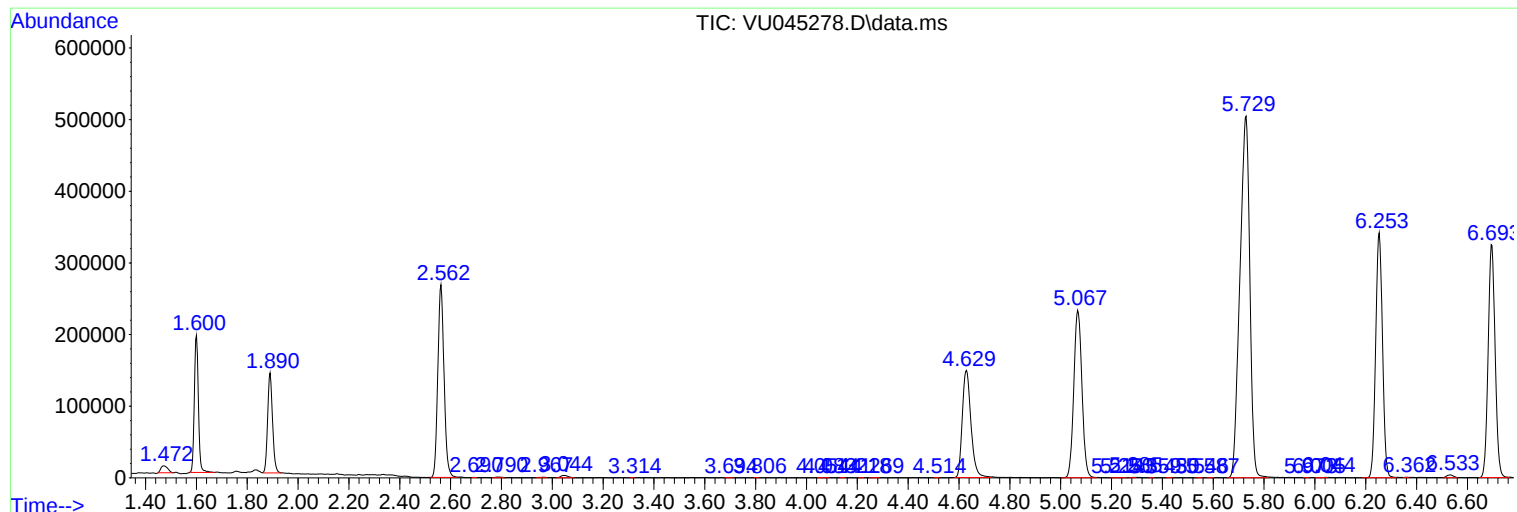

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
Data File : VU045278.D
Acq On : 11 Oct 2021 13:09
Operator : SY/MD
Sample : VU1011WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101121\
Data File : VU045278.D
Acq On : 11 Oct 2021 13:09
Operator : SY/MD
Sample : VU1011WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
